
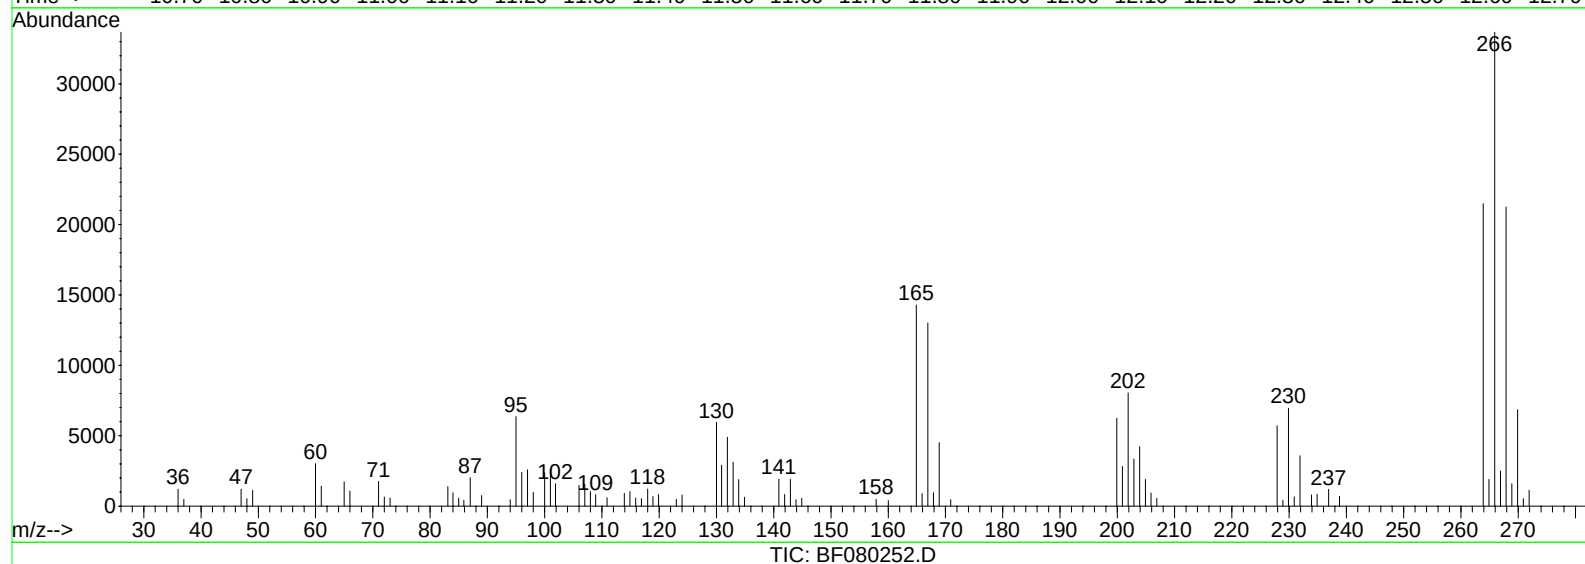


Data Path : Z:\HPCHEM1\BNA F\Data\BF063015\
Data File : BF080252.D
Acq On : 1 Jul 2015 00:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 07:14:23 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

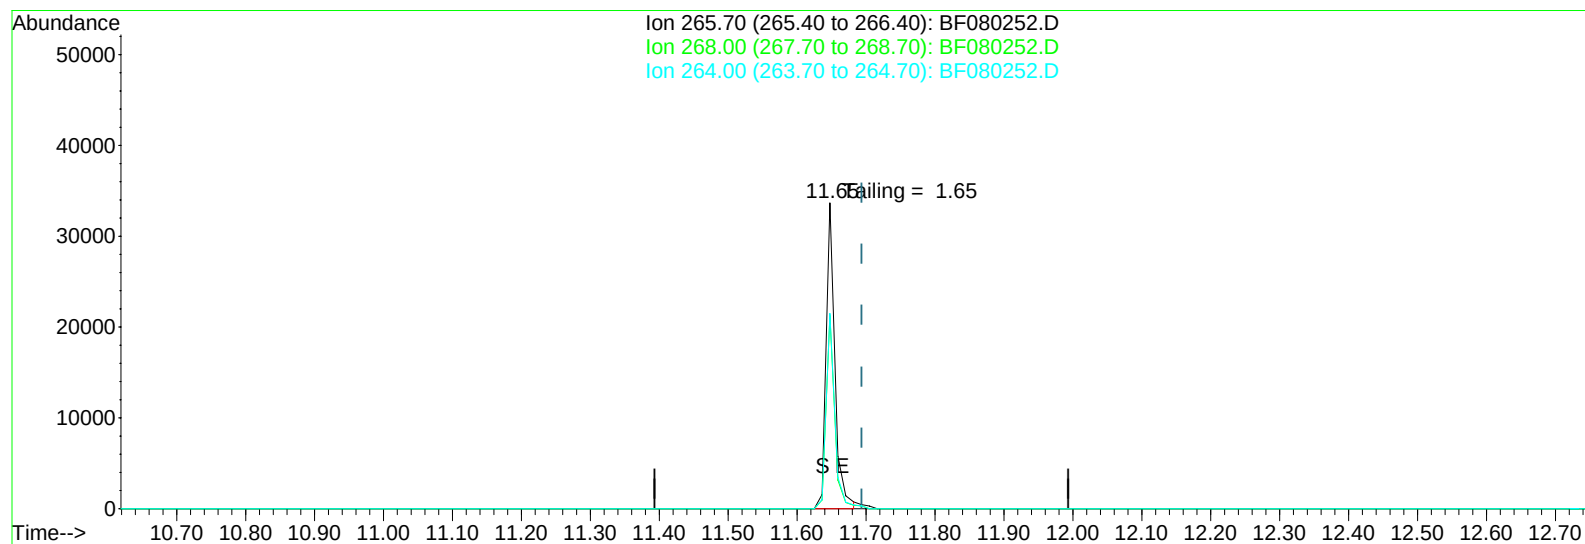

(69) Pentachlorophenol (C)



11.648min (-0.046) 0.00ng

response 30122

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.13
264.00	62.70	63.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF063015\
Data File : BF080252.D
Acq On : 1 Jul 2015 00:19
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 07:14:23 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

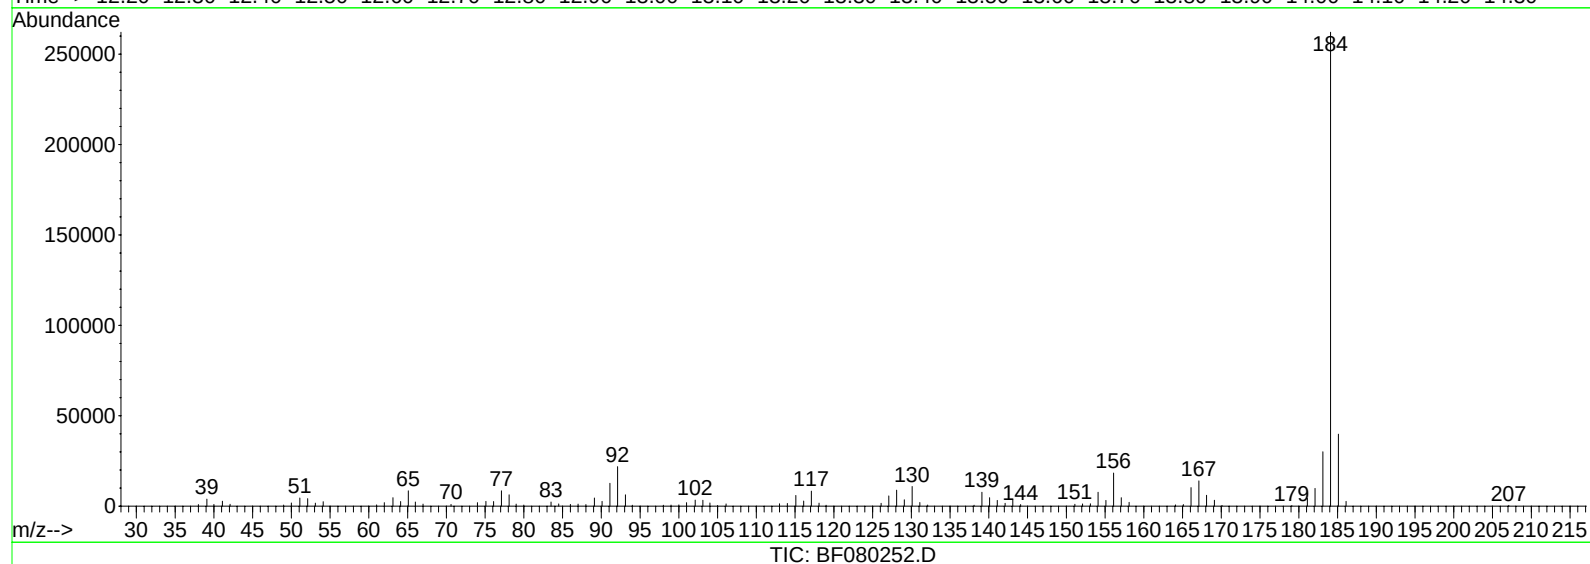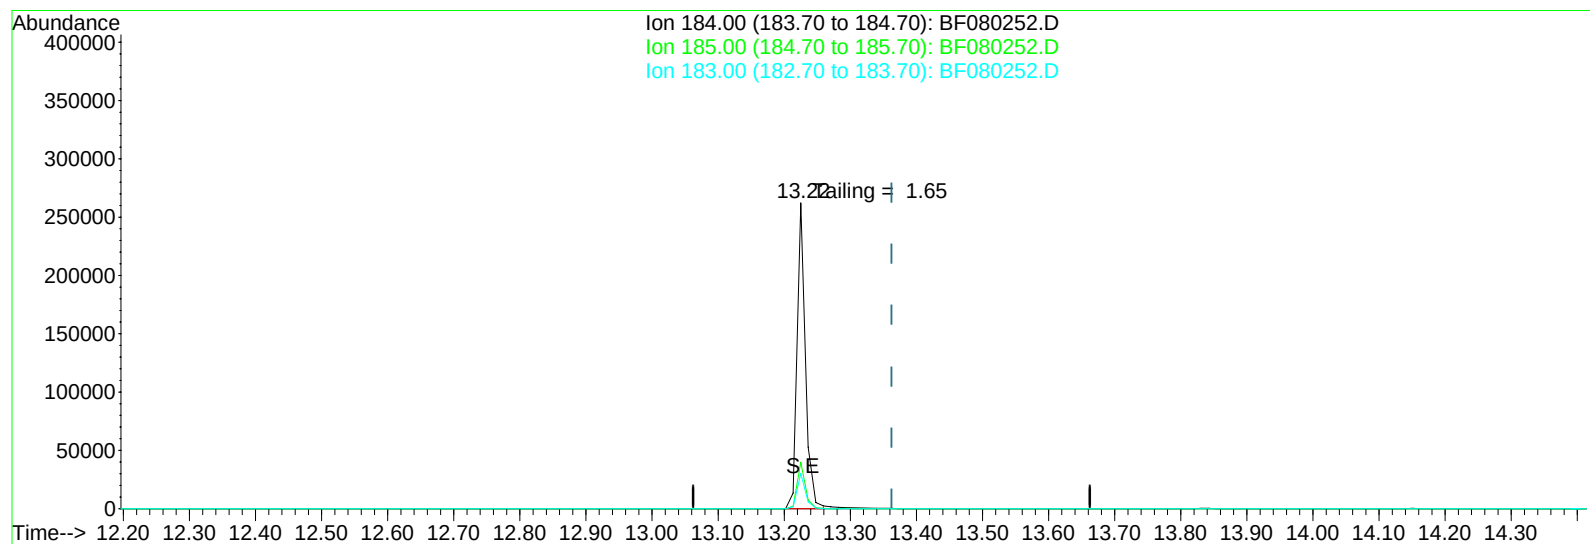

(76) Benzidine

13.225min (-0.137) 37545.74ng

response 235085

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.18
183.00	9.50	11.47#
0.00	0.00	0.00