

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
 Data File : BF080240.D
 Acq On : 30 Jun 2015 17:05
 Operator : TP/IZ
 Sample : PB84281BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB84281BL

Quant Time: Jul 01 02:59:25 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 23 00:53:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.28	152	37194	20.00	ng	-0.05
21) Naphthalene-d8	8.57	136	153535	20.00	ng	-0.05
38) Acenaphthene-d10	10.34	164	80701	20.00	ng	-0.05
63) Phenanthrene-d10	11.85	188	153823	20.00	ng	-0.06
75) Chrysene-d12	14.76	240	165239	20.00	ng	-0.24
86) Perylene-d12	16.59	264	158950	20.00	ng	-0.34
System Monitoring Compounds						
5) 2-Fluorophenol	5.90	112	248038	118.05	ng	-0.03
7) Phenol-d6	6.89	99	324798	116.16	ng	-0.03
23) Nitrobenzene-d5	7.84	82	191154	72.48	ng	-0.03
41) 2,4,6-Tribromophenol	11.14	330	78708	99.74	ng	-0.03
44) 2-Fluorobiphenyl	9.65	172	384542	67.95	ng	-0.05
78) Terphenyl-d14	13.51	244	475762	67.24	ng	-0.16


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080240.D
Acq On : 30 Jun 2015 17:05
Operator : TP/IZ
Sample : PB84281BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84281BL

Quant Time: Jul 01 02:59:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

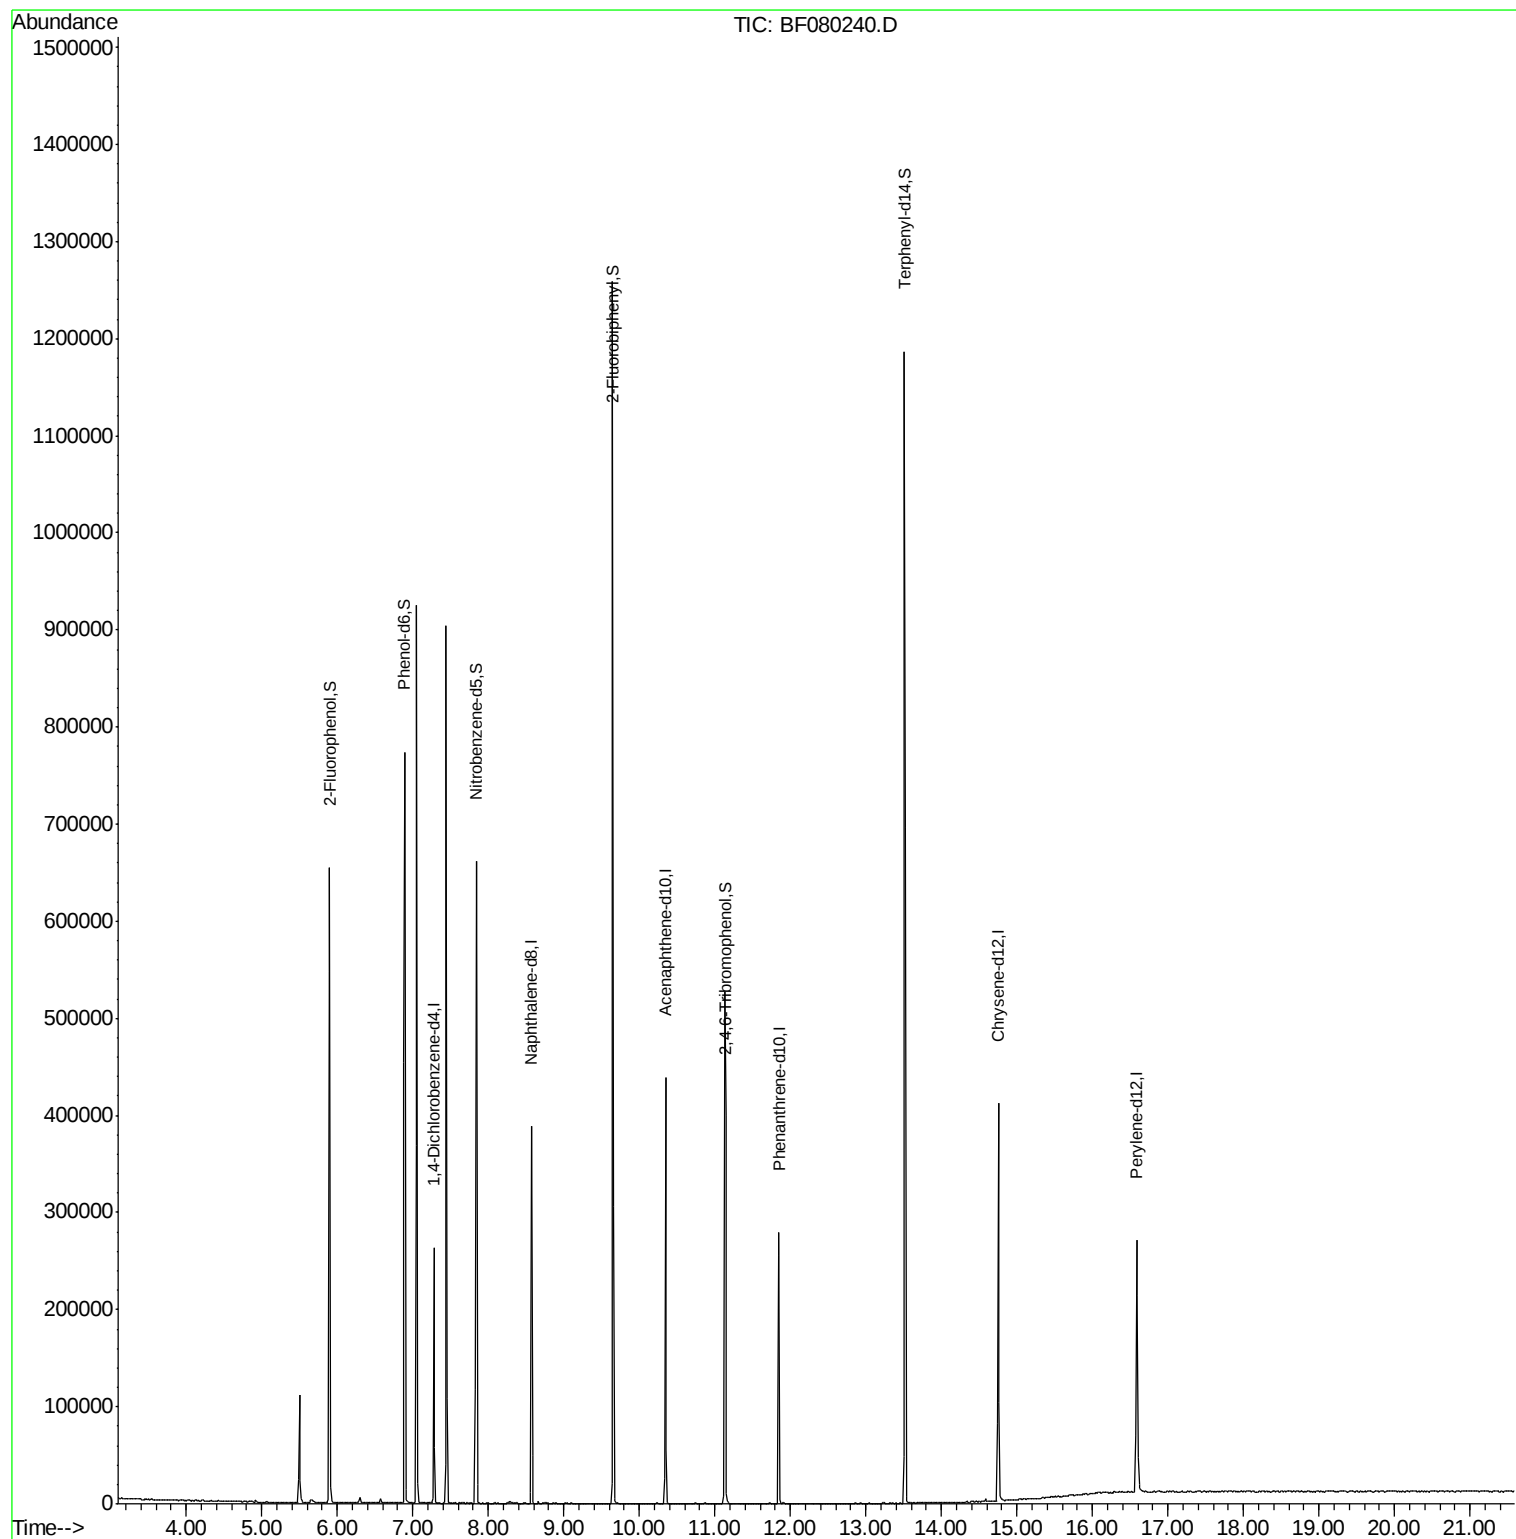

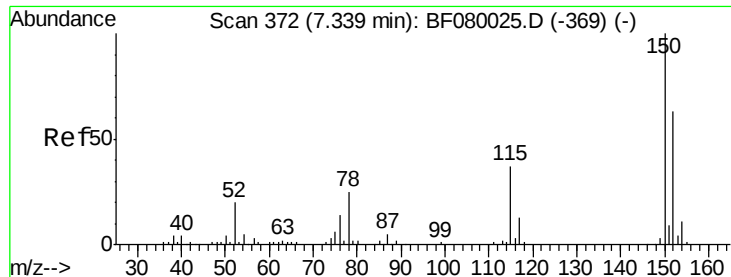

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.28 min Scan# 367

Delta R.T. -0.05 min

Lab File: BF080240.D

Acq: 30 Jun 2015 17:05

Instrument :

BNA_F

ClientSampleId :

PB84281BL





Tgt Ion:152 Resp: 37194

Ion Ratio Lower Upper

152 100

150 158.9 124.7 187.1

115 62.5 39.0 58.4#

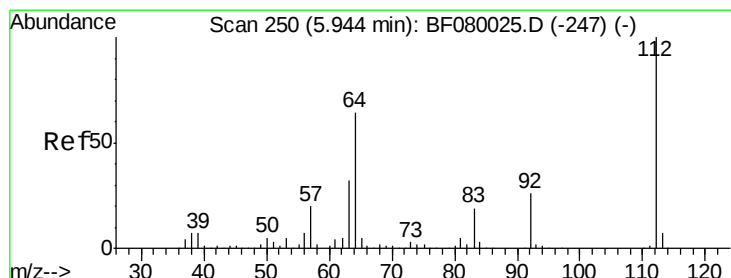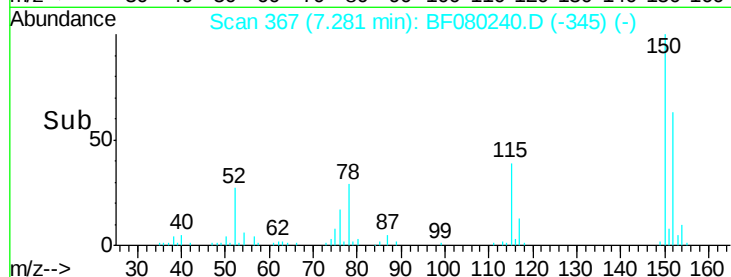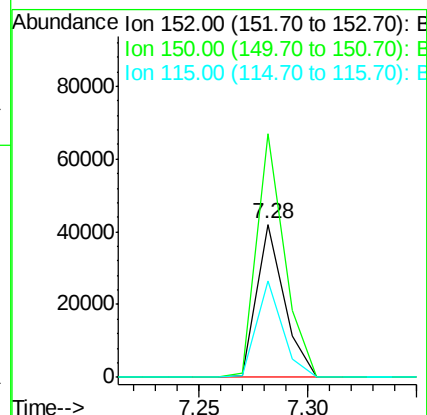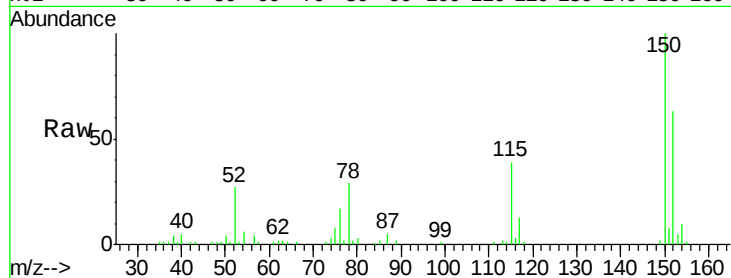

#5

2-Fluorophenol

Concen: 118.05 ng

RT: 5.90 min Scan# 246

Delta R.T. -0.03 min

Lab File: BF080240.D

Acq: 30 Jun 2015 17:05




Tgt Ion:112 Resp: 248038

Ion Ratio Lower Upper

112 100

64 50.2 39.7 59.5

63 25.1 17.4 26.0

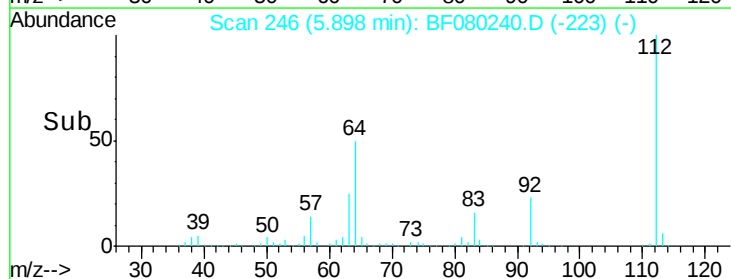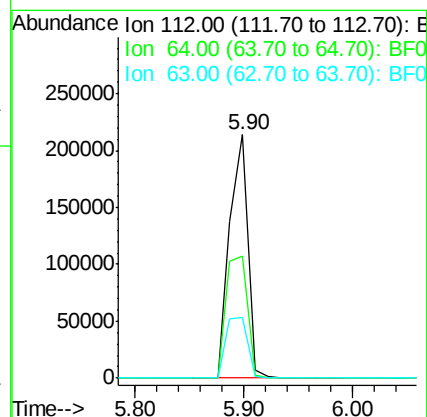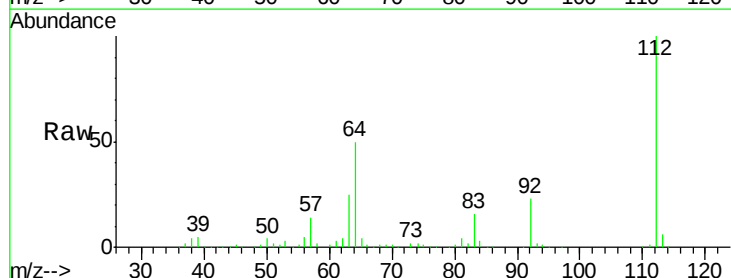



#7

Phenol-d6

Concen: 116.16 ng

RT: 6.89 min Scan# 333

Delta R.T. -0.03 min

Lab File: BF080240.D

Acq: 30 Jun 2015 17:05

Instrument :

BNA_F

ClientSampleId :

PB84281BL


Tgt Ion: 99 Resp: 324798

Ion Ratio Lower Upper

99 100

42 14.6 13.7 20.5




71 27.9 14.2 21.2#

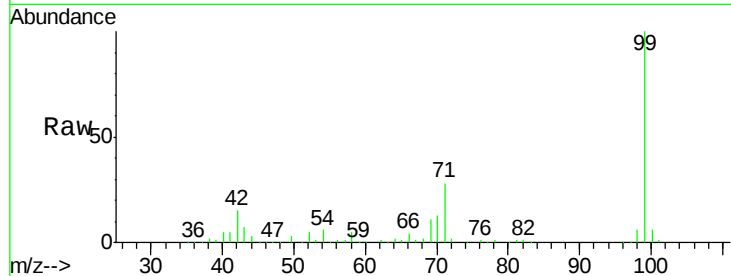

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

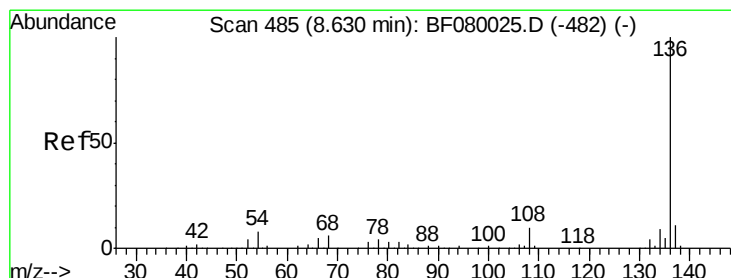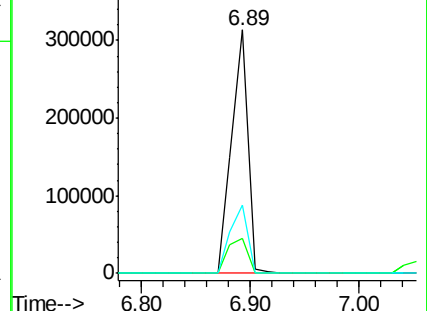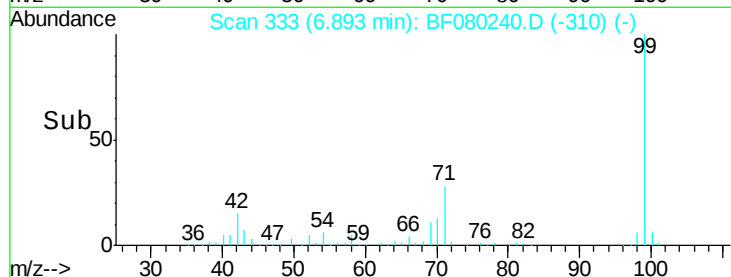

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.57 min Scan# 480

Delta R.T. -0.05 min

Lab File: BF080240.D

Acq: 30 Jun 2015 17:05

Tgt Ion: 136 Resp: 153535


Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.6

54 9.1 8.2 12.2

68 7.0 5.8 8.6


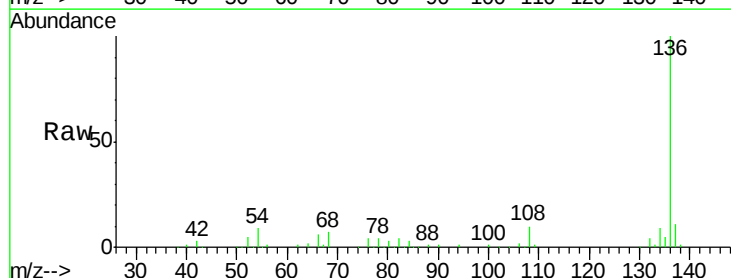



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

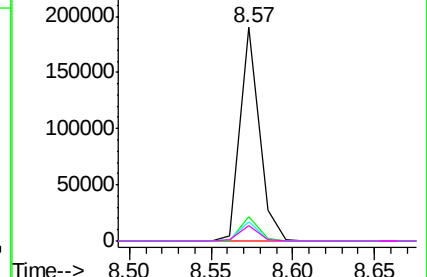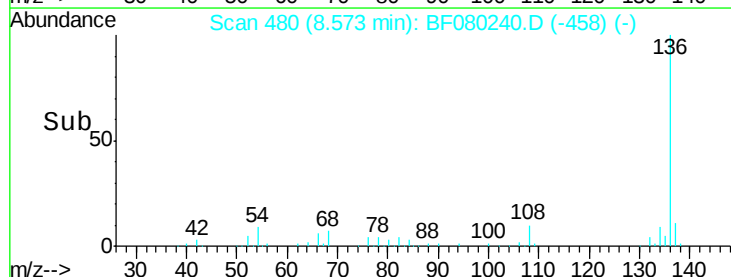


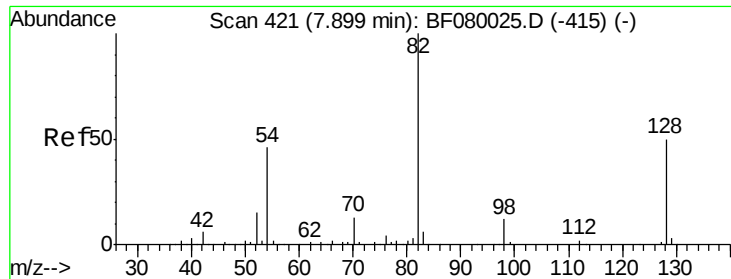




#23
 Nitrobenzene-d5
 Concen: 72.48 ng
 RT: 7.84 min Scan# 416
 Delta R.T. -0.03 min
 Lab File: BF080240.D
 Acq: 30 Jun 2015 17:05

Instrument :
 BNA_F
 ClientSampleId :
 PB84281BL

Tgt Ion	Ratio	Lower	Upper
82	100		
128	44.6	51.0	76.6#
54	49.1	47.5	71.3

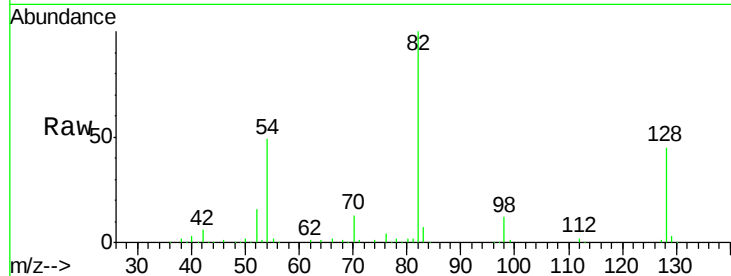


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

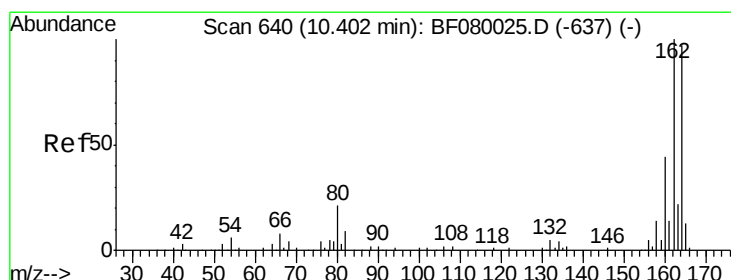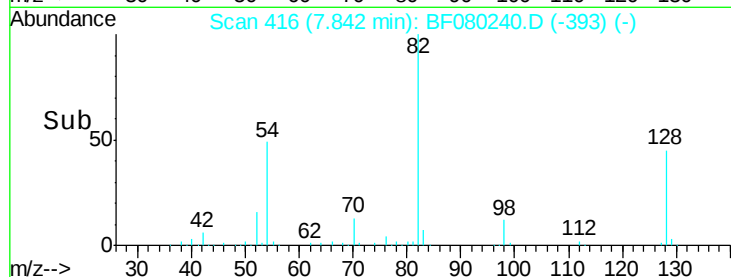
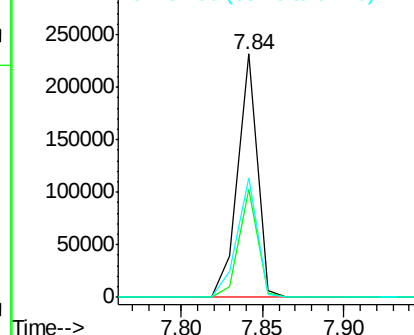


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.34 min Scan# 635
 Delta R.T. -0.05 min
 Lab File: BF080240.D
 Acq: 30 Jun 2015 17:05

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.0	75.2	112.8
160	44.8	31.5	47.3

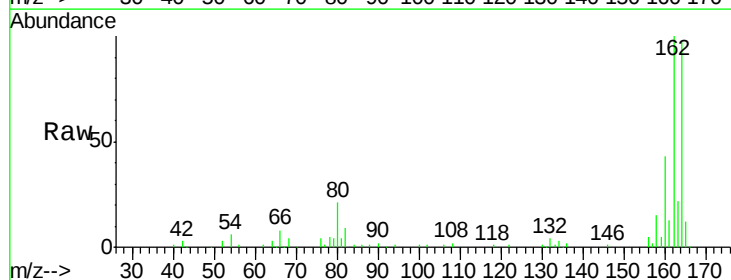

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

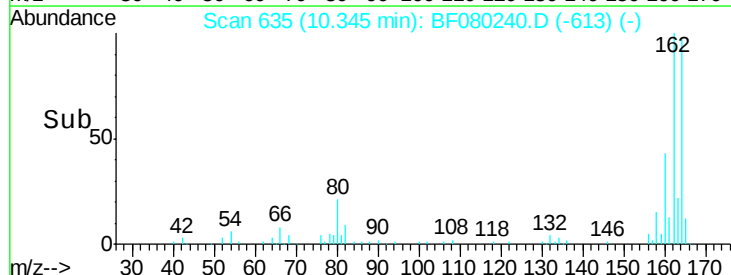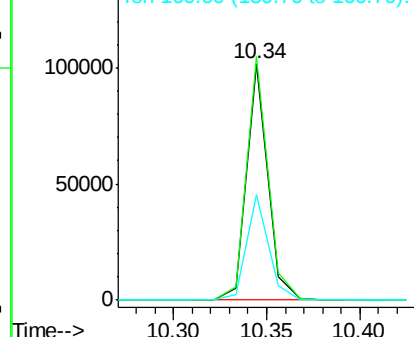






#41
 2,4,6-Tribromophenol
 Concen: 99.74 ng
 RT: 11.14 min Scan# 705
 Delta R.T. -0.03 min
 Lab File: BF080240.D
 Acq: 30 Jun 2015 17:05

Instrument :
 BNA_F
 ClientSampleId :
 PB84281BL

Tgt Ion:330 Resp: 78708
 Ion Ratio Lower Upper
 330 100
 332 98.3 76.6 114.8
 141 36.3 29.7 44.5

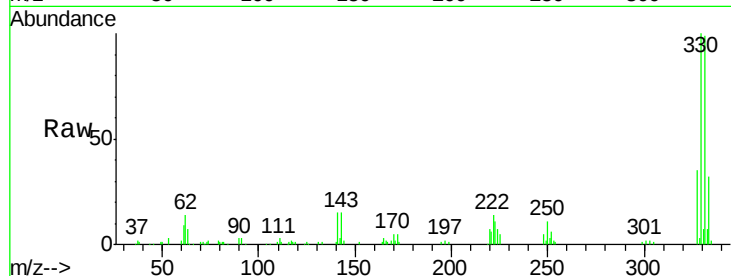


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

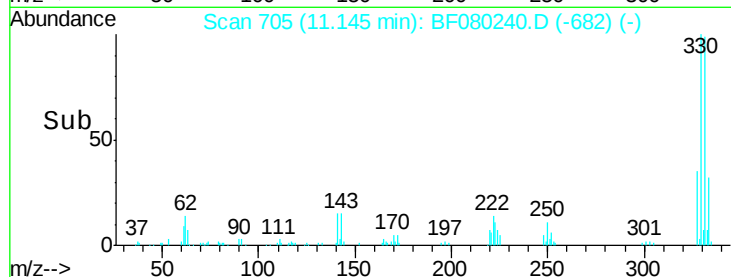
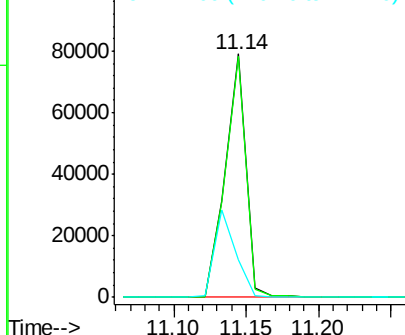



#44
 2-Fluorobiphenyl
 Concen: 67.95 ng
 RT: 9.65 min Scan# 574
 Delta R.T. -0.05 min
 Lab File: BF080240.D
 Acq: 30 Jun 2015 17:05

Tgt Ion:172 Resp: 384542
 Ion Ratio Lower Upper
 172 100
 171 35.7 26.1 39.1
 170 23.8 17.4 26.2

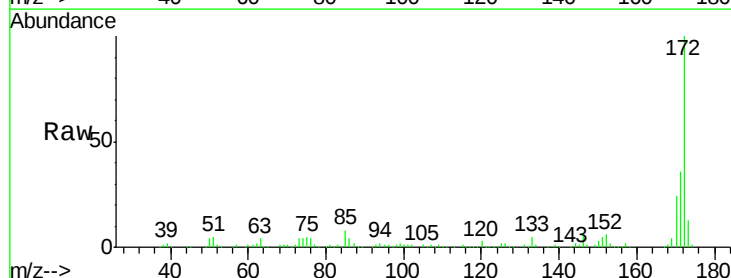

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

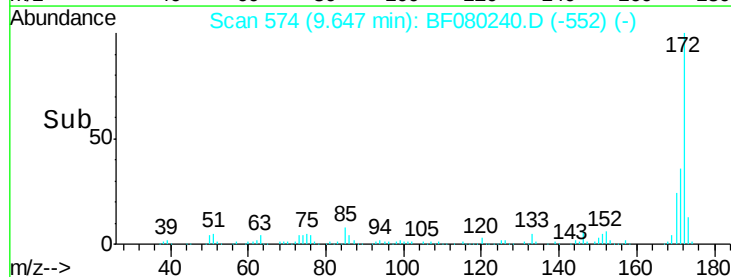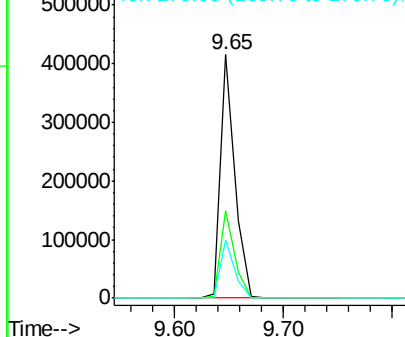


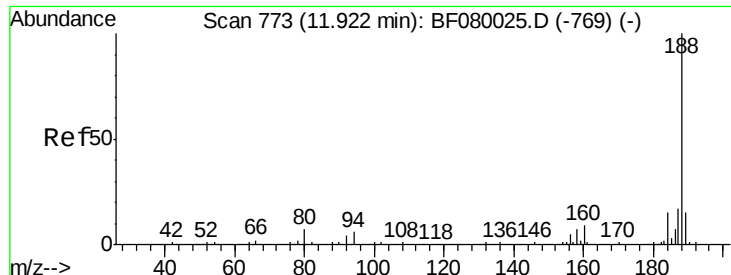




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.85 min Scan# 767
Delta R.T. -0.06 min
Lab File: BF080240.D
Acq: 30 Jun 2015 17:05

Instrument :
BNA_F
ClientSampleId :
PB84281BL

Tgt Ion:188 Resp: 153823
Ion Ratio Lower Upper
188 100
94 6.0 11.1 16.7#
80 6.6 11.0 16.4#

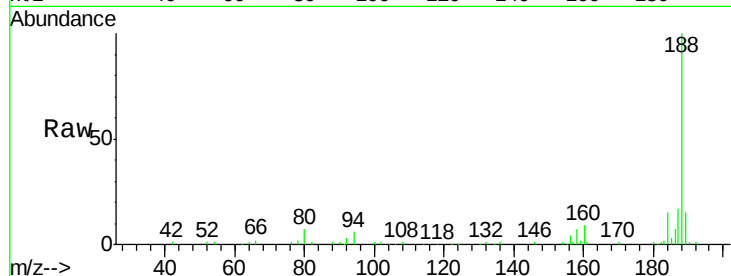


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

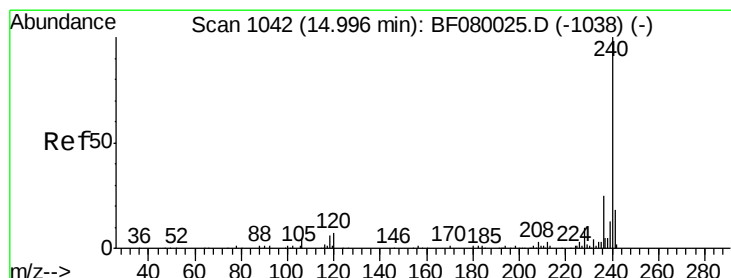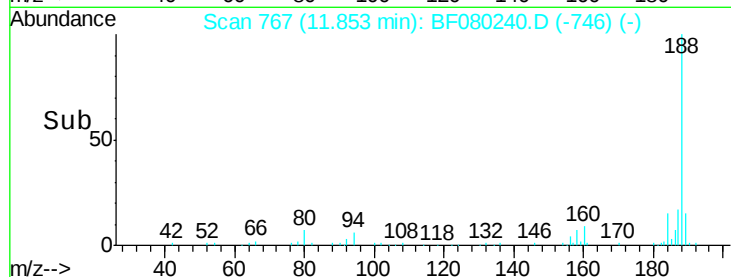
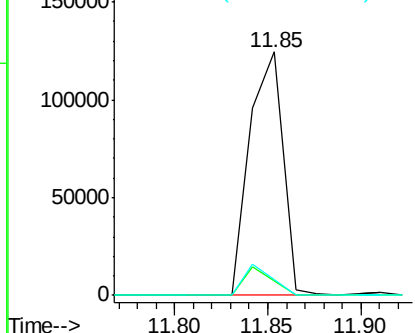



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.76 min Scan# 1021
Delta R.T. -0.24 min
Lab File: BF080240.D
Acq: 30 Jun 2015 17:05

Tgt Ion:240 Resp: 165239
Ion Ratio Lower Upper
240 100
120 10.5 16.2 24.2#
236 25.1 18.4 27.6

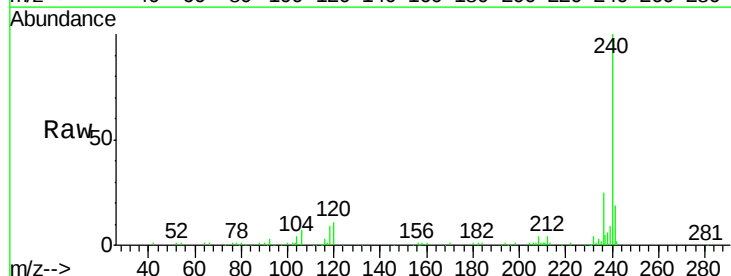

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



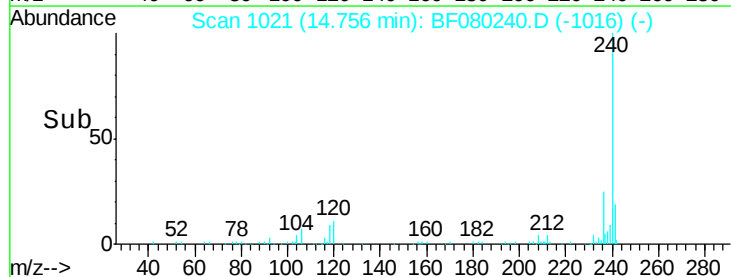
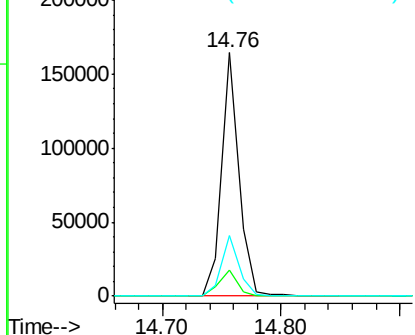


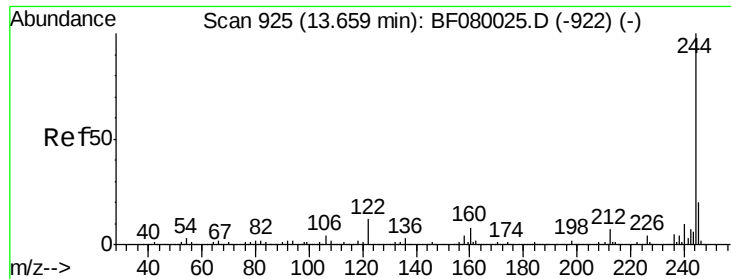

#78
 Terphenyl-d14
 Concen: 67.24 ng
 RT: 13.51 min Scan# 912
 Delta R.T. -0.16 min
 Lab File: BF080240.D
 Acq: 30 Jun 2015 17:05

Instrument :
 BNA_F
 ClientSampleId :
 PB84281BL

Tgt Ion:244 Resp: 475762
 Ion Ratio Lower Upper
 244 100
 212 7.6 4.3 6.5#
 122 15.5 17.4 26.2#

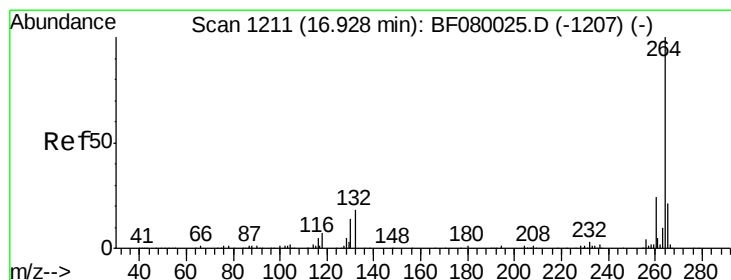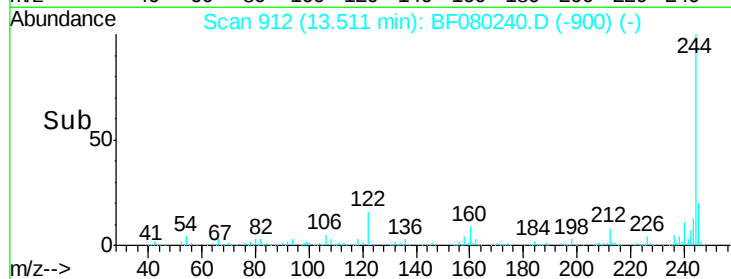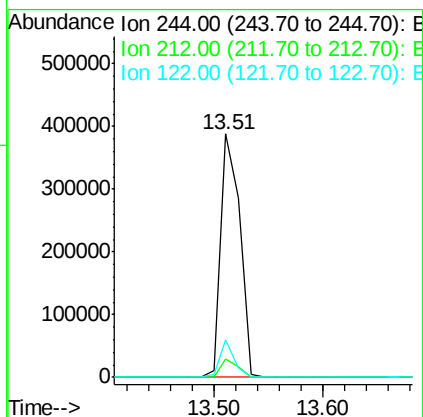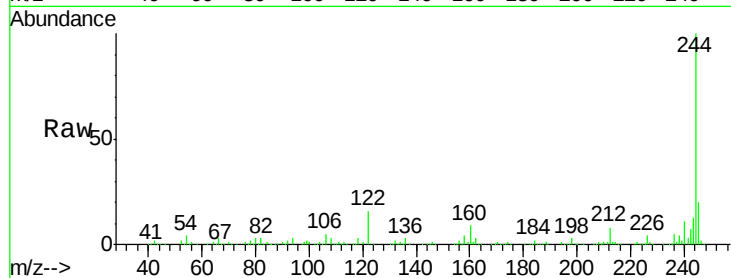

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 16.59 min Scan# 1181
 Delta R.T. -0.34 min
 Lab File: BF080240.D
 Acq: 30 Jun 2015 17:05

Tgt Ion:264 Resp: 158950
 Ion Ratio Lower Upper
 264 100
 260 23.1 16.7 25.1
 265 21.1 17.2 25.8

