

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF063015\  
Data File : BF080233.D  
Acq On : 30 Jun 2015 13:12  
Operator : TP/IZ  
Sample : G2826-05  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF061715.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 7.281       | 365           | 367         | 370          | rVB      | 178286         | 162155        | 46.87%          | 9.742%        |
| 2         | 8.573       | 478           | 480         | 483          | rVB      | 263135         | 228003        | 65.91%          | 13.699%       |
| 3         | 10.230      | 623           | 625         | 630          | rBV      | 3055           | 4381          | 1.27%           | 0.263%        |
| 4         | 10.344      | 633           | 635         | 638          | rVB      | 322502         | 274352        | 79.30%          | 16.483%       |
| 5         | 11.853      | 765           | 767         | 770          | rBV      | 371901         | 305592        | 88.33%          | 18.360%       |
| 6         | 14.802      | 1022          | 1025        | 1027         | rBV      | 256675         | 345957        | 100.00%         | 20.785%       |
| 7         | 15.682      | 1099          | 1102        | 1105         | rBV5     | 1548           | 4544          | 1.31%           | 0.273%        |
| 8         | 16.208      | 1146          | 1148        | 1149         | rBV2     | 2992           | 4822          | 1.39%           | 0.290%        |
| 9         | 16.642      | 1183          | 1186        | 1191         | rBV      | 209220         | 334618        | 96.72%          | 20.104%       |


Sum of corrected areas: 1664424

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF063015\  
Data File : BF080233.D  
Acq On : 30 Jun 2015 13:12  
Operator : TP/IZ  
Sample : G2826-05  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF061715.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

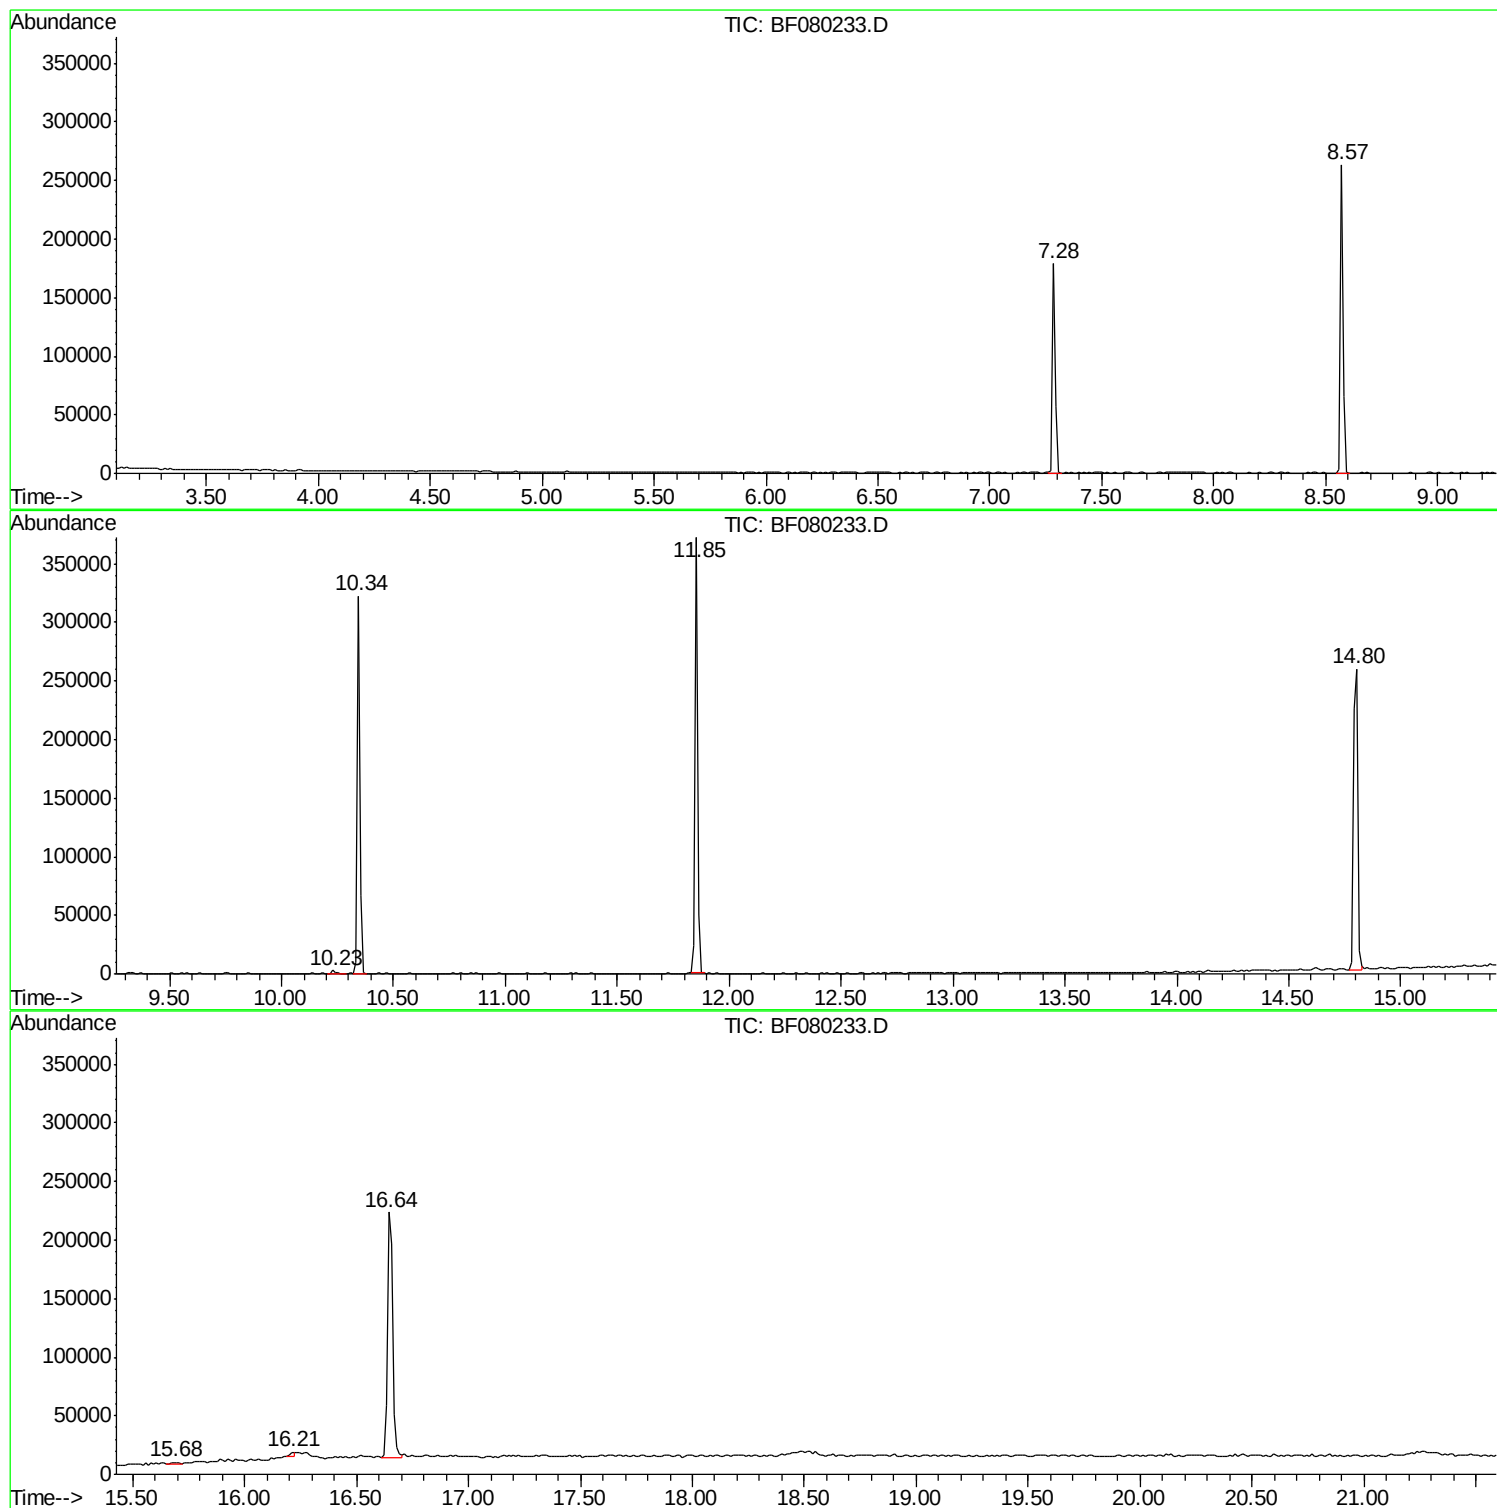

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF063015\  
Data File : BF080233.D  
Acq On : 30 Jun 2015 13:12  
Operator : TP/IZ  
Sample : G2826-05  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF061715.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF063015\  
Data File : BF080233.D  
Acq On : 30 Jun 2015 13:12  
Operator : TP/IZ  
Sample : G2826-05  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF061715.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |

-----