

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
 Data File : BF080234.D
 Acq On : 30 Jun 2015 14:13
 Operator : TP/IZ
 Sample : PB84280BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB84280BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.499	209	211	217	rBV	154133	148625	12.93%	1.894%
2	5.899	243	246	248	rBV	684099	722962	62.88%	9.211%
3	6.893	330	333	335	rBV	819605	759443	66.05%	9.676%
4	7.053	345	347	349	rBV	915777	786546	68.41%	10.021%
5	7.282	365	367	370	rBV	195309	191386	16.64%	2.438%
6	7.442	379	381	384	rVB	675528	596168	51.85%	7.596%
7	7.842	414	416	418	rBV	588117	461540	40.14%	5.880%
8	8.573	478	480	483	rVB	270136	257160	22.37%	3.276%
9	9.648	572	574	577	rBV	711082	878798	76.43%	11.197%
10	10.345	633	635	638	rBB2	307736	297237	25.85%	3.787%
11	11.145	703	705	707	rBV	629646	566275	49.25%	7.215%
12	11.865	766	768	771	rBV2	241195	318069	27.66%	4.052%
13	13.648	922	924	927	rBV	1138031	1149829	100.00%	14.650%
14	15.008	1041	1043	1046	rBV	292504	358837	31.21%	4.572%
15	16.985	1213	1216	1221	rBV	253596	355921	30.95%	4.535%


Sum of corrected areas: 7848796

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080234.D
Acq On : 30 Jun 2015 14:13
Operator : TP/IZ
Sample : PB84280BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84280BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

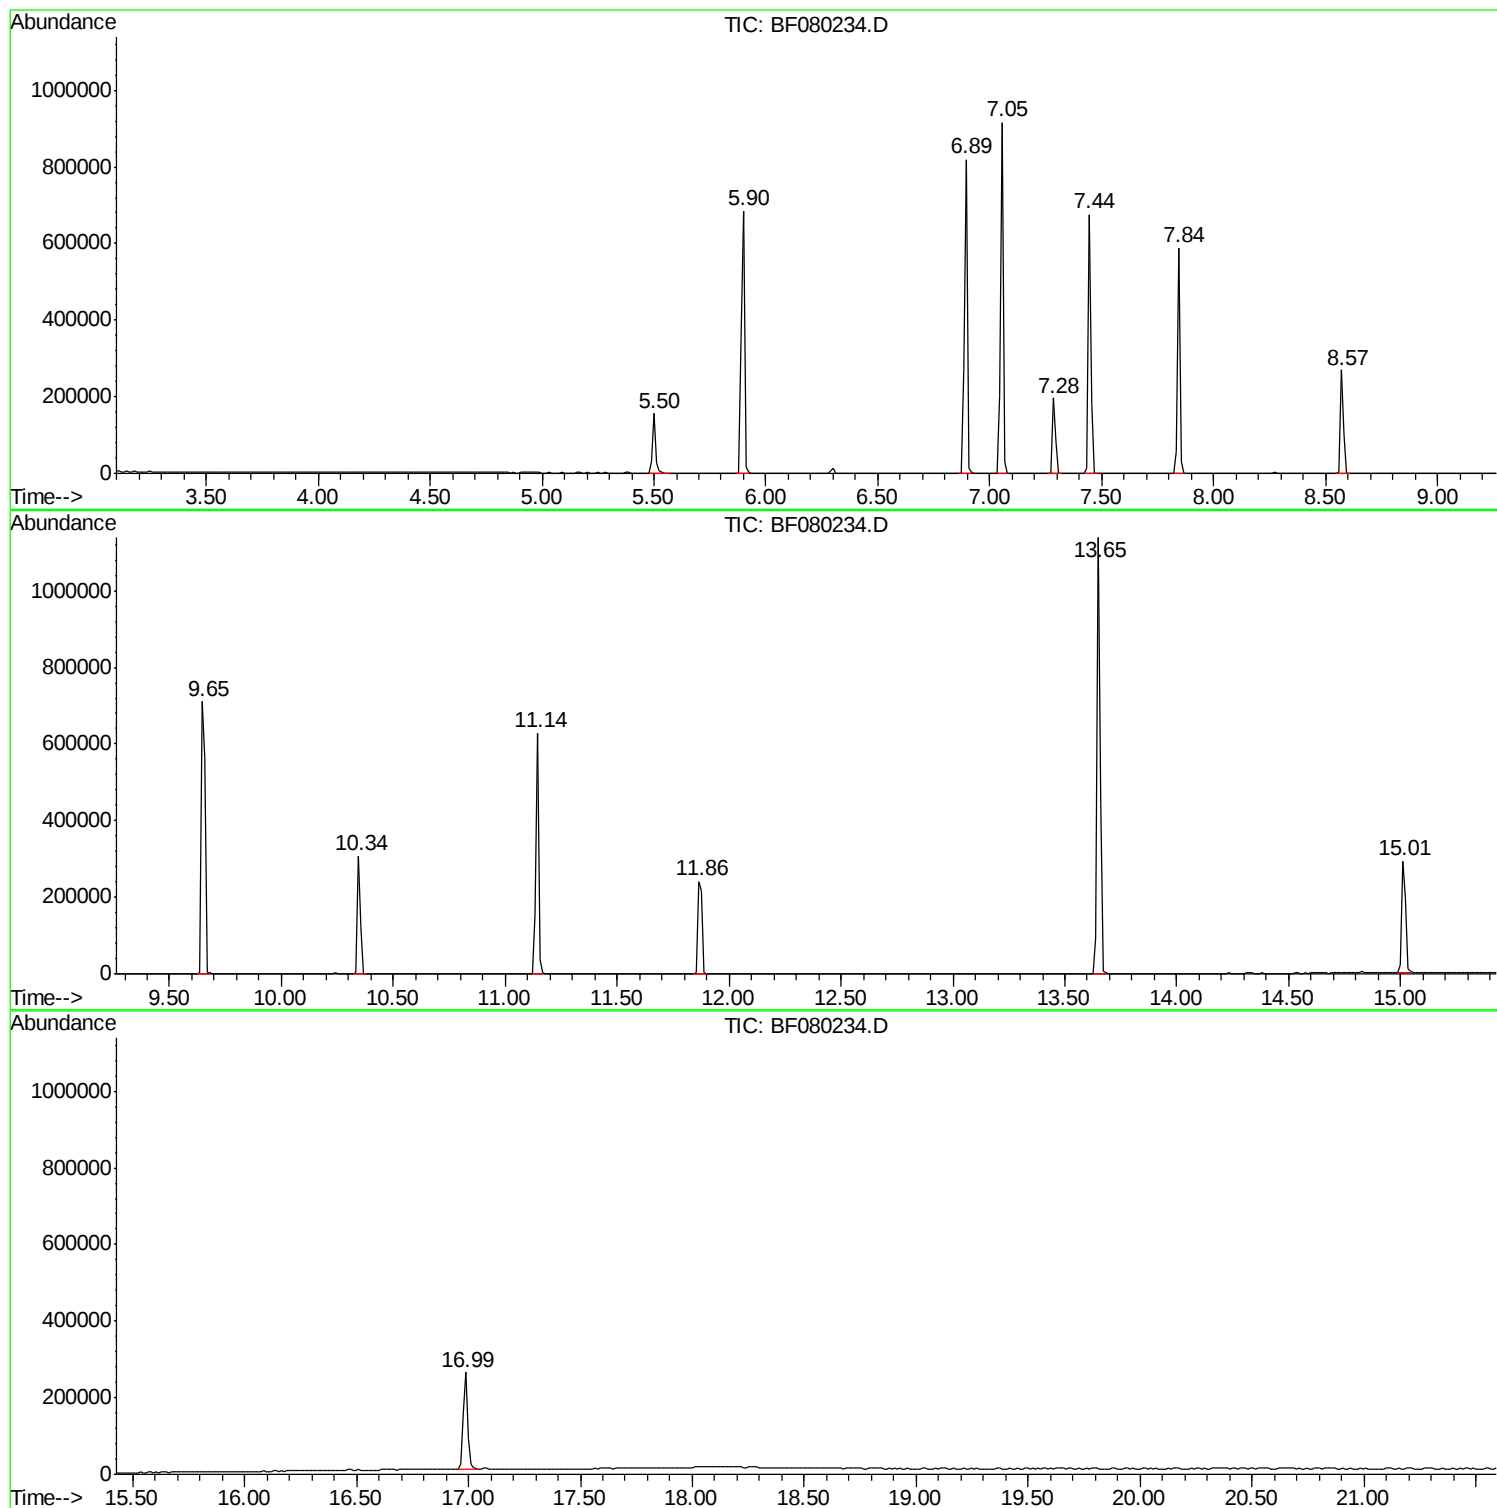

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080234.D
Acq On : 30 Jun 2015 14:13
Operator : TP/IZ
Sample : PB84280BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84280BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.50	15.53 ng	148625	1,4-Dichlorobenzene-d4	7.28

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4			1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	23
5			Acetone	58	C3H6O	000067-64-1	9

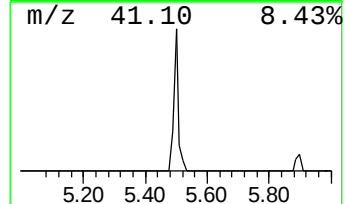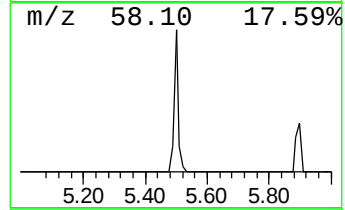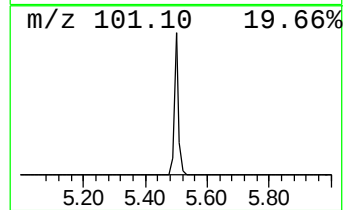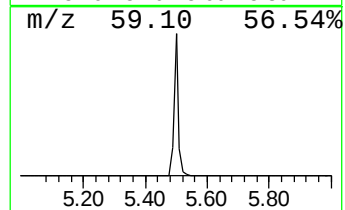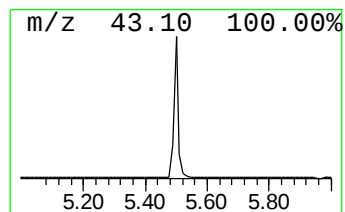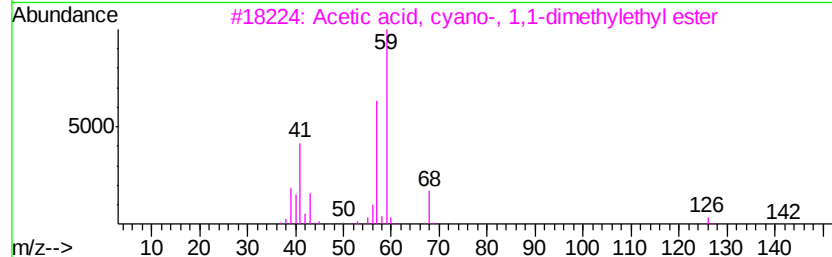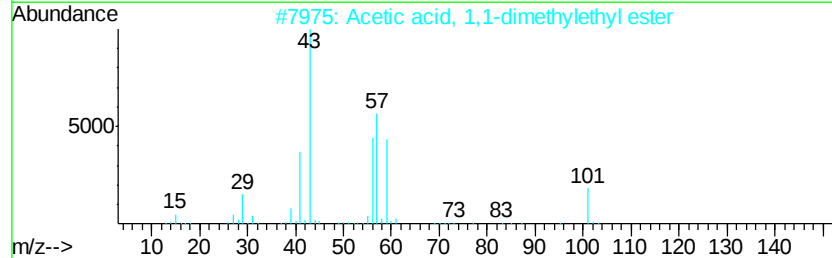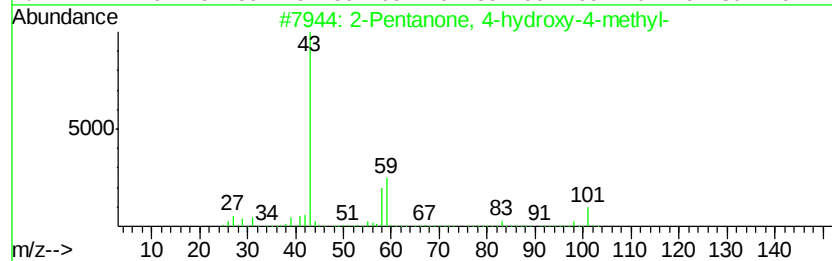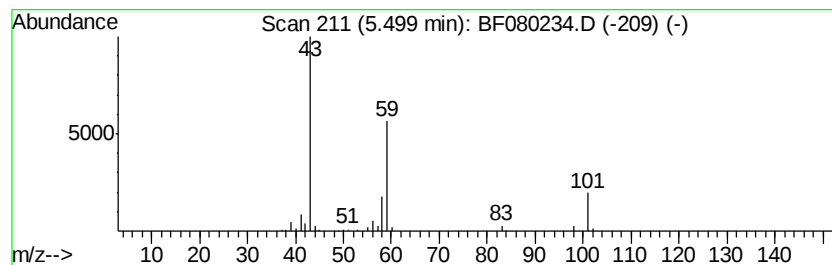

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080234.D
Acq On : 30 Jun 2015 14:13
Operator : TP/IZ
Sample : PB84280BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84280BL








Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.05 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.05	82.19 ng	786546	1,4-Dichlorobenzene-d4	7.28

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

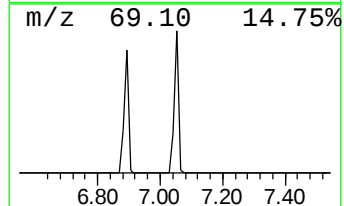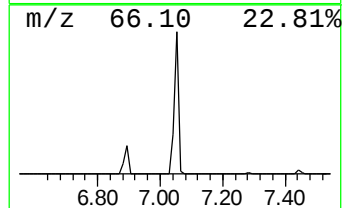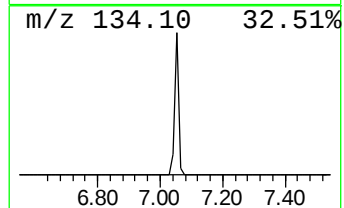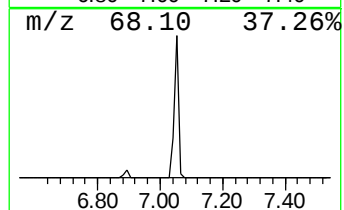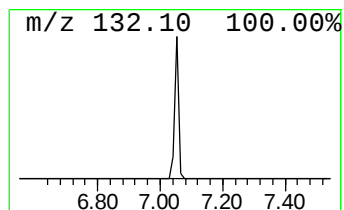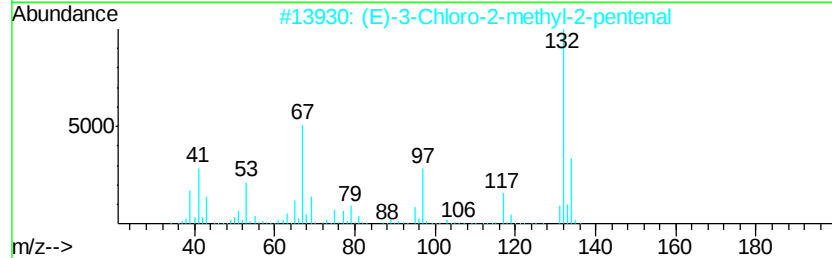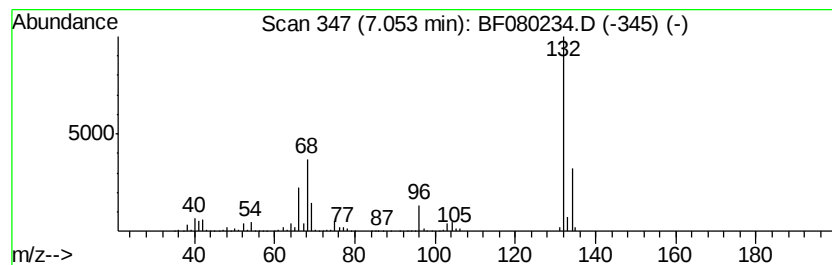

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080234.D
Acq On : 30 Jun 2015 14:13
Operator : TP/IZ
Sample : PB84280BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84280BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.50	15.5	ng	148625	1	7.28	191386	20.0
unknown7.05	7.05	82.2	ng	786546	1	7.28	191386	20.0