

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
 Data File : BF080254.D
 Acq On : 1 Jul 2015 1:46
 Operator : TP/IZ
 Sample : G2841-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SIDEWALLWEST(4FT)-062915

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.498	208	211	216	rVB	120500	168516	12.89%	1.911%
2	5.887	243	245	248	rBV	686054	769776	58.88%	8.729%
3	6.893	330	333	335	rBV	619261	796881	60.95%	9.036%
4	7.053	344	347	349	rBV	826238	852141	65.18%	9.663%
5	7.281	365	367	369	rBV	234755	199241	15.24%	2.259%
6	7.441	379	381	383	rBV	851664	683477	52.28%	7.750%
7	7.841	413	416	418	rBV	604925	510097	39.02%	5.784%
8	8.573	478	480	482	rBV	339852	268502	20.54%	3.045%
9	9.647	572	574	577	rVB	1229712	1065536	81.50%	12.083%
10	10.036	606	608	611	rBV	162895	135935	10.40%	1.541%
11	10.345	633	635	638	rBV	376485	318311	24.35%	3.610%
12	11.133	702	704	707	rBV2	512349	619736	47.40%	7.028%
13	11.853	765	767	769	rBV	354054	344930	26.38%	3.911%
14	13.534	911	914	916	rBV	1349401	1307388	100.00%	14.825%
15	14.585	1004	1006	1012	rBV	16431	34947	2.67%	0.396%
16	14.791	1022	1024	1027	rBV	298327	365436	27.95%	4.144%
17	16.654	1184	1187	1190	rBV	243943	338161	25.87%	3.835%
18	18.025	1302	1307	1314	rVB3	10518	39593	3.03%	0.449%


Sum of corrected areas: 8818604

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080254.D
Acq On : 1 Jul 2015 1:46
Operator : TP/IZ
Sample : G2841-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SIDEWALLWEST(4FT)-062915

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

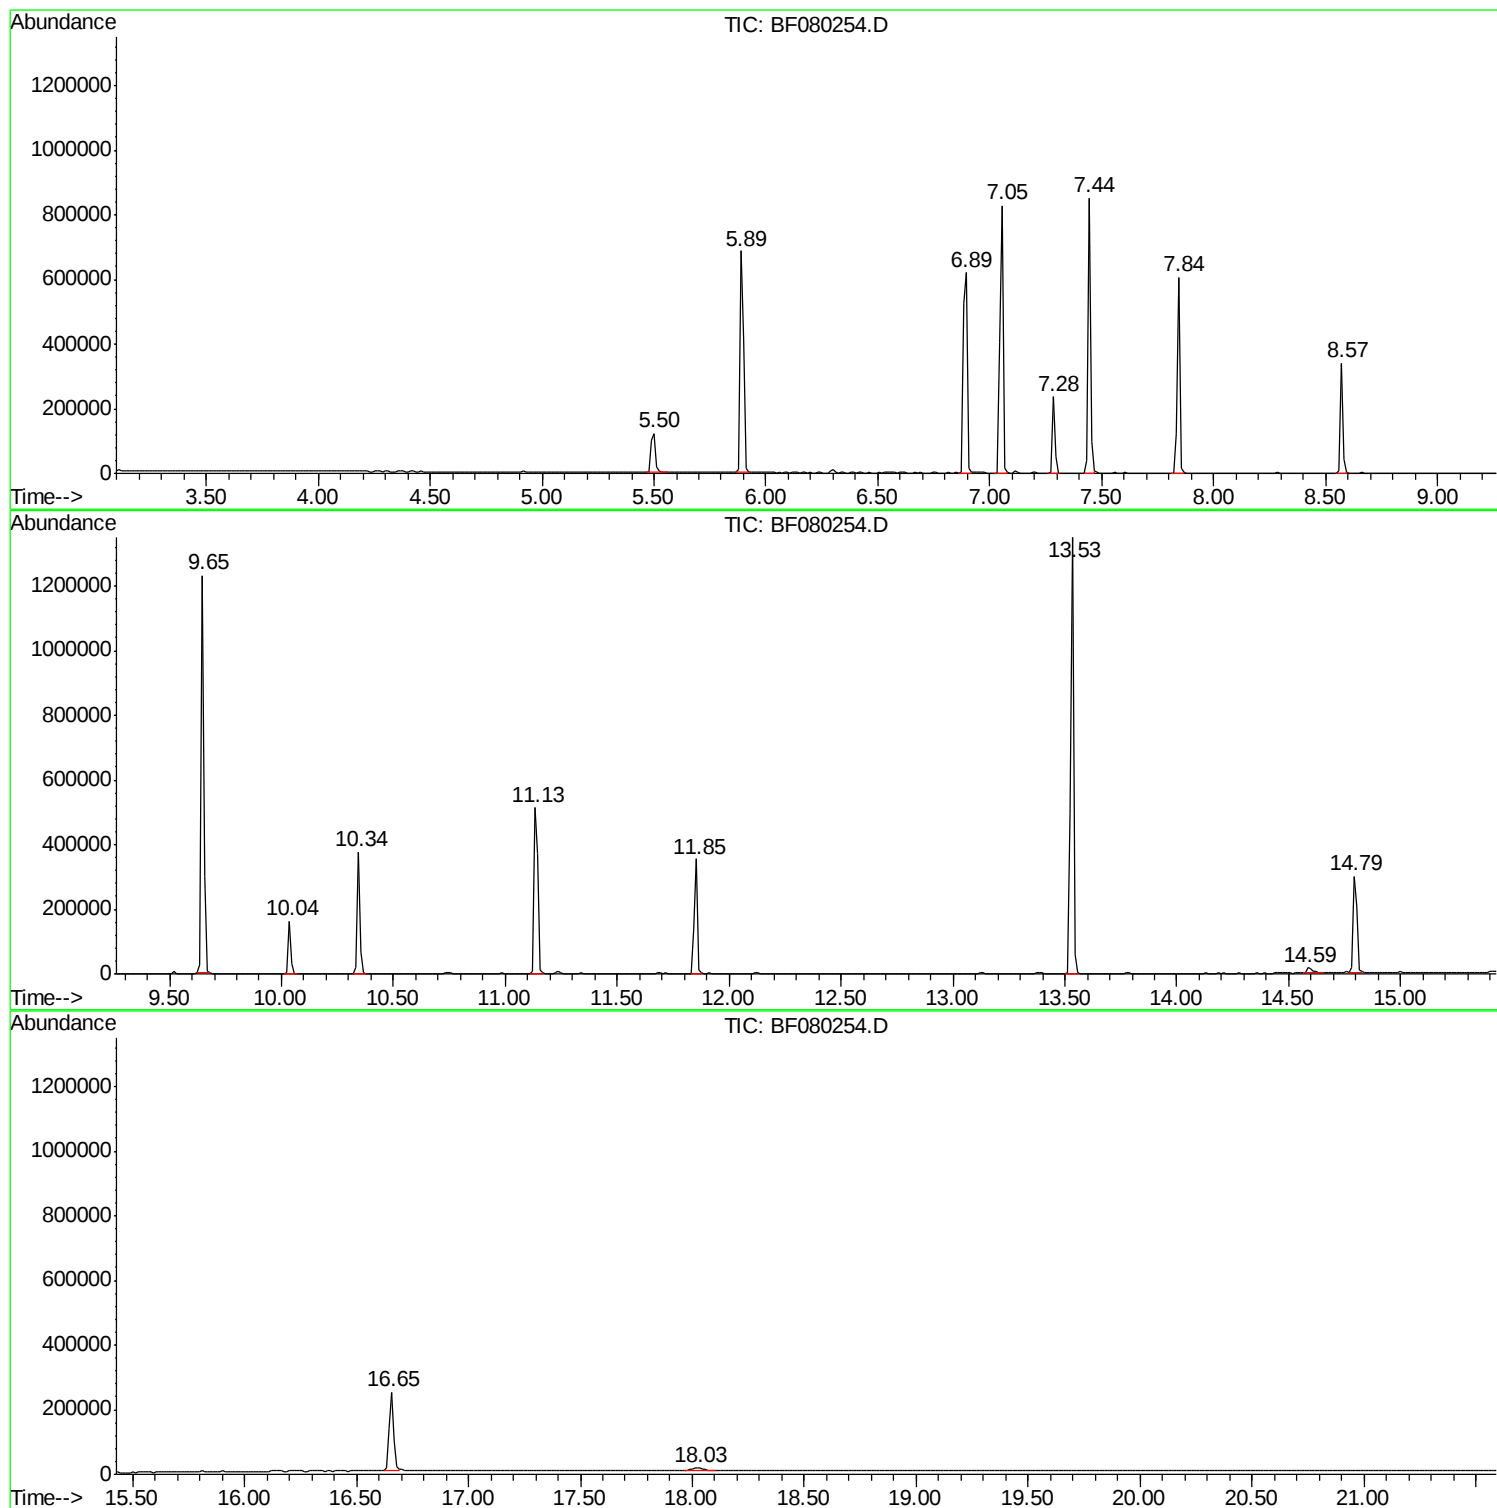

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080254.D
Acq On : 1 Jul 2015 1:46
Operator : TP/IZ
Sample : G2841-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SIDEWALLWEST(4FT)-062915










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.50	16.92 ng	168516	1,4-Dichlorobenzene-d4	7.28

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53
2		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
3		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
4		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

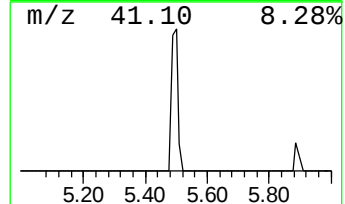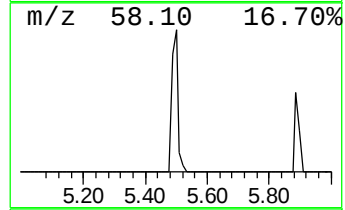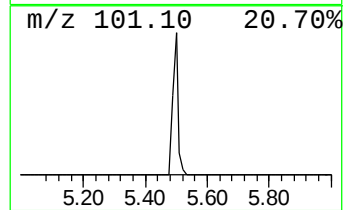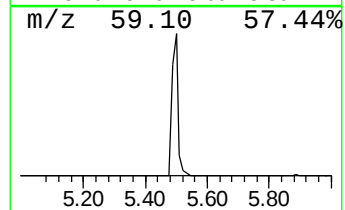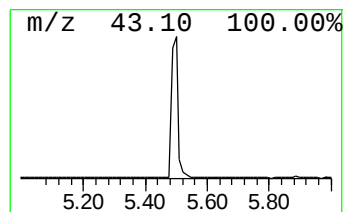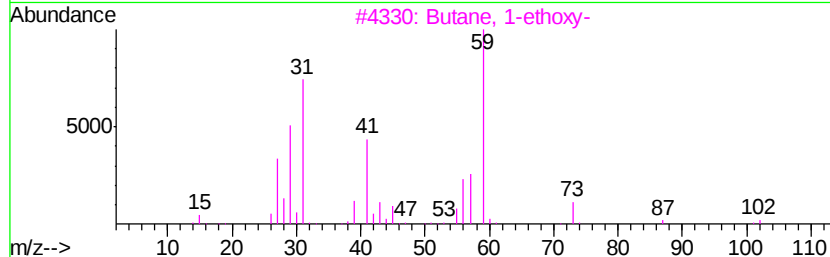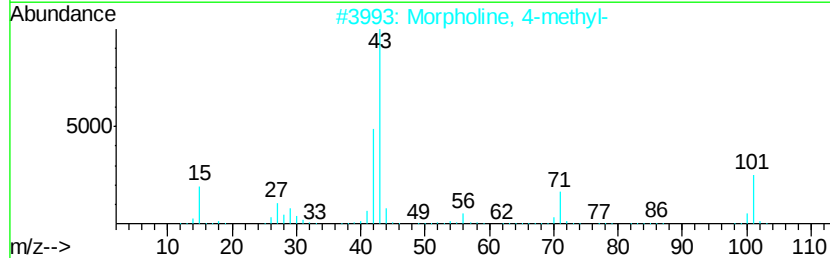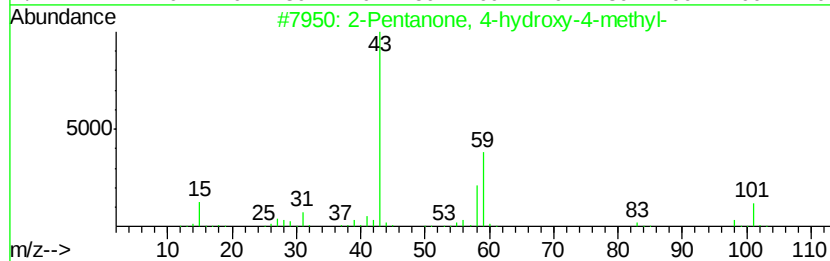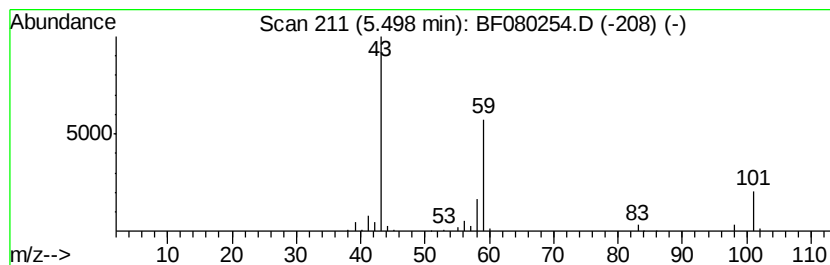

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080254.D
Acq On : 1 Jul 2015 1:46
Operator : TP/IZ
Sample : G2841-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SIDEWALLWEST(4FT)-062915










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.05 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.05	85.54 ng	852141	1,4-Dichlorobenzene-d4	7.28

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	38
2	Amphetaminil			250	C17H18N2	017590-01-1	12
3	(E)-3-Chloro-2-methyl-2-pentenal			132	C6H9ClO	031357-76-3	12
4	5-Aminoindole			132	C8H8N2	005192-03-0	12
5	Xenon			132	Xe	007440-63-3	9

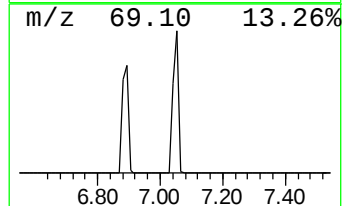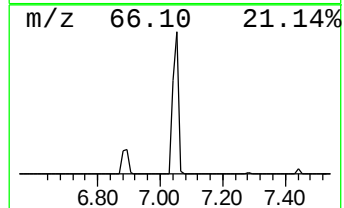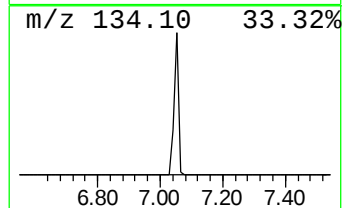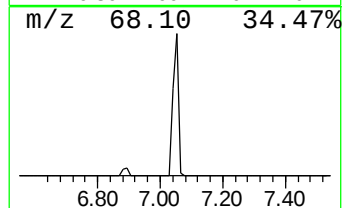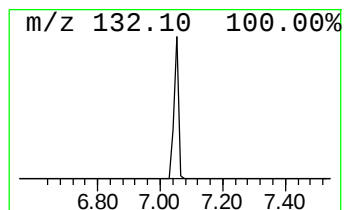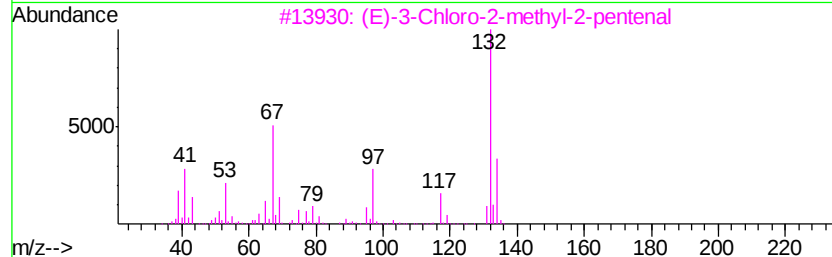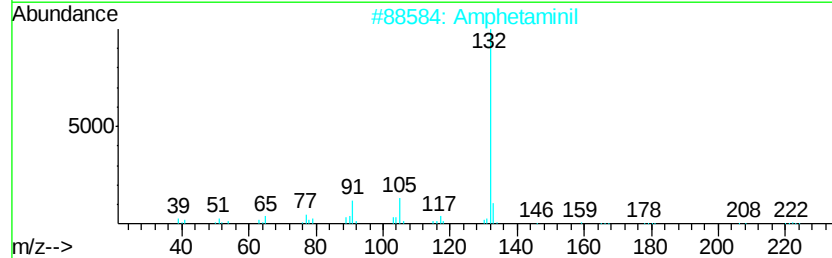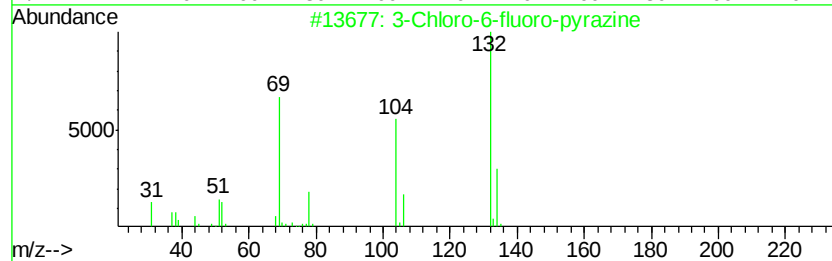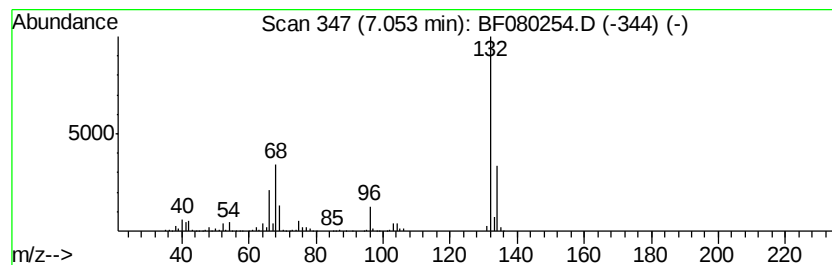

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063015\
Data File : BF080254.D
Acq On : 1 Jul 2015 1:46
Operator : TP/IZ
Sample : G2841-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SIDEWALLWEST(4FT)-062915

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.50	16.9	ng	168516	1	7.28	199241	20.0
unknown7.05	7.05	85.5	ng	852141	1	7.28	199241	20.0