


Data Path : Z:\HPCHEM1\BNA_F\Data\BF063015\
 Data File : BF080252.D
 Acq On : 1 Jul 2015 00:19
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 01 18:15:00 2015

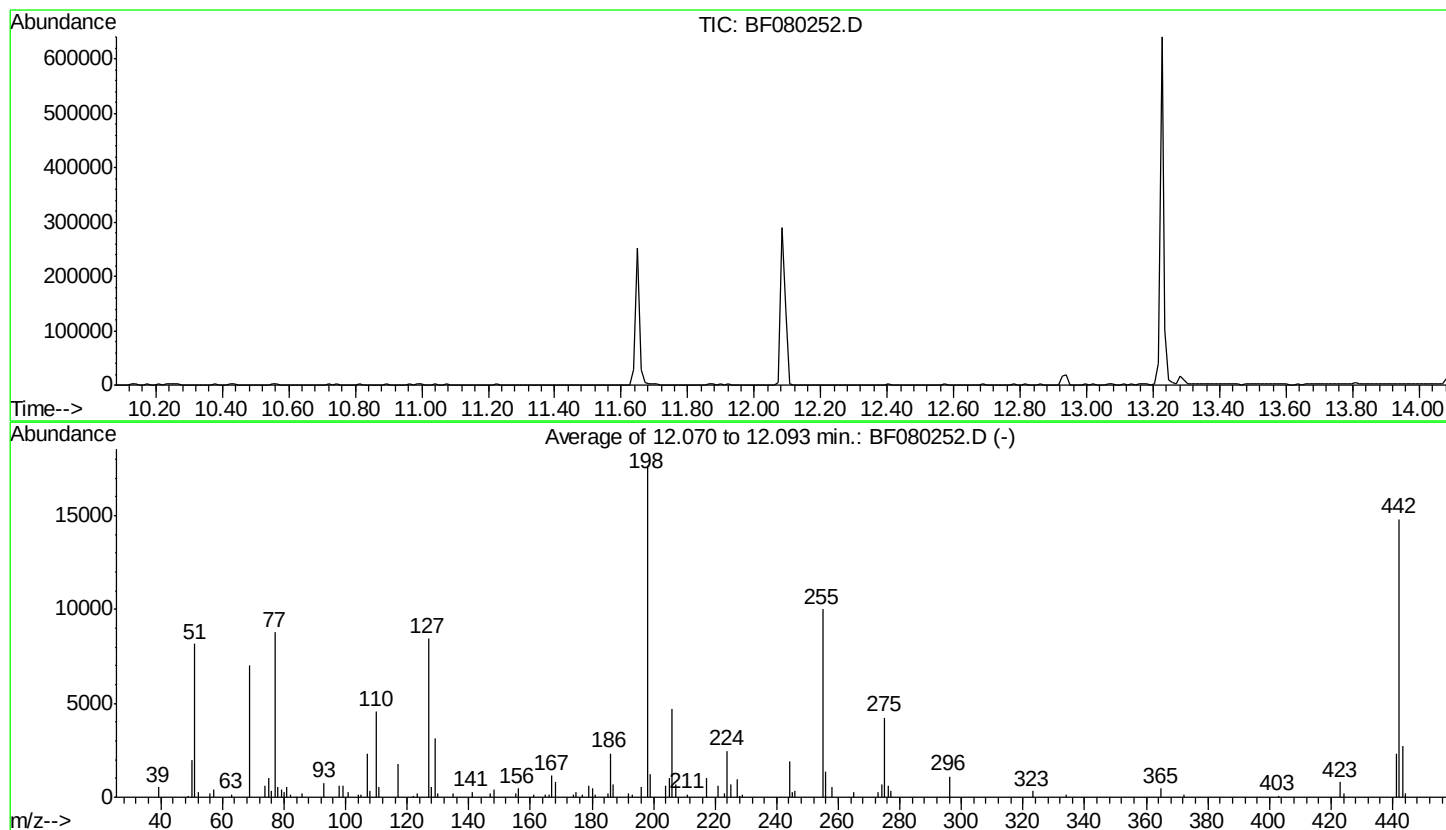

AutoFind: Scans 786, 787, 788; Background Corrected with Scan 783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	8173	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.9	7050	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	8440	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17671	PASS
199	198	5	9	7.1	1251	PASS
275	198	10	60	24.1	4254	PASS
365	198	1	100	2.7	477	PASS
441	442	0.01	24	15.8	2340	PASS
442	198	50	100	83.8	14809	PASS
443	442	15	24	18.3	2714	PASS