
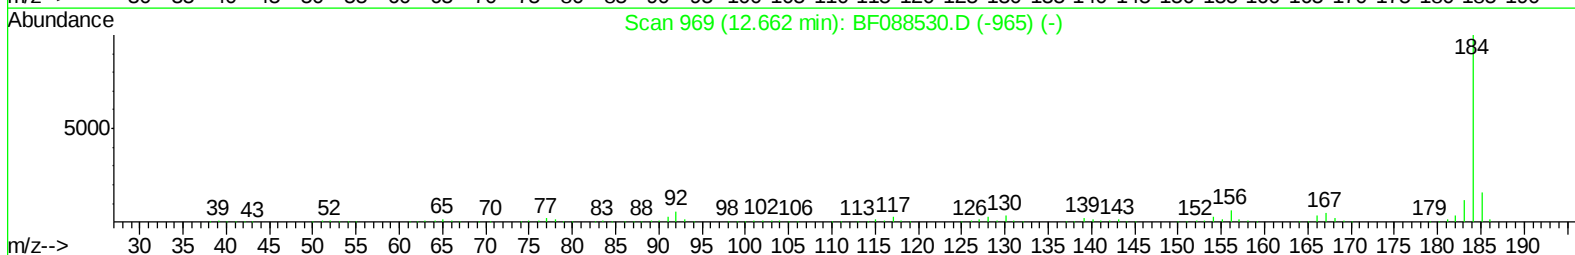
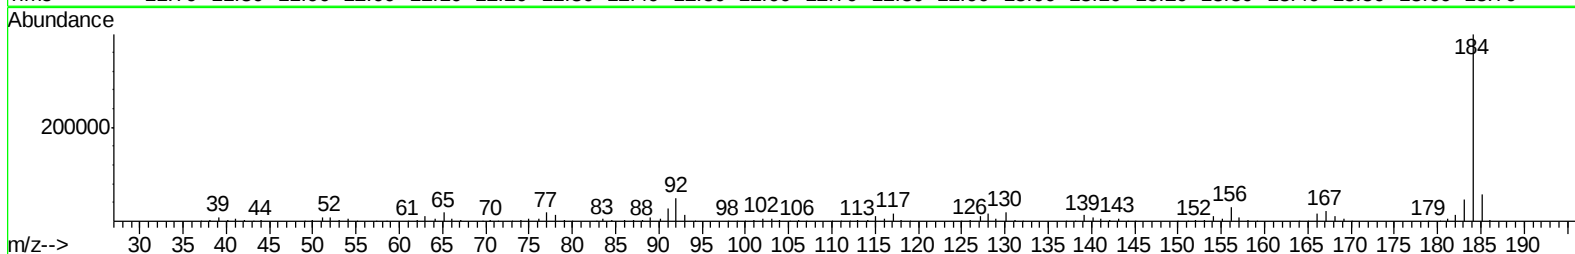


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063016\
Data File : BF088525.D
Acq On : 30 Jun 2016 8:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 07:21:09 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 01 01:58:49 2016
Response via : Initial Calibration

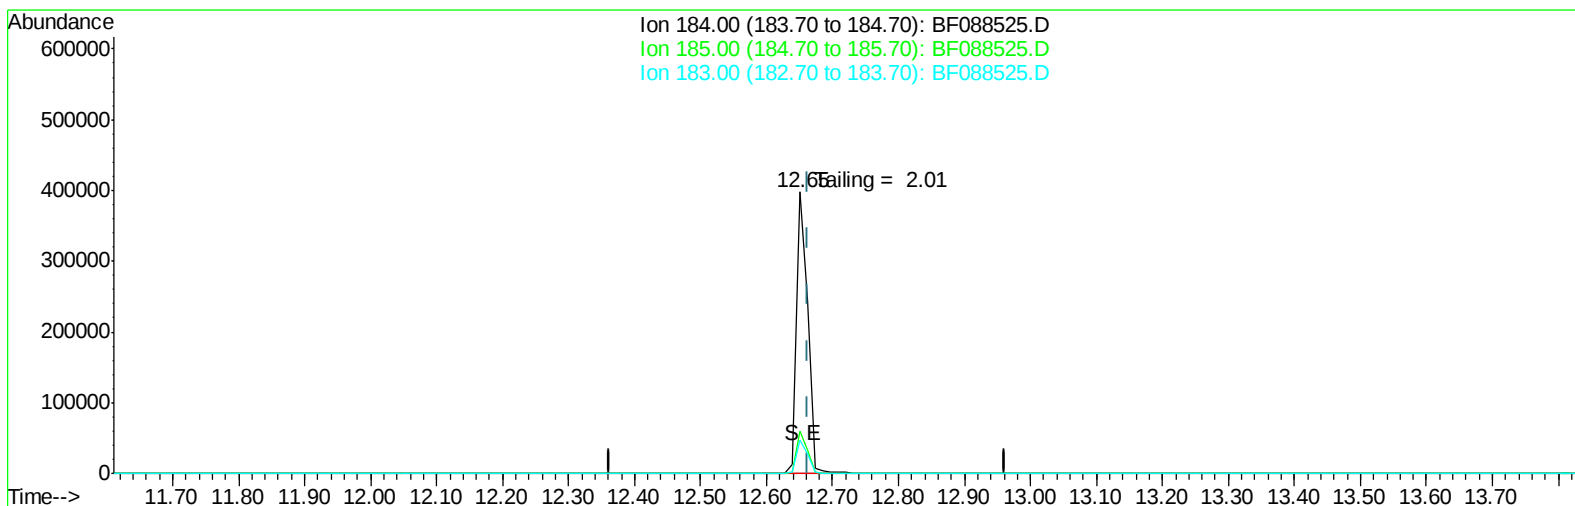

TIC: BF088525.D

(76) Benzidine




12.651min (-0.011) 0.00ng

response 460677

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.82
183.00	11.60	11.70
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063016\
Data File : BF088525.D
Acq On : 30 Jun 2016 8:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 07:21:09 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 01 01:58:49 2016
Response via : Initial Calibration

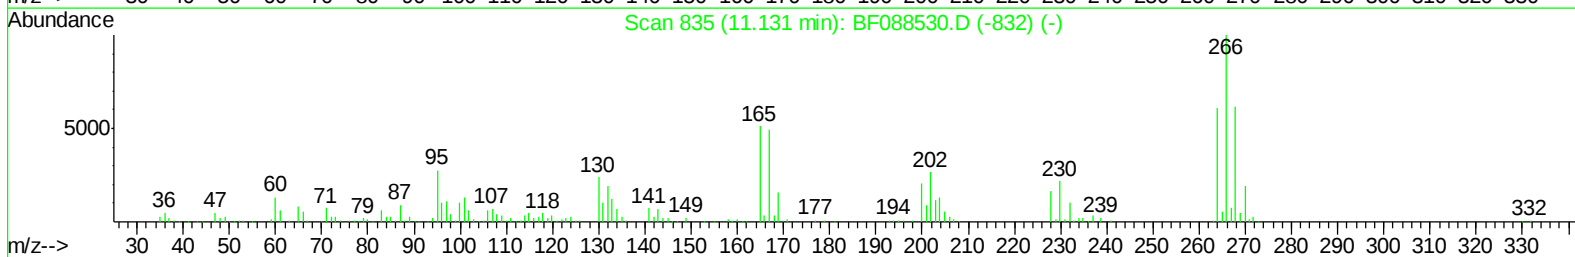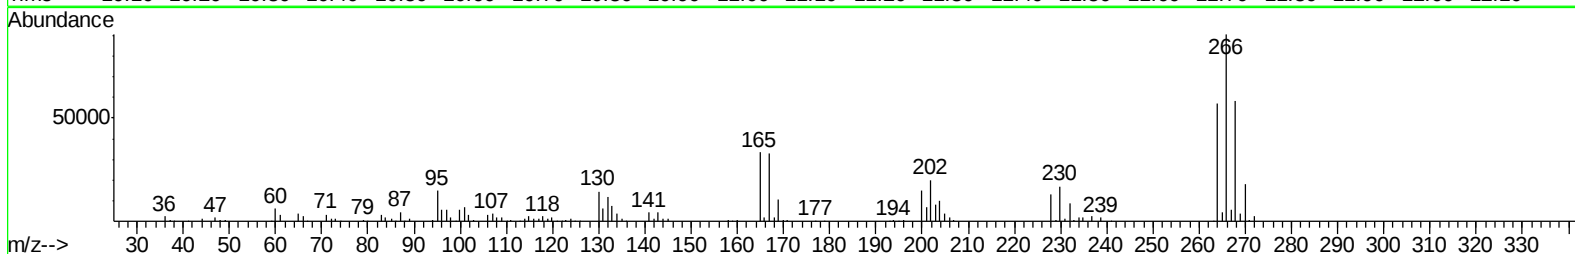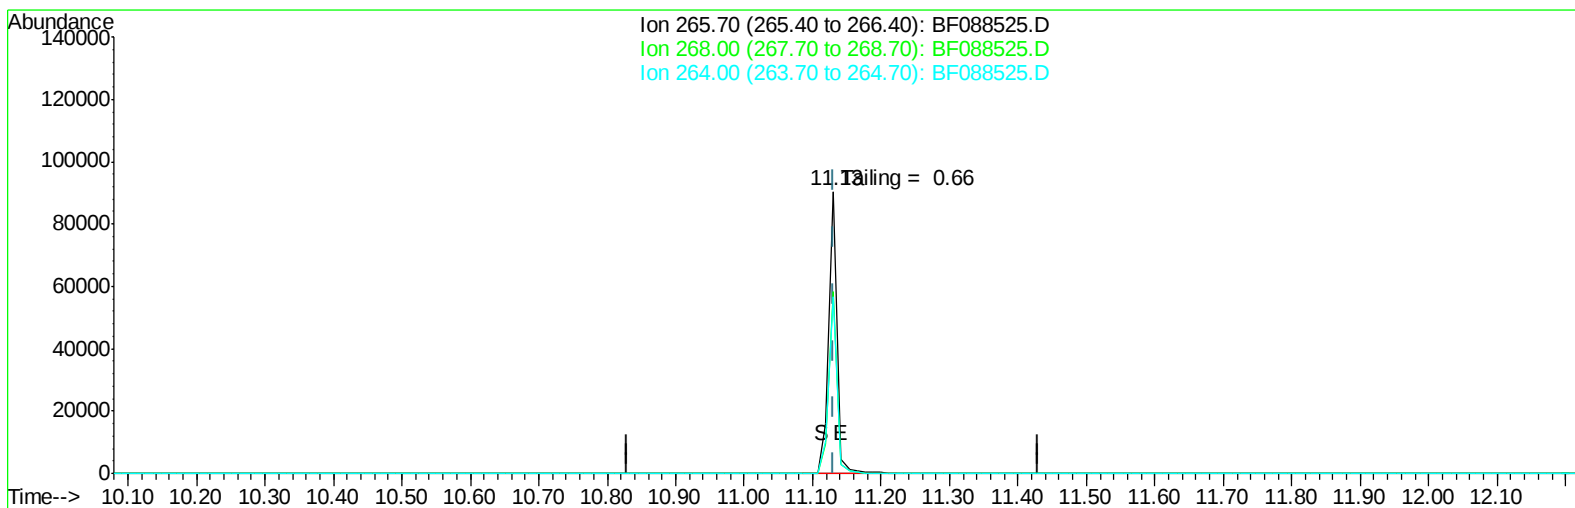

TIC: BF088525.D

(69) Pentachlorophenol (C)

11.131min (+0.000) 0.00ng

response 78139

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	64.72
264.00	62.00	62.92
0.00	0.00	0.00