


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063016\
 Data File : BF088525.D
 Acq On : 30 Jun 2016 8:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 30 18:01:55 2016

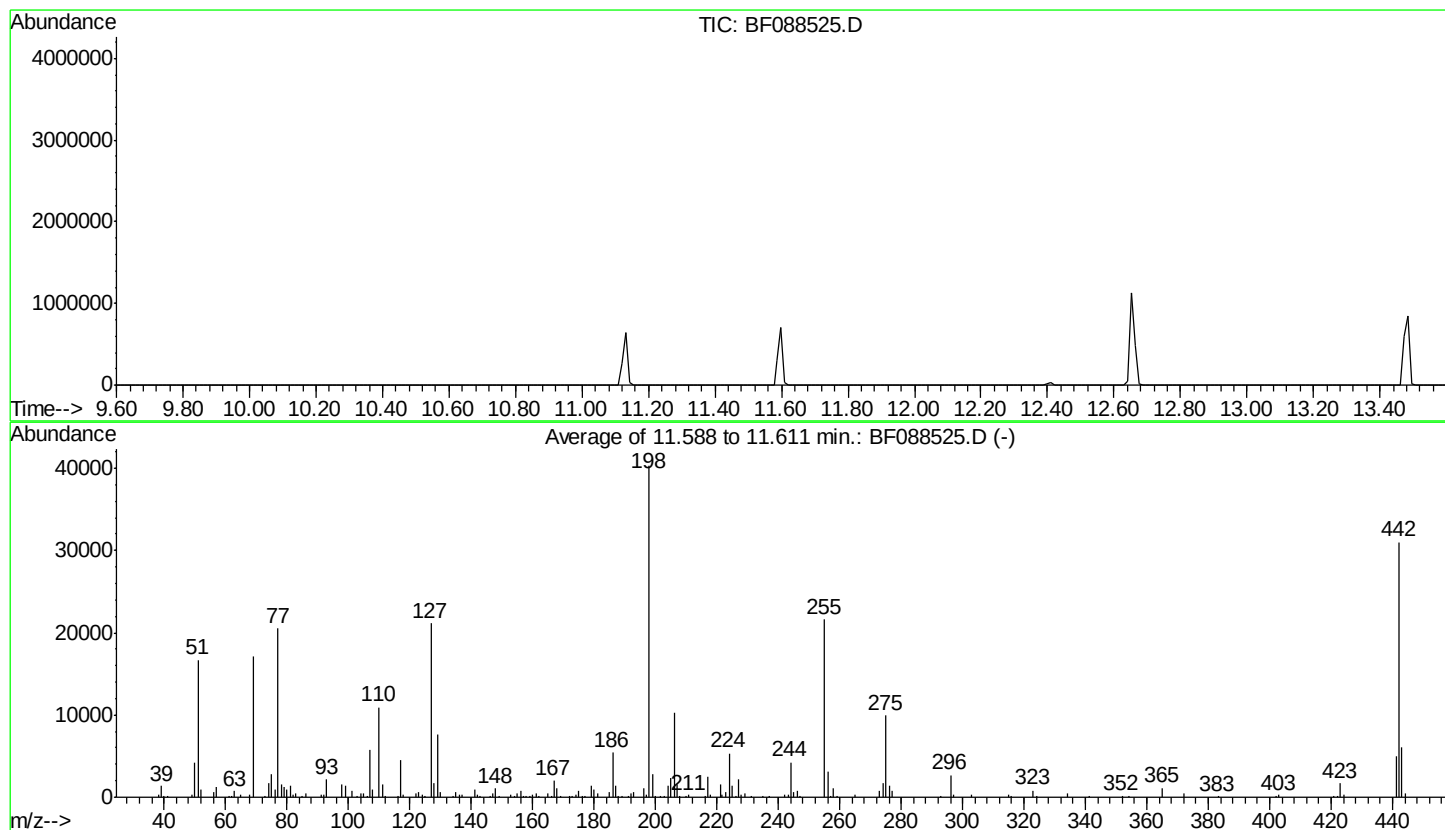

AutoFind: Scans 875, 876, 877; Background Corrected with Scan 872

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	16709	PASS
68	69	0.00	2	1.8	306	PASS
69	198	0.00	100	42.3	17050	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	21141	PASS
197	198	0.00	2	0.6	243	PASS
198	198	100	100	100.0	40319	PASS
199	198	5	9	6.8	2749	PASS
275	198	10	60	24.6	9934	PASS
365	198	1	100	2.8	1137	PASS
441	442	0.01	24	16.2	5028	PASS
442	198	50	100	76.8	30985	PASS
443	442	15	24	19.6	6083	PASS