


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063016\
 Data File : BF088539.D
 Acq On : 30 Jun 2016 20:00
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 30 18:01:55 2016

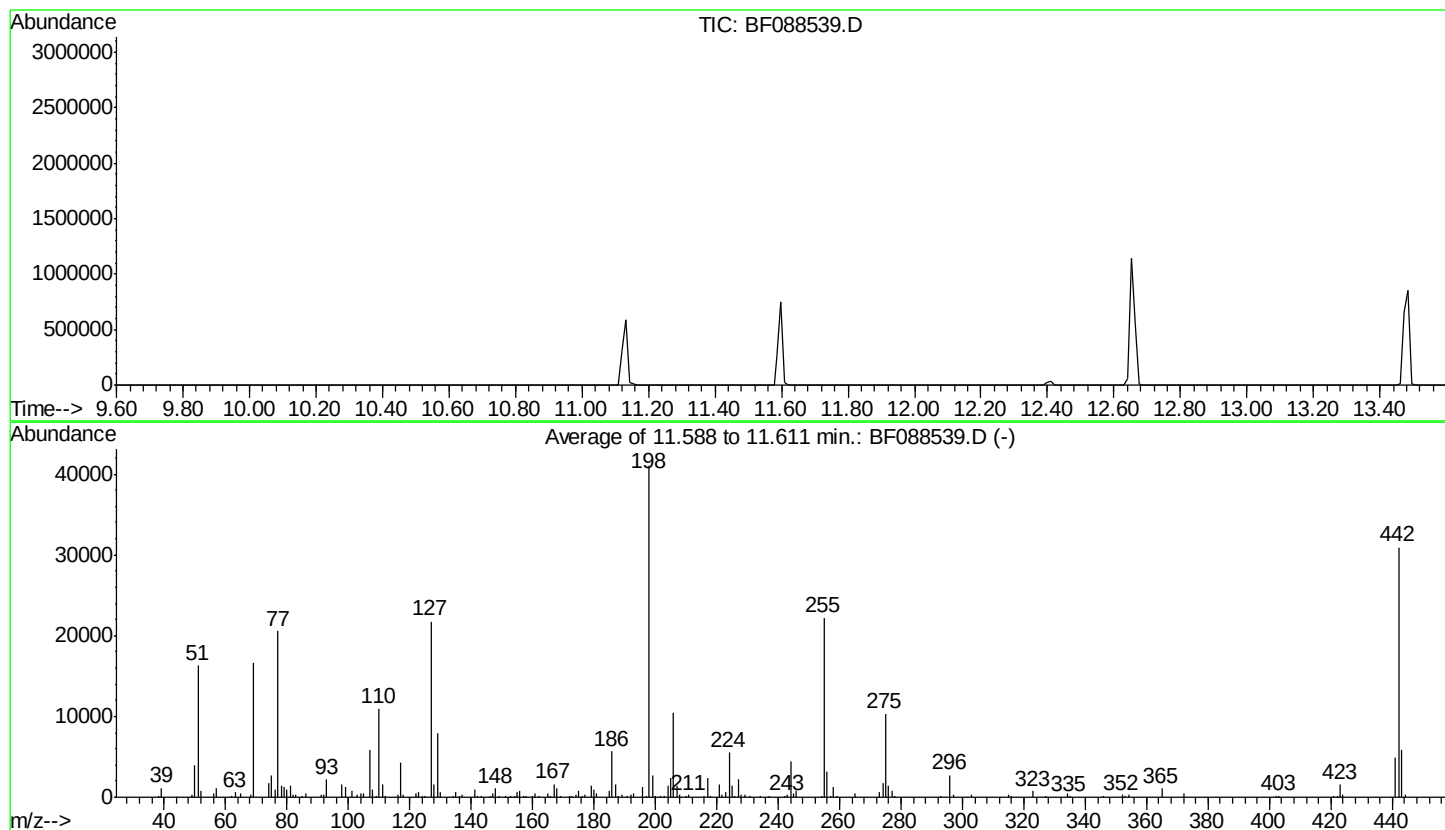

AutoFind: Scans 875, 876, 877; Background Corrected with Scan 871

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	16261	PASS
68	69	0.00	2	1.8	298	PASS
69	198	0.00	100	40.4	16578	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	21776	PASS
197	198	0.00	2	0.6	237	PASS
198	198	100	100	100.0	41047	PASS
199	198	5	9	6.5	2661	PASS
275	198	10	60	25.1	10312	PASS
365	198	1	100	2.6	1067	PASS
441	442	0.01	24	15.7	4851	PASS
442	198	50	100	75.4	30936	PASS
443	442	15	24	19.1	5896	PASS