

Data Path : Z:\HPCHEM1\BNA F\DATA\BF063017\
 Data File : BF096360.D
 Acq On : 1 Jul 2017 2:24
 Operator : SJ/MA
 Sample : I3930-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jul 01 04:05:35 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 15:41:49 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	152160	20.00	ng	-0.02
21) Naphthalene-d8	8.04	136	578740	20.00	ng	-0.02
38) Acenaphthene-d10	9.79	164	206955	20.00	ng	-0.02
63) Phenanthrene-d10	11.27	188	311439	20.00	ng	-0.01
75) Chrysene-d12	13.90	240	308336	20.00	ng	-0.01
86) Perylene-d12	15.33	264	210308	20.00	ng	-0.01

System Monitoring Compounds

5) 2-Fluorophenol	5.37	112	882526	83.56	ng	0.00
7) Phenol-d6	6.39	99	1042421	81.51	ng	0.00
23) Nitrobenzene-d5	7.32	82	589471	70.51	ng	-0.04
41) 2,4,6-Tribromophenol	10.57	330	172901	106.16	ng	-0.02
44) 2-Fluorobiphenyl	9.12	172	876412	77.55	ng	-0.03
78) Terphenyl-d14	12.86	244	636903	51.54	ng	-0.01

Target Compounds


						Qvalue
9) Benzaldehyde	6.30	77	4164	Below Cal	#	82
19) n-Nitroso-di-n-propylamine	7.32	70	77382	10.10	ng	# 87
25) Isophorone	7.32	82	587110	30.92	ng	# 67
32) Benzoic acid	7.82	122	300	8.83	ng	# 27
49) Dimethylphthalate	9.51	163	120775	8.15	ng	97
53) 2,4-Dinitrophenol	10.09	184	128	7.67	ng	# 4
56) 2,4-Dinitrotoluene	9.79	165	28047	7.22	ng	# 33
57) Fluorene	10.33	166	4007	Below Cal	#	88
64) 4,6-Dinitro-2-methylphenol	10.57	198	287	8.89	ng	# 1
66) 4-Bromophenyl-phenylether	10.57	248	9400	2.93	ng	# 1
70) Phenanthrene	11.29	178	81909	Below Cal		99
74) Fluoranthene	12.48	202	155177	8.97	ng	97
77) Pyrene	12.71	202	148245	5.85	ng	99
80) Benzo(a)anthracene	13.89	228	77179	4.11	ng	96
82) Chrysene	13.89	228	77179	3.97	ng	97
85) Indeno(1,2,3-cd)pyrene	16.70	276	38294	2.37	ng	98
87) Benzo(b)fluoranthene	14.92	252	125186	9.06	ng	# 92
88) Benzo(k)fluoranthene	14.92	252	125186	9.93	ng	# 96
89) Benzo(a)pyrene	15.26	252	55801	4.57	ng	# 88
91) Benzo(a,h,i)perylene	17.12	276	40094	4.04	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF063017\
Data File : BF096360.D
Acq On : 1 Jul 2017 2:24
Operator : SJ/MA
Sample : I3930-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 01 04:05:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 15:41:49 2017
Response via : Initial Calibration

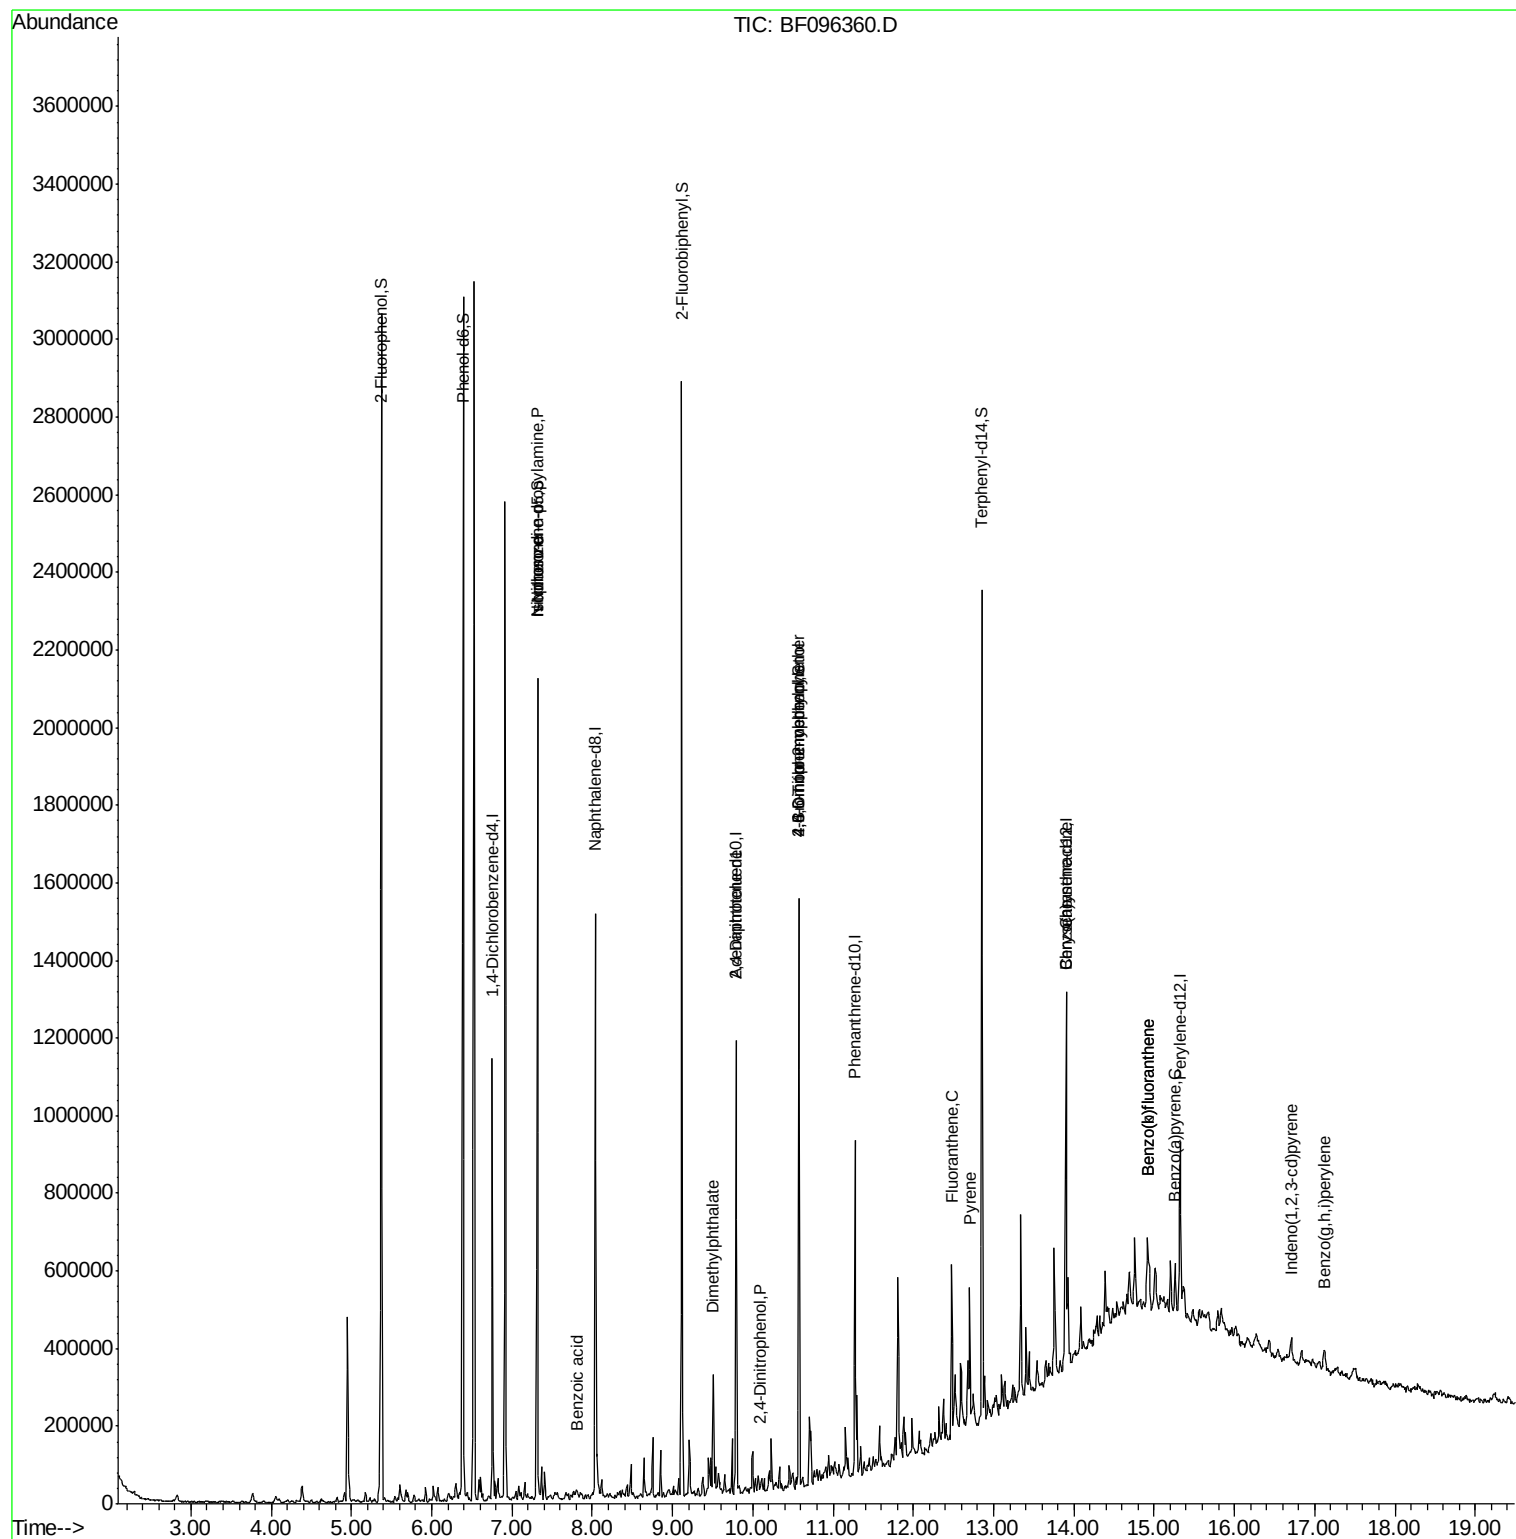

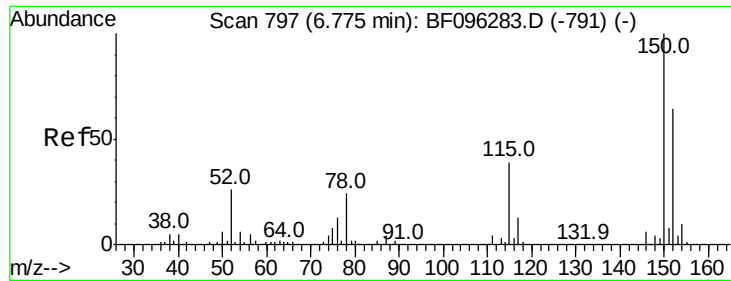


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.76 min Scan# 794
Delta R.T. -0.02 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	161.2	126.2	189.2
115	67.5	52.2	78.2

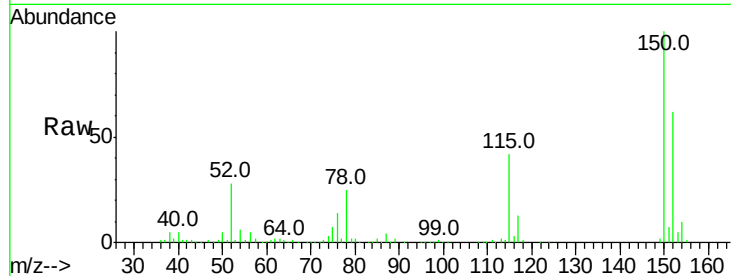


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

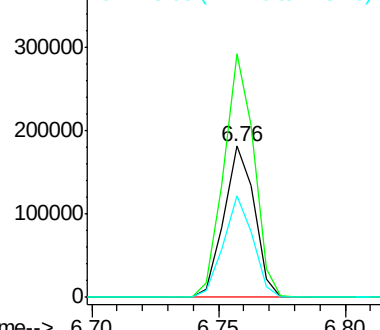



#5


2-Fluorophenol
Concen: 83.56 ng
RT: 5.37 min Scan# 559
Delta R.T. -0.01 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Tgt Ion	Ratio	Lower	Upper
112	100		
64	61.7	46.0	69.0
63	31.8	23.4	35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

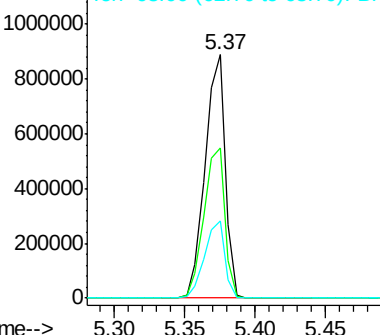

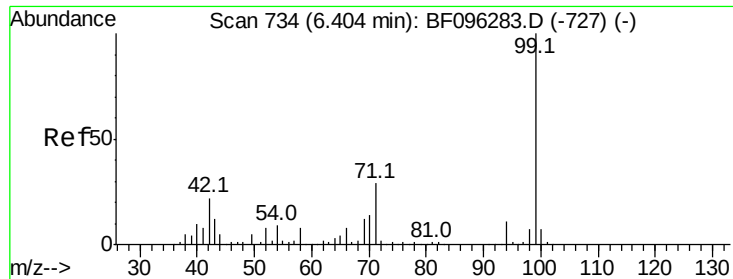

#7

Phenol-d6

Concen: 81.51 ng

RT: 6.39 min Scan# 732

Delta R.T. -0.00 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24





Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 1042421

Ion	Ratio	Lower	Upper
99	100		
42	21.1	13.5	20.3#
71	29.8	24.5	36.7

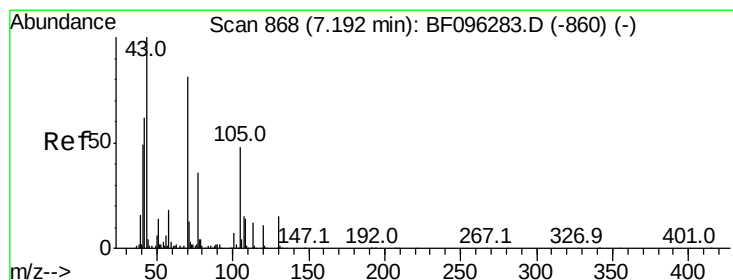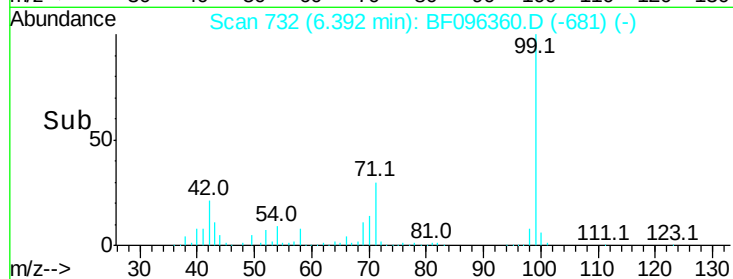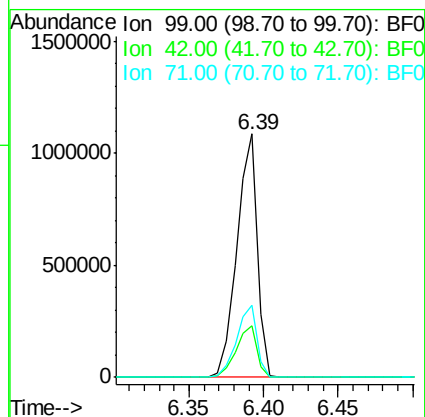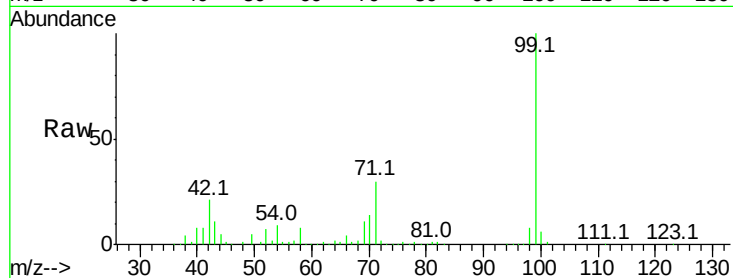

#19

n-Nitroso-di-n-propylamine

Concen: 10.10 ng

RT: 7.32 min Scan# 889




Delta R.T. 0.14 min


Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Tgt Ion: 70 Resp: 77382

Ion	Ratio	Lower	Upper
70	100		
42	61.4	47.2	70.8
101	0.0	7.2	10.8#
130	2.3	15.9	23.9#

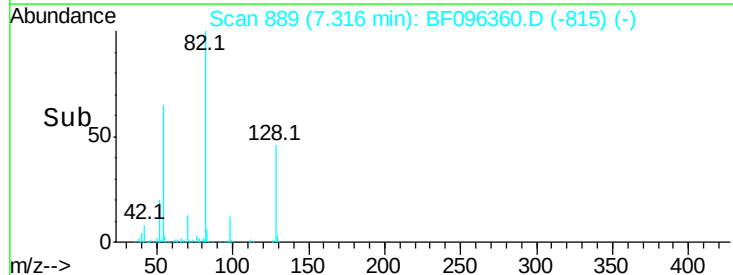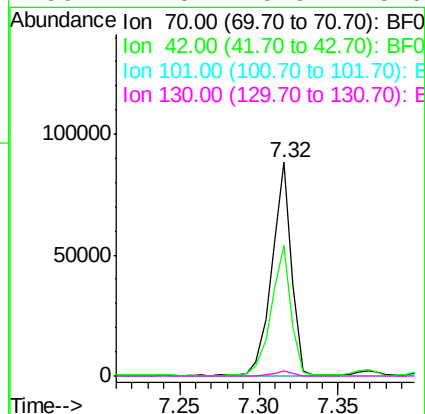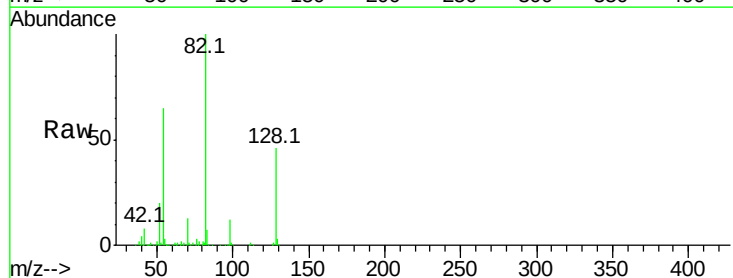



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.04 min Scan# 1012

Delta R.T. -0.02 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 578740


Ion Ratio Lower Upper

136 100

137 11.3 8.5 12.7

54 11.2 4.9 7.3#

68 6.5 4.1 6.1#




Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



Time-->



#23

Nitrobenzene-d5

Concen: 70.51 ng

RT: 7.32 min Scan# 889

Delta R.T. -0.04 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24


Tgt Ion: 82 Resp: 589471

Ion Ratio Lower Upper

82 100

128 46.1 34.0 51.0


54 65.4 42.2 63.2#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0



Time-->

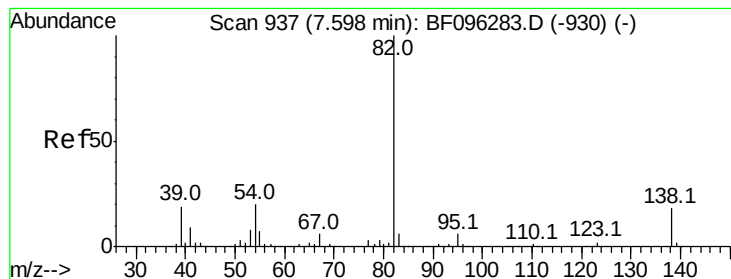

#25

Isophorone

Concen: 30.92 ng

RT: 7.32 min Scan# 889

Delta R.T. -0.28 min





Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :
BNA_F
ClientSampled :

Tot Ion: 82 Resp: 587110

Ion	Ratio	Lower	Upper
82	100		
95	0.2	5.3	7.9#
138	0.0	13.1	19.7#

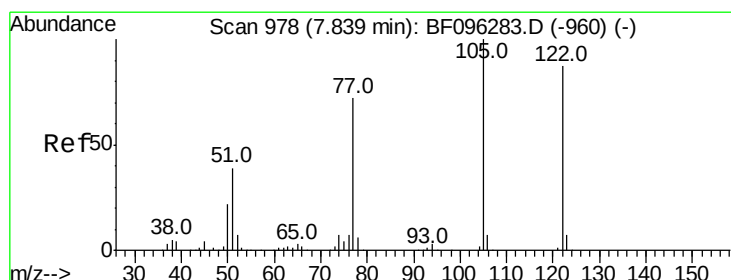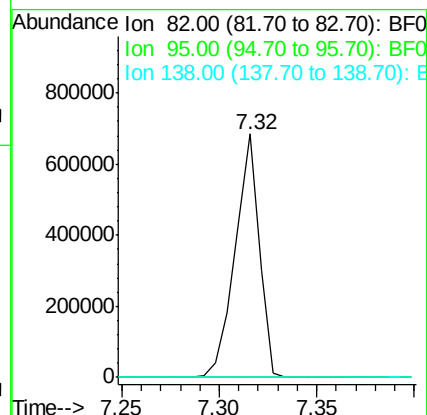

#32

Benzoic acid

Concen: 8.83 ng

RT: 7.82 min Scan# 975




Delta R.T. -0.06 min


Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Tgt Ion: 122 Resp: 300

Ion	Ratio	Lower	Upper
122	100		
105	210.0	103.3	143.3#
77	158.2	73.7	113.7#

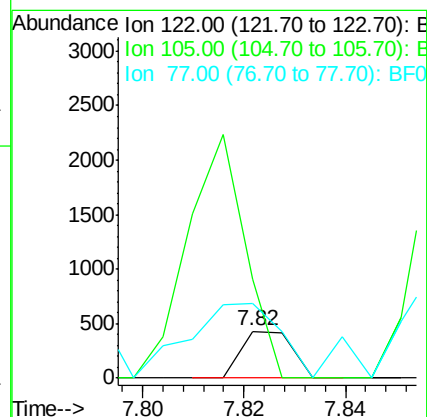

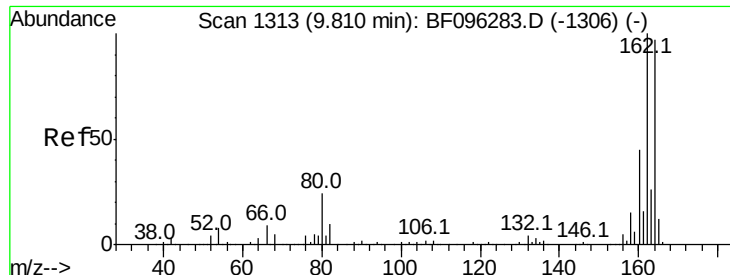

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.79 min Scan# 1310

Delta R.T. -0.02 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 206955

Ion Ratio Lower Upper

164 100

162 101.8 82.6 123.8




160 45.3 36.2 54.2

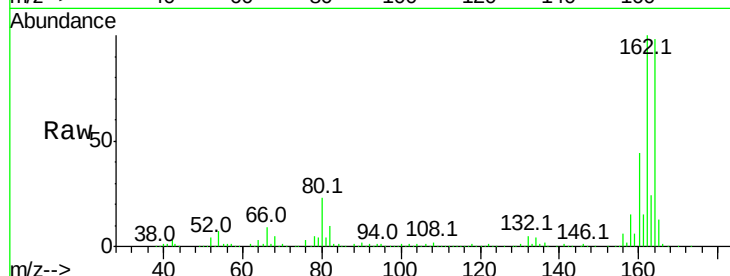

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

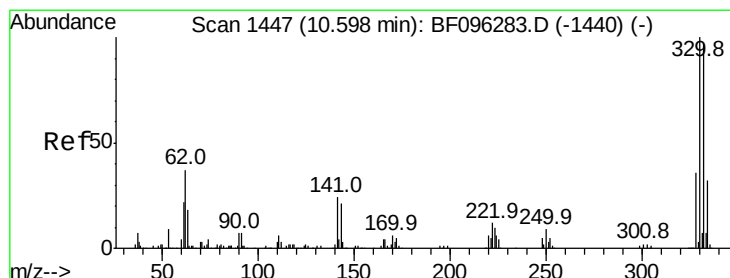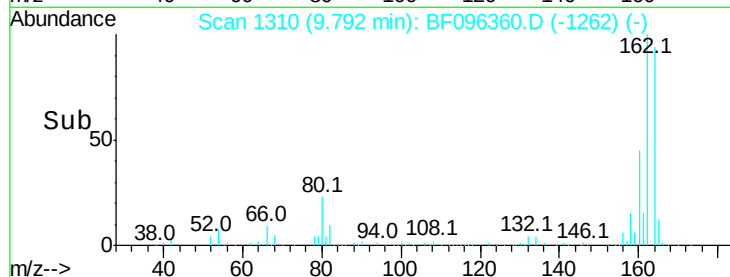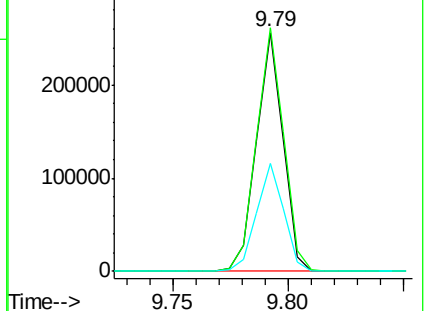

#41

2,4,6-Tribromophenol

Concen: 106.16 ng

RT: 10.57 min Scan# 1443

Delta R.T. -0.02 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24


Tgt Ion:330 Resp: 172901

Ion Ratio Lower Upper

330 100

332 95.7 76.6 115.0



141 30.7 31.4 47.2#

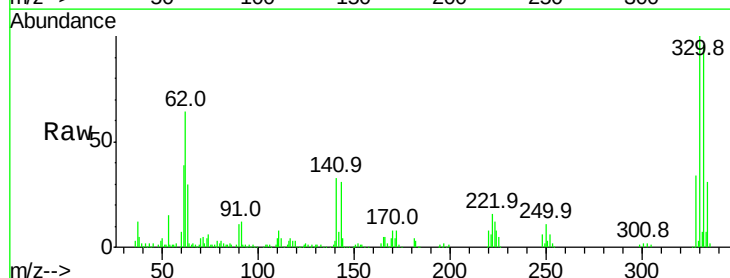


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

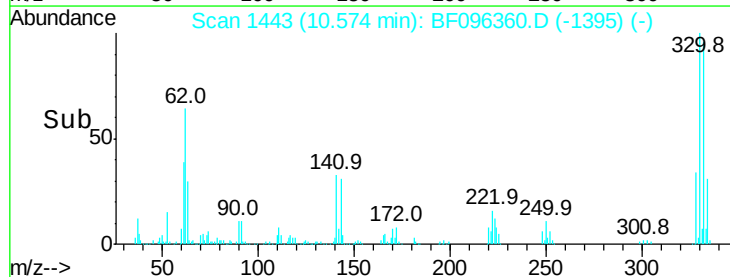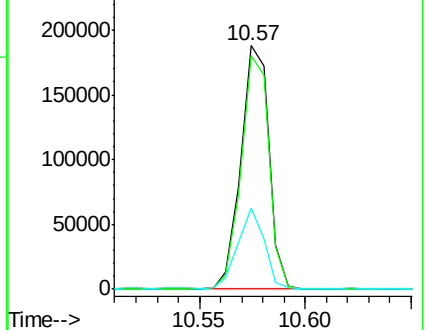


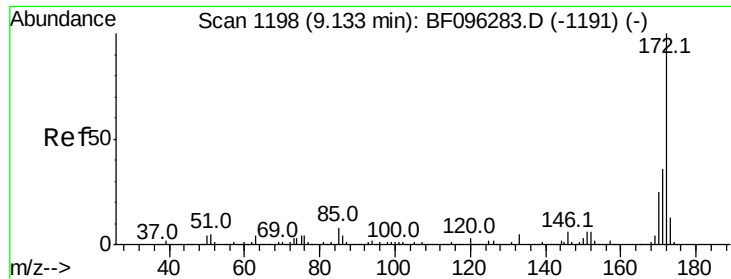




#44
2-Fluorobiphenyl
Concen: 77.55 ng
RT: 9.12 min Scan# 1195
Delta R.T. -0.03 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 876412
Ion Ratio Lower Upper
172 100
171 35.7 29.6 44.4
170 24.2 19.8 29.8




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


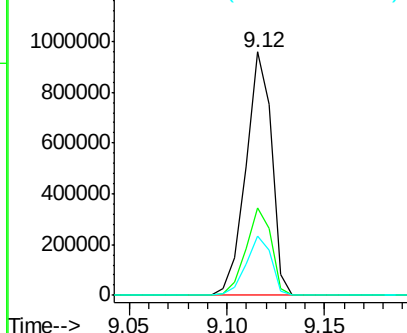



#49
Dimethylphthalate
Concen: 8.15 ng
RT: 9.51 min Scan# 1262
Delta R.T. -0.02 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Tgt Ion:163 Resp: 120775
Ion Ratio Lower Upper
163 100
194 3.3 2.6 4.0
164 9.2 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



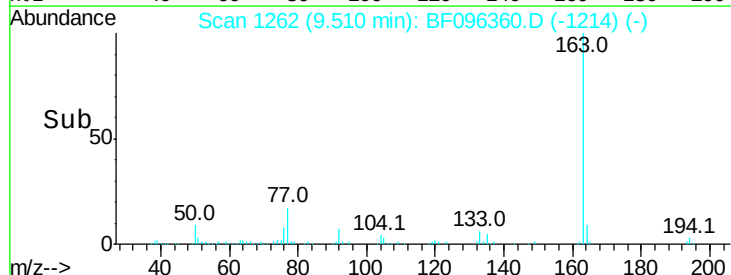
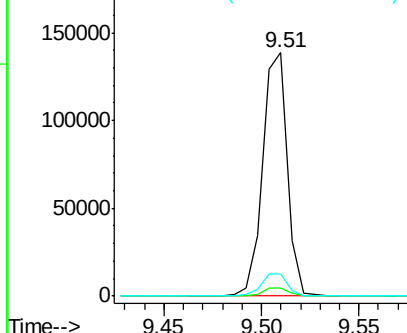


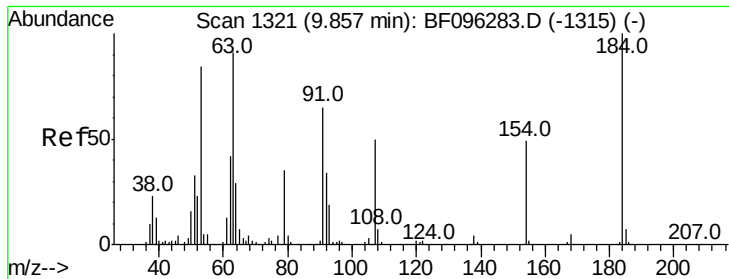

#53
2,4-Dinitrophenol
Concen: 7.67 ng
RT: 10.09 min Scan# 1361
Delta R.T. 0.22 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24




Instrument :
BNA_F
ClientSampleId :


Tot Ion:184 Resp: 128
Ion Ratio Lower Upper
184 100
63 0.0 62.7 94.1#
154 0.0 81.1 121.7#

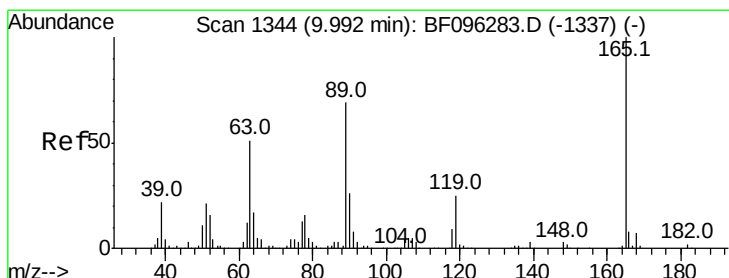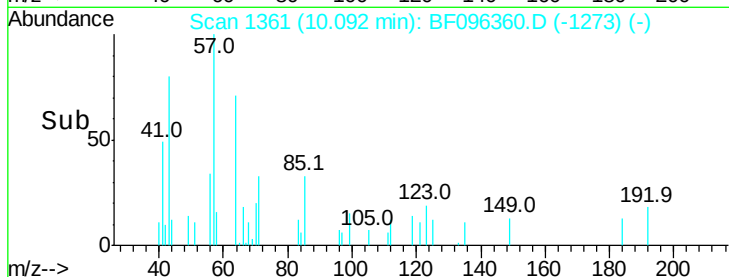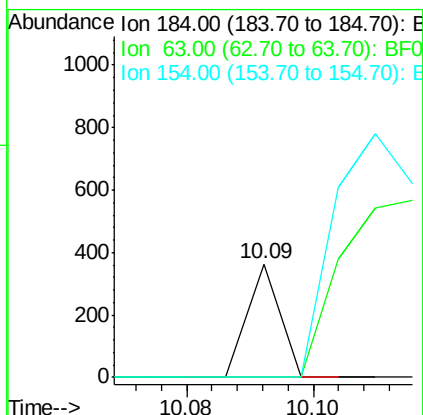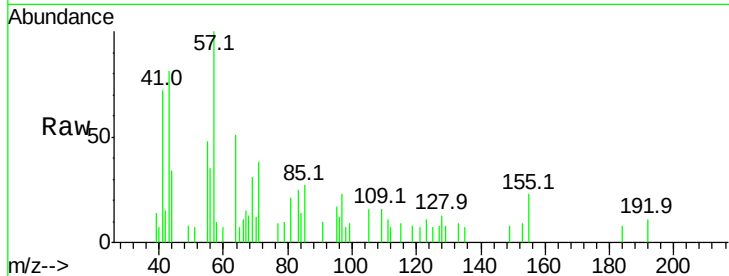

#56
2,4-Dinitrotoluene
Concen: 7.22 ng
RT: 9.79 min Scan# 1310
Delta R.T. -0.22 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Tgt Ion:165 Resp: 28047
Ion Ratio Lower Upper
165 100
63 1.5 25.4 38.0#
89 1.9 46.4 69.6#
182 0.0 1.8 2.6#


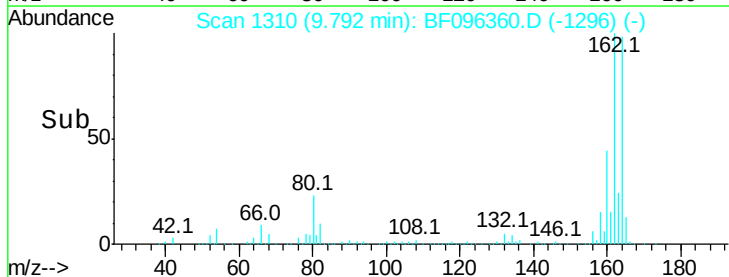
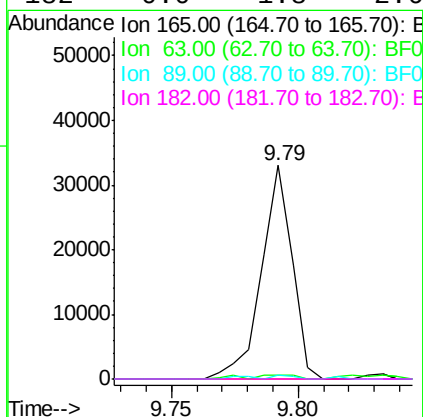
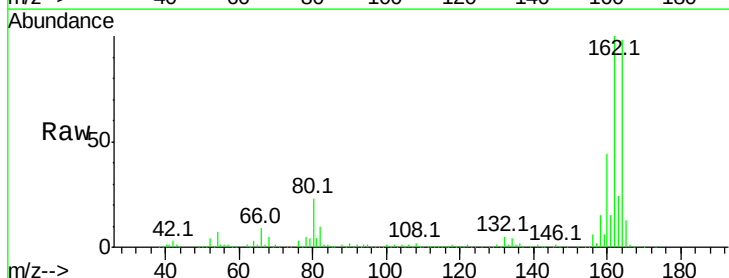




#57
Fluorene
 Concen: Below Cal
 RT: 10.33 min Scan# 1402
 Delta R.T. -0.03 min
 Lab File: BF096360.D
 Acq: 1 Jul 2017 2:24




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:166 Resp: 4007
 Ion Ratio Lower Upper
 166 100
 165 105.6 78.8 118.2
 167 33.9 10.6 16.0#

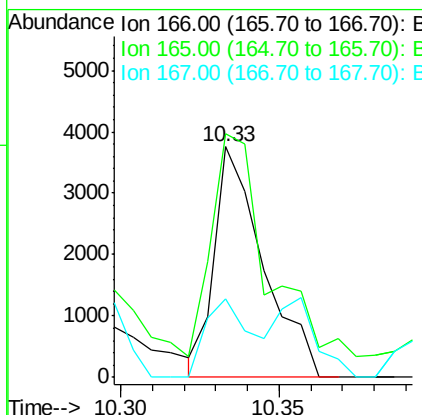

#63
Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.27 min Scan# 1562
 Delta R.T. -0.01 min
 Lab File: BF096360.D
 Acq: 1 Jul 2017 2:24

Tgt Ion:188 Resp: 311439
 Ion Ratio Lower Upper
 188 100
 94 11.8 9.4 14.2
 80 11.7 10.2 15.2

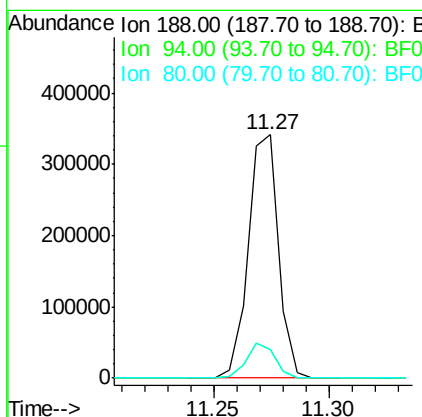

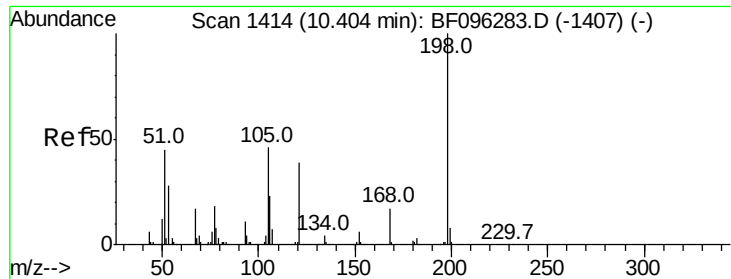

#64

4,6-Dinitro-2-methylphenol

Concen: 8.89 ng

RT: 10.57 min Scan# 1443

Delta R.T. 0.16 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :

BNA_F

ClientSampled :


Tot Ion:198 Resp: 287

Ion Ratio Lower Upper

198 100

51 375.6 53.2 93.2#




105 277.2 45.8 85.8#

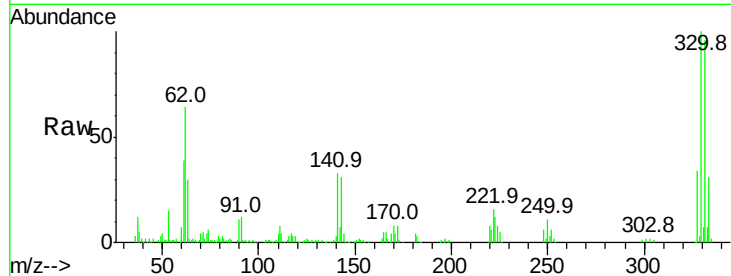

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF0

Ion 105.00 (104.70 to 105.70): E

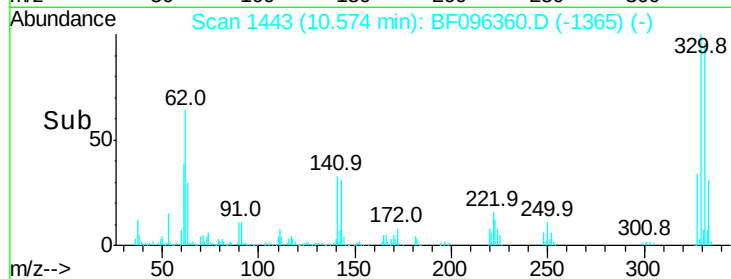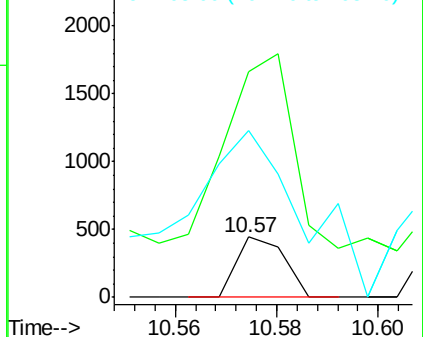

#66

4-Bromophenyl-phenylether

Concen: 2.93 ng

RT: 10.57 min Scan# 1443

Delta R.T. -0.26 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24


Tgt Ion:248 Resp: 9400

Ion Ratio Lower Upper

248 100

250 183.1 76.8 115.2#



141 576.8 68.6 103.0#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

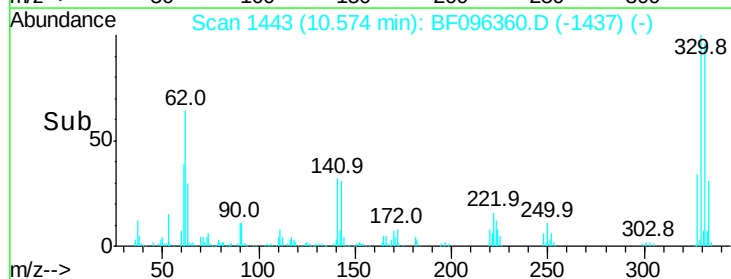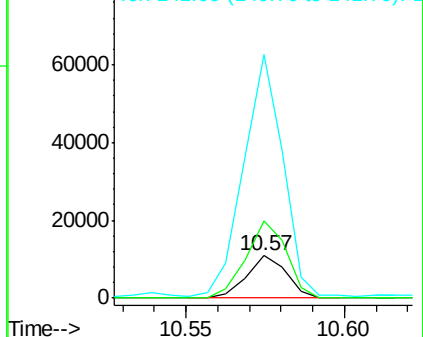

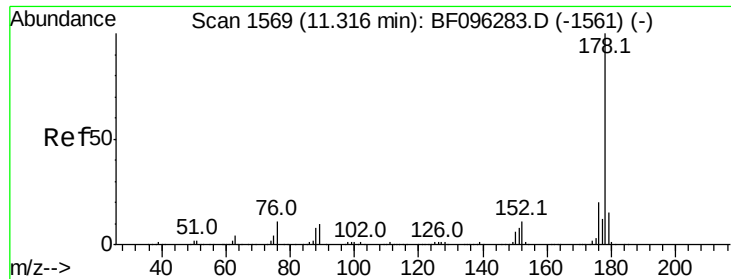

#70

Phenanthrene

Concen: Below Cal

RT: 11.29 min Scan# 1565

Delta R.T. -0.03 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :

BNA_F

ClientSampleId :


Tot Ion:178 Resp: 81909

Ion Ratio Lower Upper

178 100

176 19.4 16.2 24.4




179 15.7 12.6 19.0



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

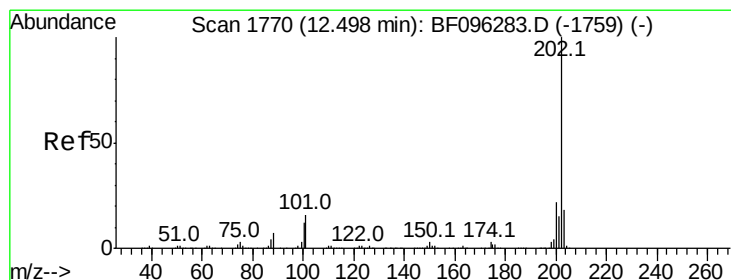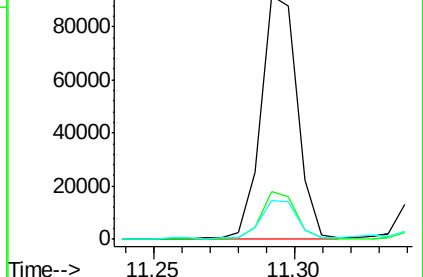

#74

Fluoranthene

Concen: 8.97 ng

RT: 12.48 min Scan# 1767

Delta R.T. -0.01 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24


Tgt Ion:202 Resp: 155177

Ion Ratio Lower Upper

202 100

101 15.6 0.0 33.2



203 17.6 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

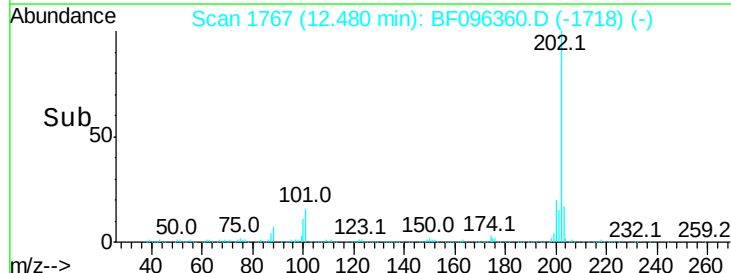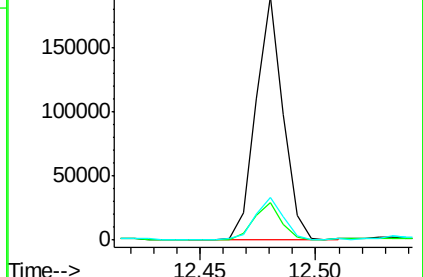

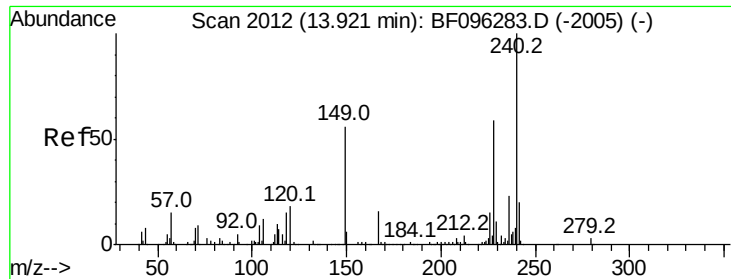

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.90 min Scan# 2009

Delta R.T. -0.01 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 308336

Ion Ratio Lower Upper

240 100

120 14.4 5.8 8.8#




236 23.8 20.5 30.7

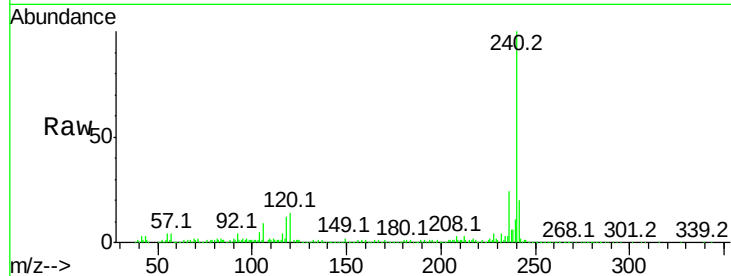

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

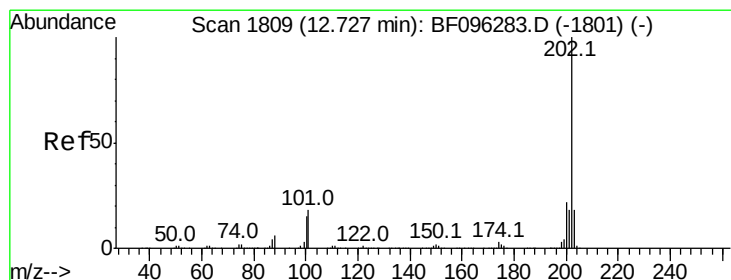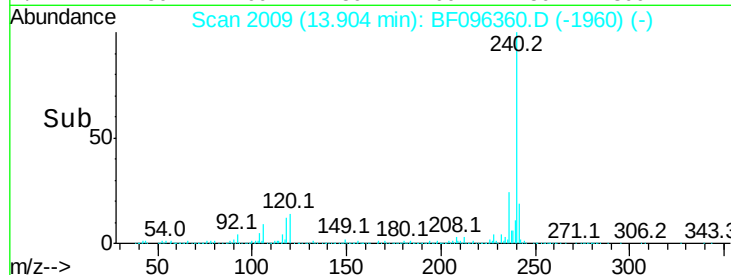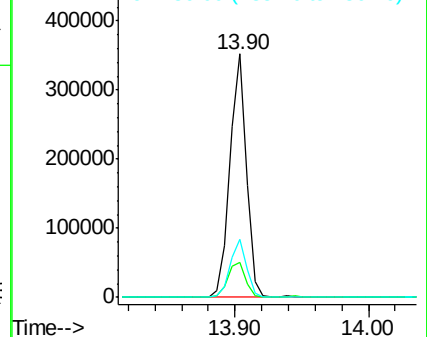

#77

Pyrene

Concen: 5.85 ng

RT: 12.71 min Scan# 1806

Delta R.T. -0.01 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24


Tgt Ion:202 Resp: 148245

Ion Ratio Lower Upper

202 100

200 22.7 17.6 26.4



203 18.5 14.4 21.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

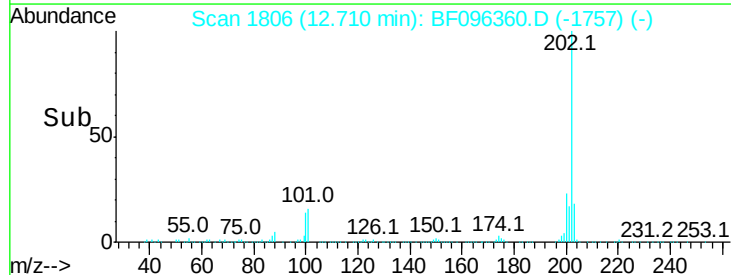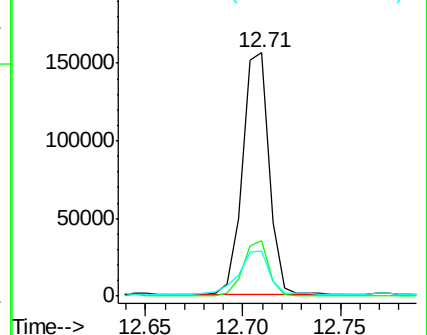



#78

Terphenyl-d14

Concen: 51.54 ng

RT: 12.86 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 636903

Ion Ratio Lower Upper

244 100

212 6.4 6.0 9.0




122 15.6 10.3 15.5#

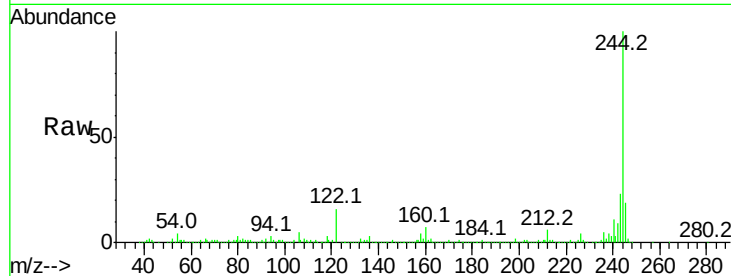

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

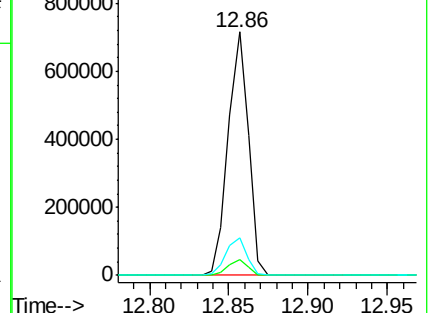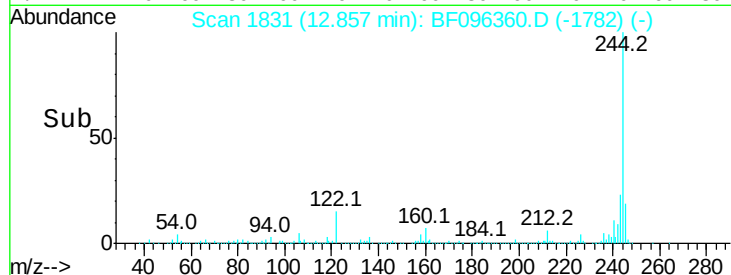

#80

Benzo(a)anthracene

Concen: 4.11 ng

RT: 13.89 min Scan# 2007

Delta R.T. -0.01 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24


Tgt Ion:228 Resp: 77179

Ion Ratio Lower Upper

228 100

226 30.4 22.6 33.8



229 21.9 16.3 24.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



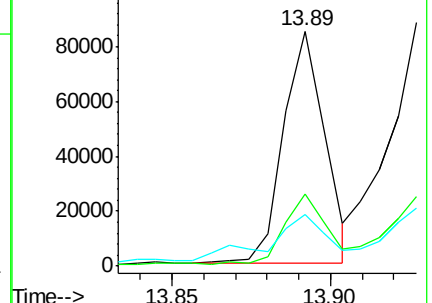



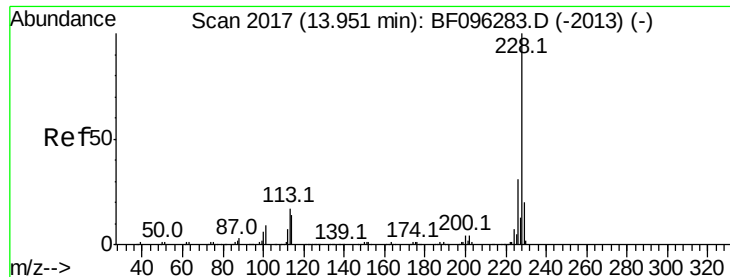

#82
Chrysene
Concen: 3.97 ng
RT: 13.89 min Scan# 2007
Delta R.T. -0.05 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 77179
Ion Ratio Lower Upper
228 100
226 30.4 24.9 37.3
229 21.9 15.8 23.6

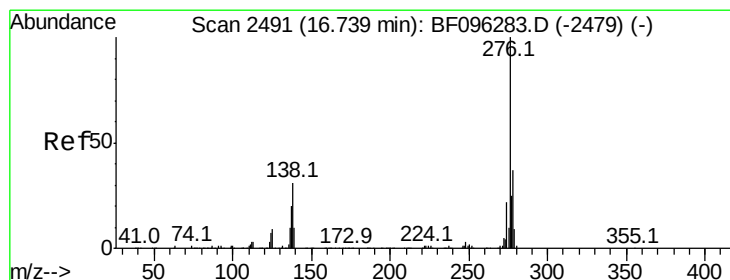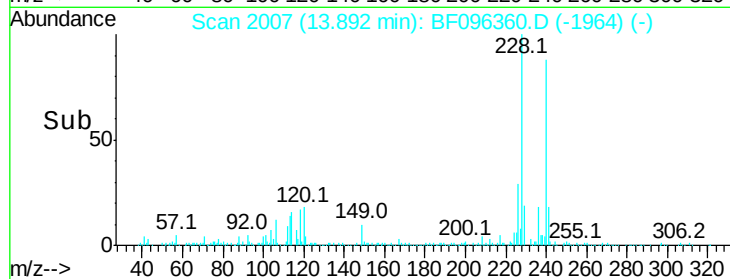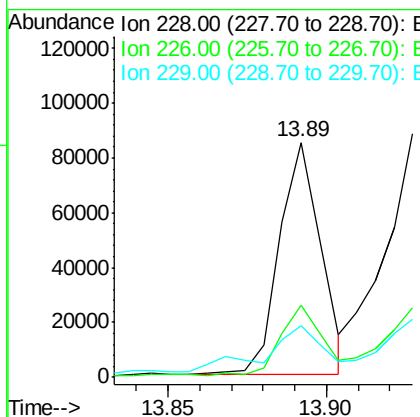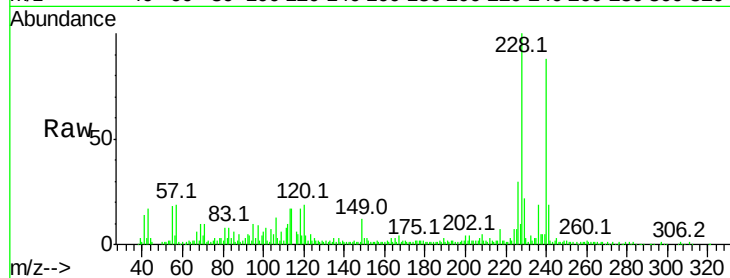

#85
Indeno(1,2,3-cd)pyrene
Concen: 2.37 ng
RT: 16.70 min Scan# 2485
Delta R.T. -0.01 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Tgt Ion:276 Resp: 38294
Ion Ratio Lower Upper
276 100
138 32.8 27.8 41.6
277 25.2 20.2 30.4


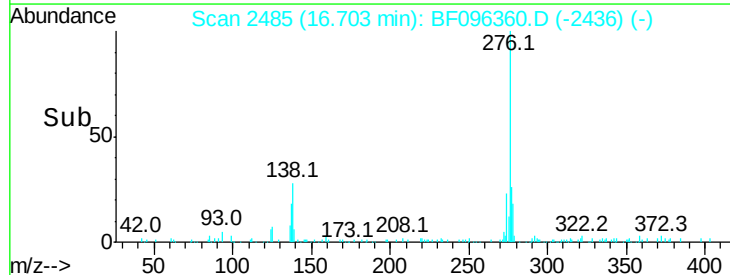
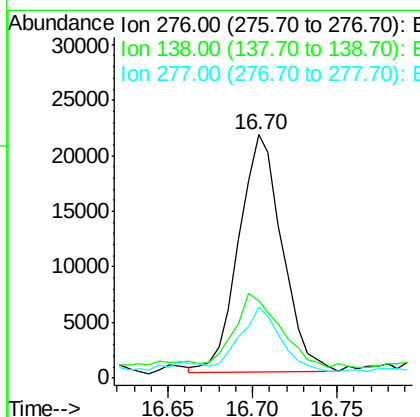
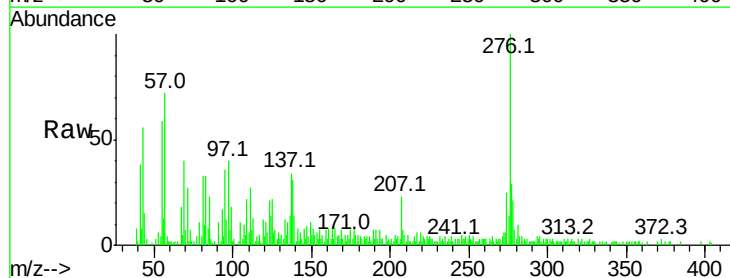




#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.33 min Scan# 2251
Delta R.T. -0.01 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.5	29.3
265	22.6	17.2	25.8

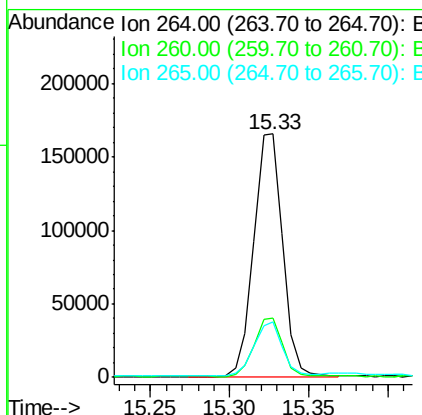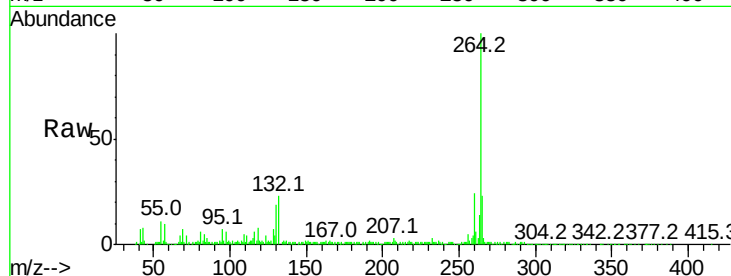

#87
Benzo(b)fluoranthene
Concen: 9.06 ng
RT: 14.92 min Scan# 2181
Delta R.T. -0.04 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.1	27.1
125	19.9	9.8	14.8

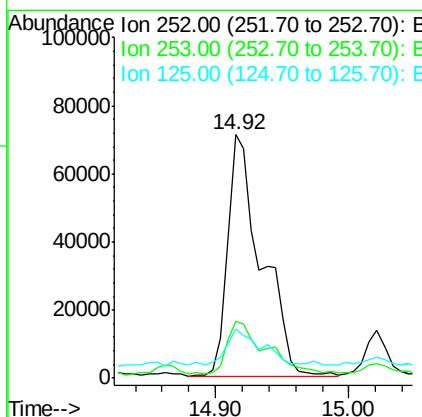


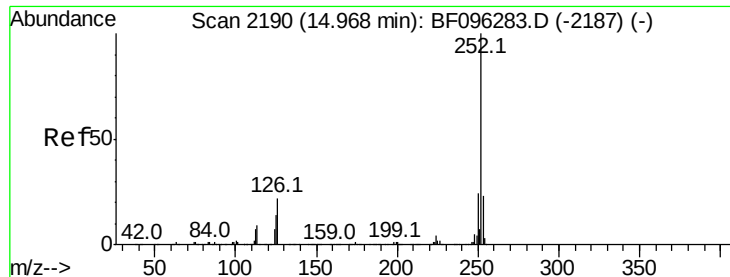




#88
Benzo(k)fluoranthene
Concen: 9.93 ng
RT: 14.92 min Scan# 2181
Delta R.T. -0.04 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.4	27.6
125	19.9	13.1	19.7

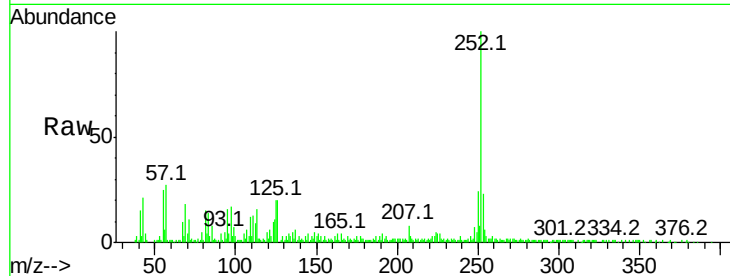


Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

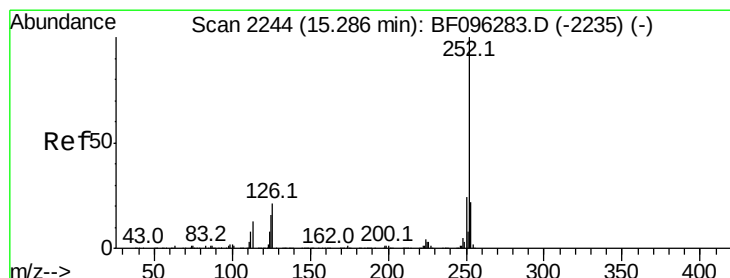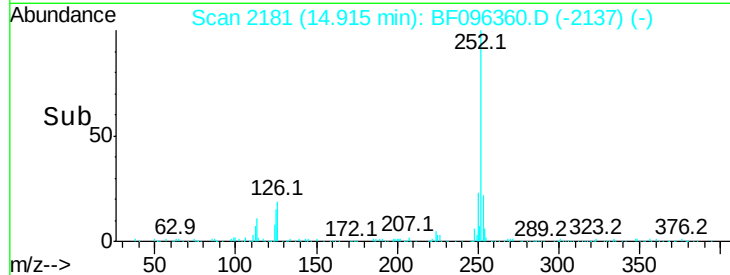
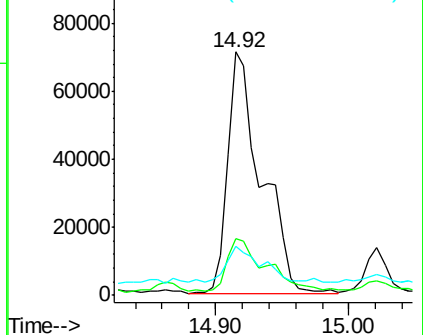



#89
Benzo(a)pyrene
Concen: 4.57 ng
RT: 15.26 min Scan# 2240
Delta R.T. -0.01 min
Lab File: BF096360.D
Acq: 1 Jul 2017 2:24

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.3	17.5	26.3
125	21.7	11.0	16.4

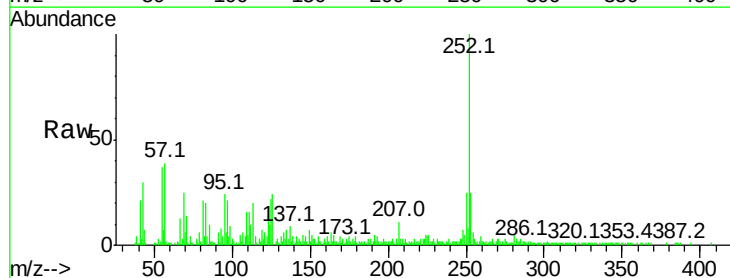

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

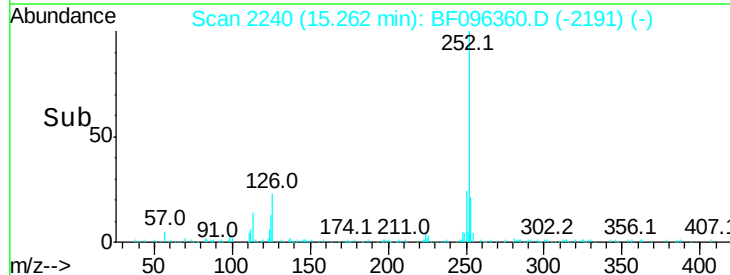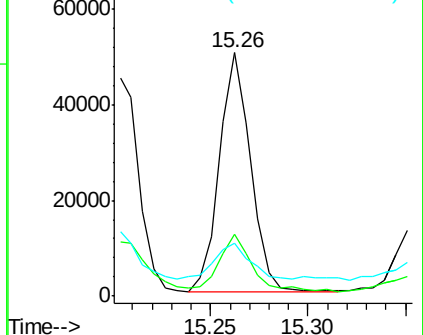

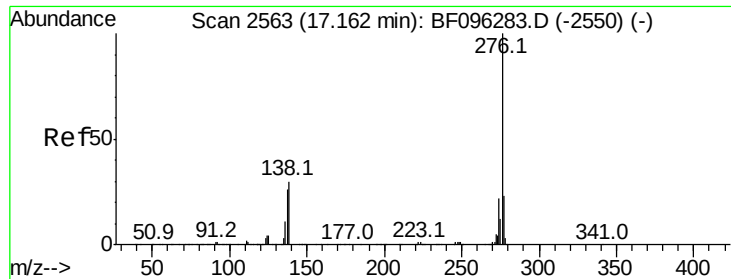

#91

Benzo(a,h,i)perylene

Concen: 4.04 ng

RT: 17.12 min Scan# 2556

Delta R.T. -0.01 min

Lab File: BF096360.D

Acq: 1 Jul 2017 2:24

Instrument :

BNA_F

ClientSampleId :


Tot Ion:276 Resp: 40094

Ion Ratio Lower Upper

276 100

277 24.9 18.6 28.0

138 34.8 25.4 38.0

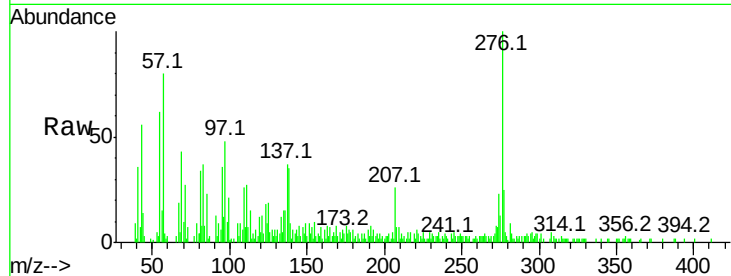

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

