

Data Path : Z:\HPCHEM1\BNA F\DATA\BF063017\
 Data File : BF096330.D
 Acq On : 30 Jun 2017 11:55
 Operator : SJ/MA
 Sample : I3883-07 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G42-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.951	484	487	493	rBV	32302	36201	2.89%	0.451%
2	5.369	554	558	562	rBV	280464	242781	19.35%	3.021%
3	6.387	728	731	738	rVB	300233	254261	20.27%	3.164%
4	6.534	752	756	760	rBV	300901	250693	19.98%	3.120%
5	6.769	792	796	800	rBV	1138350	896012	71.42%	11.151%
6	6.922	819	822	826	rVB	212518	185565	14.79%	2.309%
7	7.322	886	890	893	rBV	194461	150222	11.97%	1.870%
8	8.051	1010	1014	1017	rBV	1534375	1221074	97.32%	15.197%
9	9.128	1193	1197	1200	rBV	321282	265291	21.14%	3.302%
10	9.516	1260	1263	1267	rBV	48636	40187	3.20%	0.500%
11	9.804	1308	1312	1316	rBV2	1467907	1254640	100.00%	15.614%
12	10.586	1442	1445	1448	rBV	152511	132779	10.58%	1.652%
13	11.039	1518	1522	1526	rVB	35544	36257	2.89%	0.451%
14	11.286	1560	1564	1567	rBV	1216519	1083102	86.33%	13.479%
15	11.516	1598	1603	1605	rBV5	10797	17092	1.36%	0.213%
16	11.816	1651	1654	1657	rBV3	26321	24265	1.93%	0.302%
17	11.851	1657	1660	1663	rVV	56579	44809	3.57%	0.558%
18	11.886	1663	1666	1670	rVB4	17850	23482	1.87%	0.292%
19	12.492	1766	1769	1772	rVB	56367	45536	3.63%	0.567%
20	12.721	1805	1808	1810	rBV	35115	29192	2.33%	0.363%
21	12.863	1829	1832	1836	rBV	231313	200032	15.94%	2.489%
22	13.916	2007	2011	2014	rBV	975648	902024	71.90%	11.226%
23	15.345	2250	2254	2258	rVB	610955	699706	55.77%	8.708%


Sum of corrected areas: 8035203

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096330.D
Acq On : 30 Jun 2017 11:55
Operator : SJ/MA
Sample : I3883-07 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G42-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

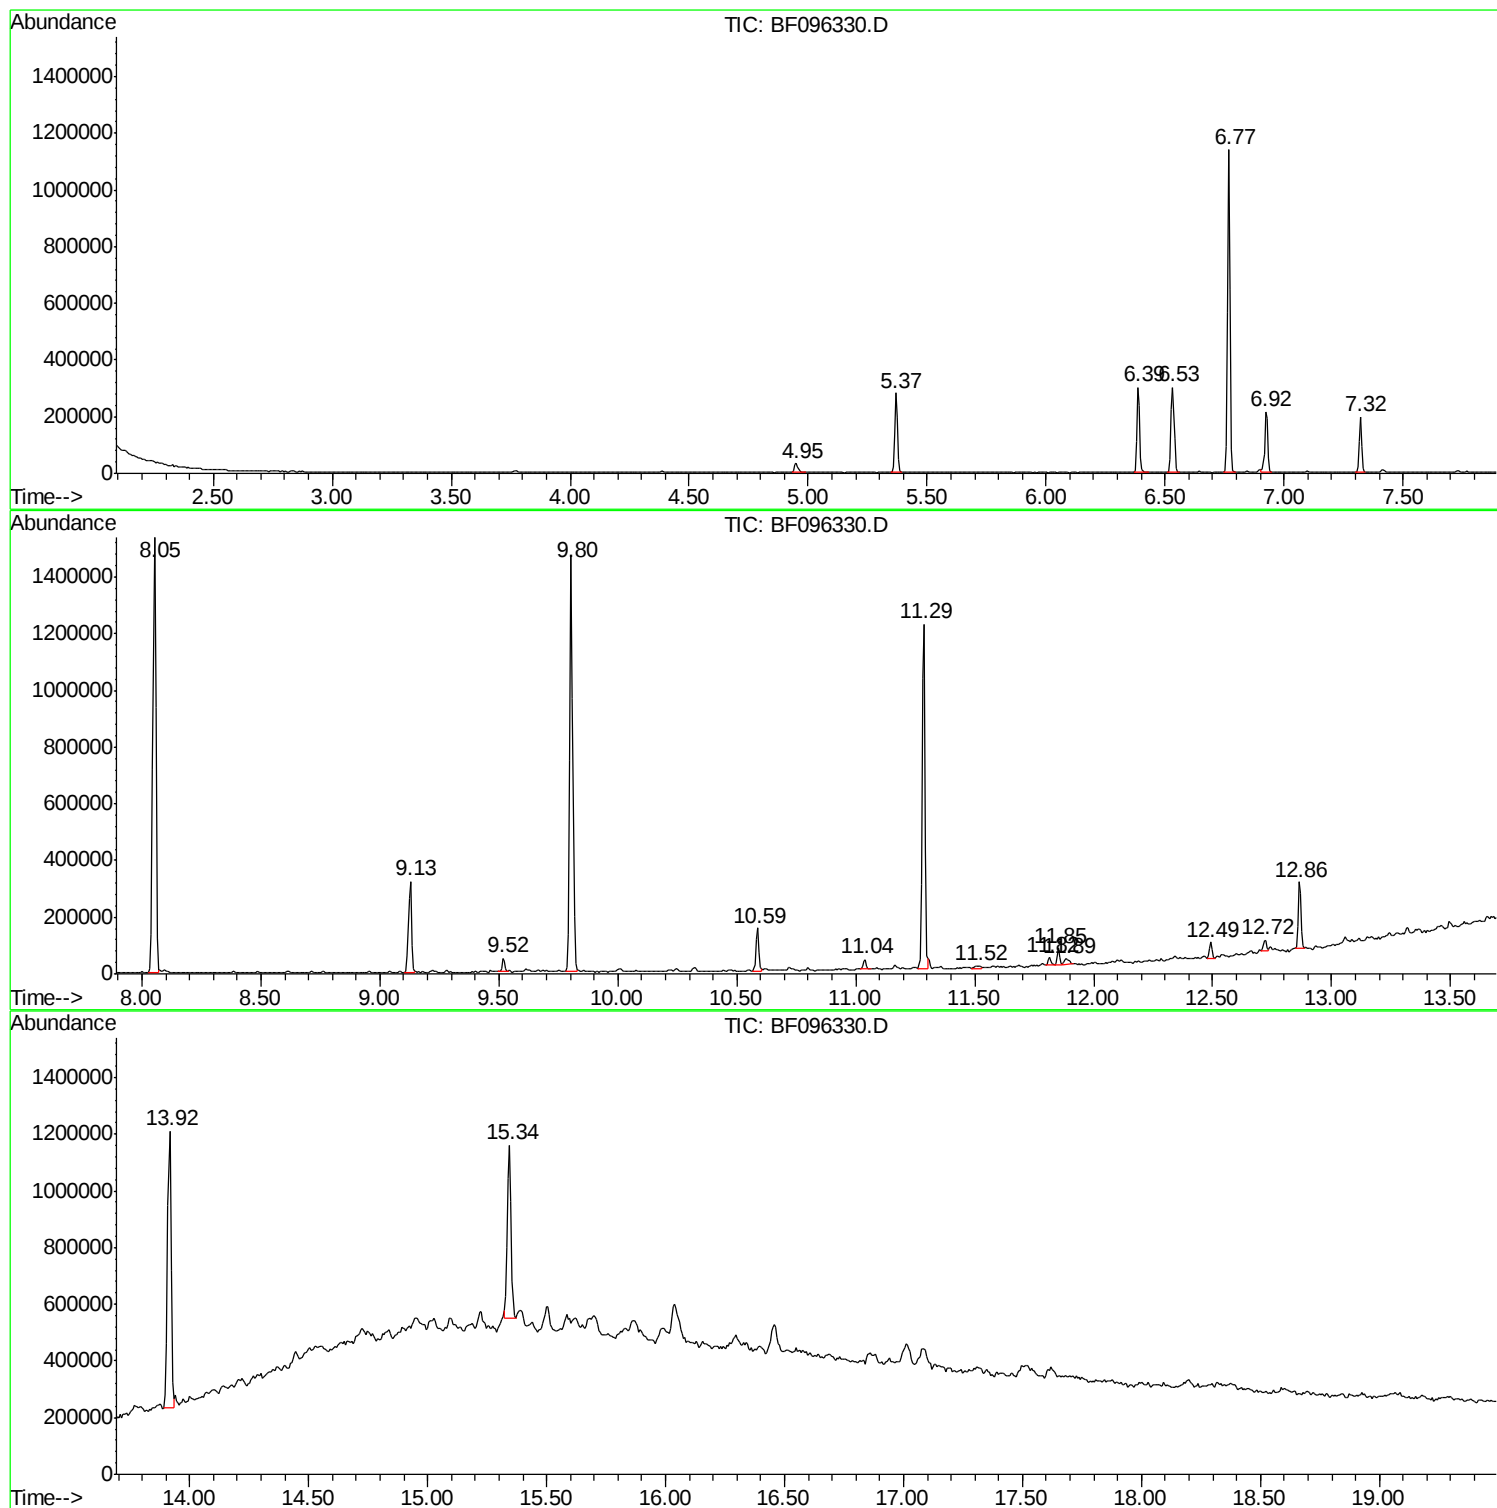

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096330.D
Acq On : 30 Jun 2017 11:55
Operator : SJ/MA
Sample : I3883-07 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G42-0-1.5










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.53	5.60 ng	250693	1,4-Dichlorobenzene-d4	6.77

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3			5-Aminoindole	132	C8H8N2	005192-03-0	12
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

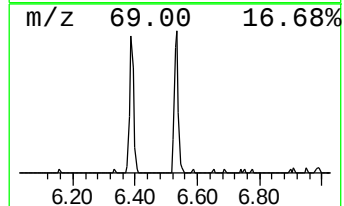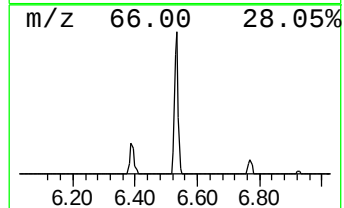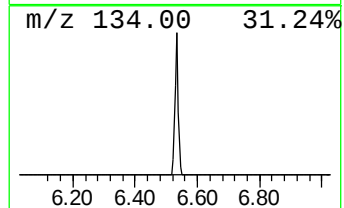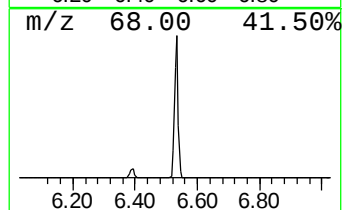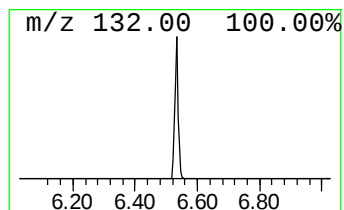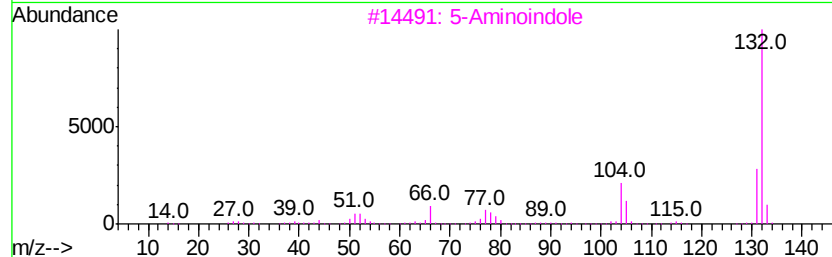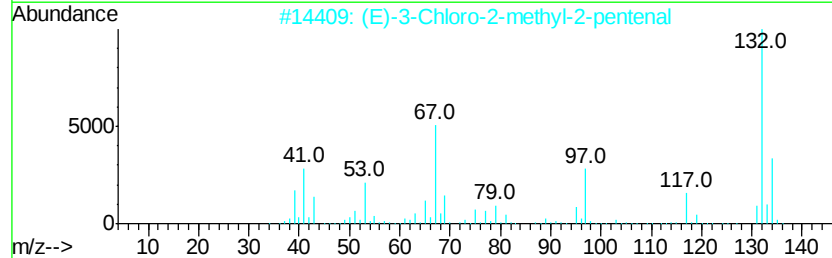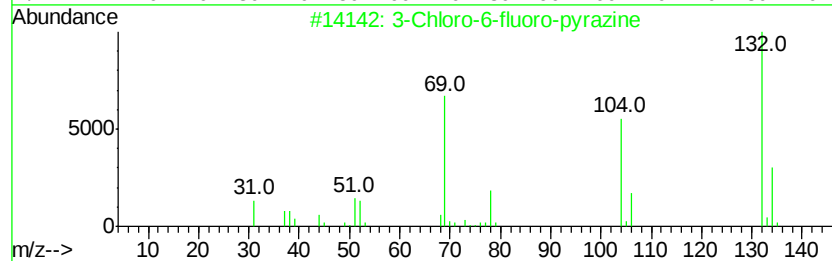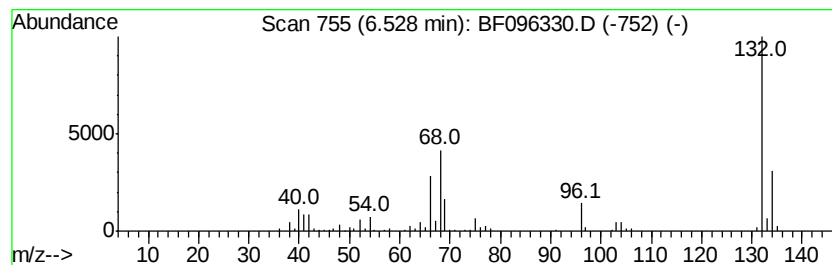

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096330.D
Acq On : 30 Jun 2017 11:55
Operator : SJ/MA
Sample : I3883-07 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G42-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.53	6.53	5.6	ng	250693	1	6.77	896012	20.0