

Data Path : Z:\HPCHEM1\BNA F\DATA\BF063017\
 Data File : BF096331.D
 Acq On : 30 Jun 2017 12:23
 Operator : SJ/MA
 Sample : I3883-08 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G42-1.5-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.393	387	392	401	rVB8	6468	14247	1.16%	0.179%
2	4.951	484	487	495	rBV2	29737	40972	3.34%	0.515%
3	5.375	555	559	562	rVB	242657	210217	17.15%	2.640%
4	6.392	728	732	737	rBV	250712	215792	17.60%	2.710%
5	6.534	752	756	764	rBV	279802	226759	18.50%	2.848%
6	6.769	792	796	800	rBV	1106638	913210	74.49%	11.468%
7	6.928	819	823	826	rBV	181330	154743	12.62%	1.943%
8	7.322	885	890	895	rBV	166132	134768	10.99%	1.692%
9	8.051	1010	1014	1018	rBV	1491389	1225930	100.00%	15.396%
10	9.128	1193	1197	1200	rBV	279481	219507	17.91%	2.757%
11	9.216	1209	1212	1216	rBV3	12629	15596	1.27%	0.196%
12	9.522	1260	1264	1266	rBV	38797	32604	2.66%	0.409%
13	9.663	1284	1288	1291	rBV	16064	15510	1.27%	0.195%
14	9.804	1308	1312	1316	rBV	1333144	1156965	94.37%	14.530%
15	10.586	1441	1445	1448	rBV	118778	101834	8.31%	1.279%
16	10.722	1465	1468	1469	rBV3	14486	15866	1.29%	0.199%
17	10.733	1469	1470	1474	rVB	23466	21240	1.73%	0.267%
18	11.033	1518	1521	1528	rBV7	21618	28769	2.35%	0.361%
19	11.169	1541	1544	1546	rBV3	13920	15374	1.25%	0.193%
20	11.198	1546	1549	1552	rVB2	19620	17799	1.45%	0.224%
21	11.286	1560	1564	1567	rBV	1023961	908112	74.08%	11.404%
22	11.357	1571	1576	1578	rVB	20492	18087	1.48%	0.227%
23	11.816	1651	1654	1656	rVB2	26572	21479	1.75%	0.270%
24	11.892	1663	1667	1670	rBV2	22114	32944	2.69%	0.414%
25	12.280	1728	1733	1738	rBV9	19773	35810	2.92%	0.450%
26	12.333	1740	1742	1746	rVV2	25862	28419	2.32%	0.357%
27	12.410	1754	1755	1757	rBV	16699	14513	1.18%	0.182%
28	12.492	1766	1769	1772	rVB	156637	128467	10.48%	1.613%
29	12.721	1803	1808	1811	rBV	121407	137362	11.20%	1.725%
30	12.839	1826	1828	1830	rBV2	19297	17606	1.44%	0.221%
31	12.863	1830	1832	1837	rVB	170346	172038	14.03%	2.161%
32	13.916	2007	2011	2014	rBV	1028480	980843	80.01%	12.318%
33	15.345	2250	2254	2258	rVB	573019	689471	56.24%	8.659%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF063017\
Data File : BF096331.D
Acq On : 30 Jun 2017 12:23
Operator : SJ/MA
Sample : I3883-08 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G42-1.5-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 7962853

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096331.D
Acq On : 30 Jun 2017 12:23
Operator : SJ/MA
Sample : I3883-08 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G42-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

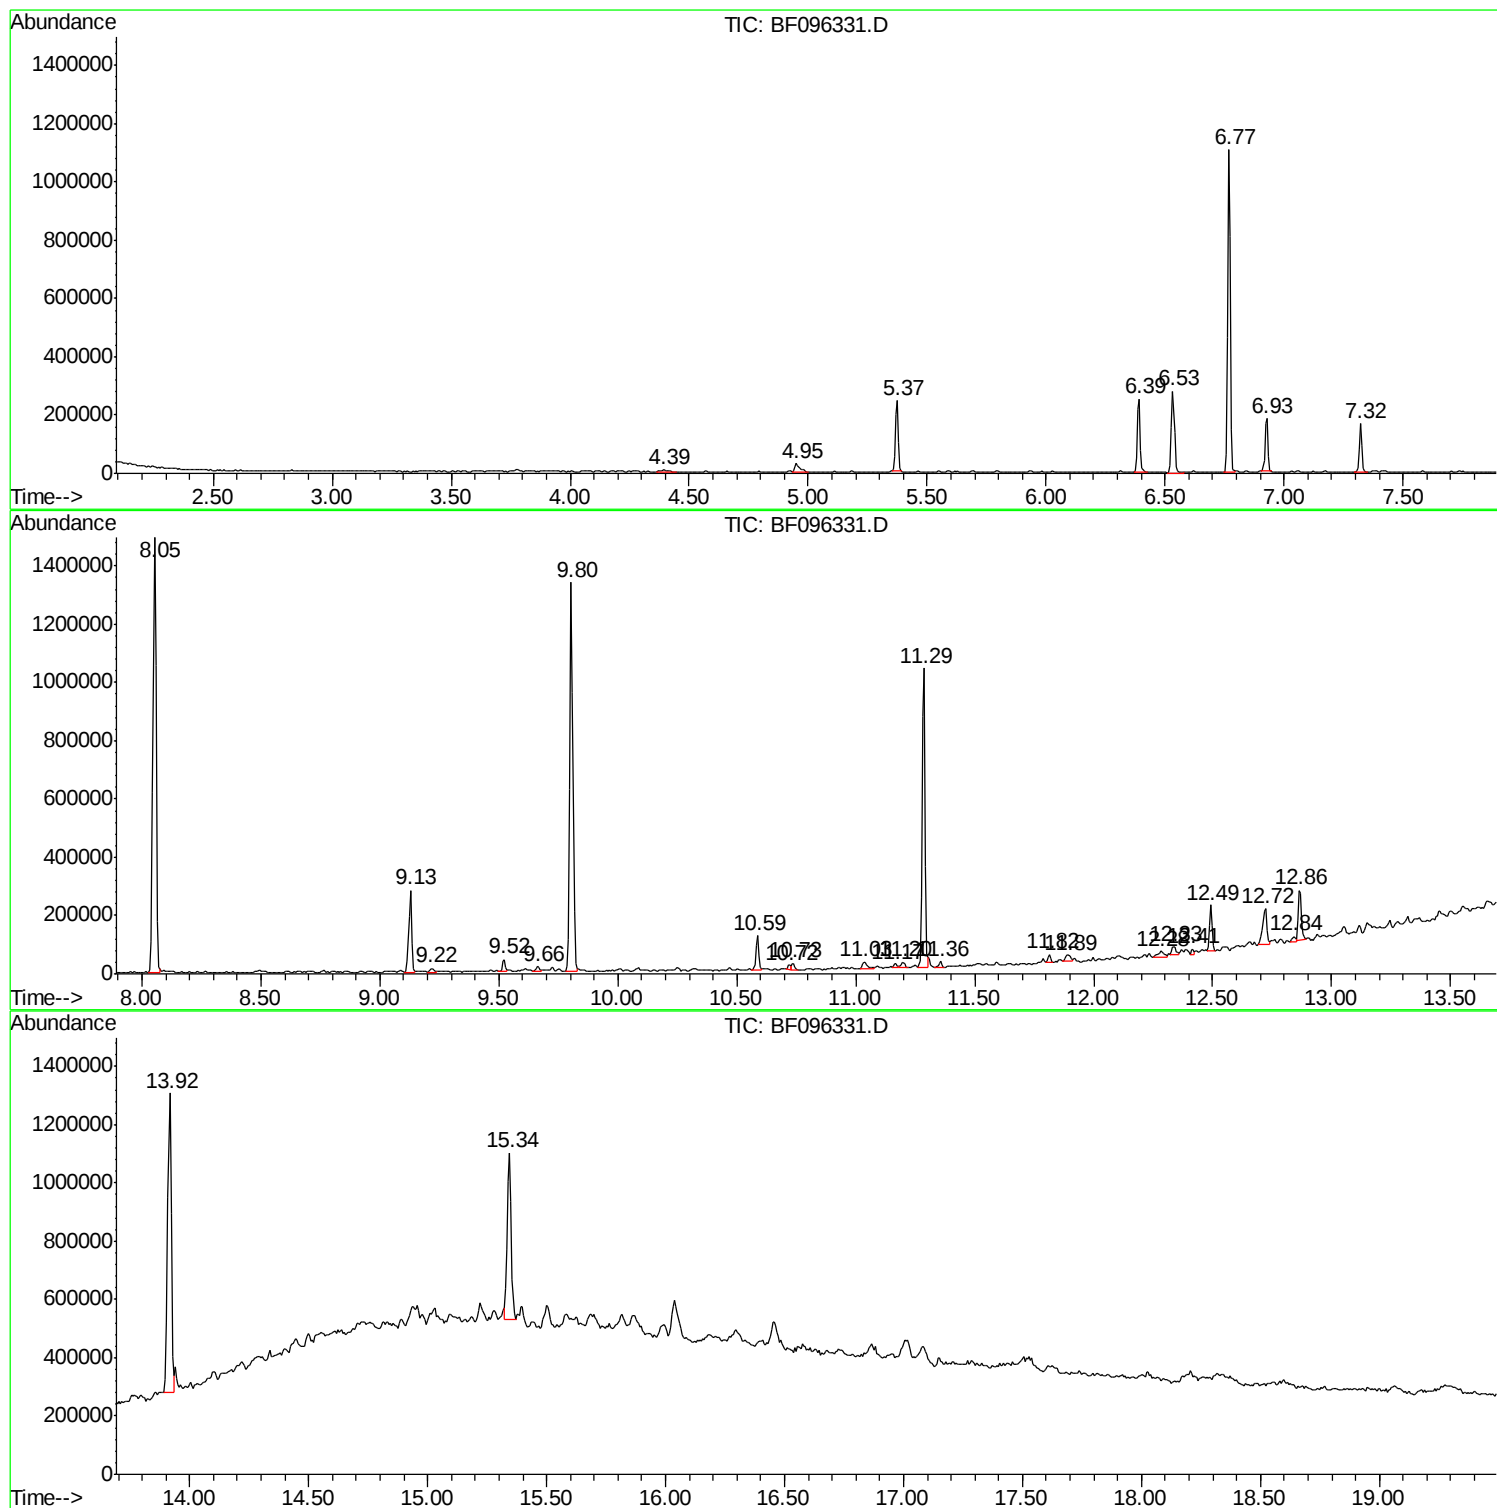

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096331.D
Acq On : 30 Jun 2017 12:23
Operator : SJ/MA
Sample : I3883-08 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G42-1.5-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.53	4.97 ng	226759	1,4-Dichlorobenzene-d4	6.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Amphetaminil	250	C17H18N2	017590-01-1	10
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

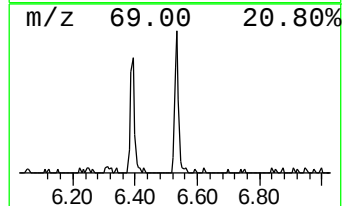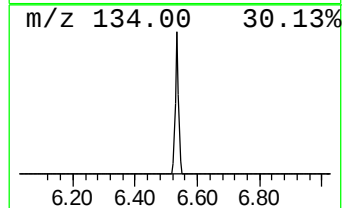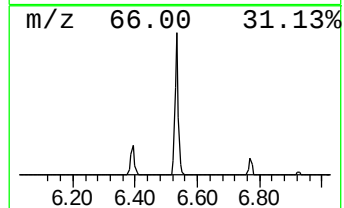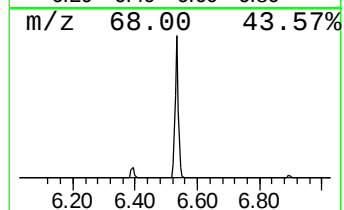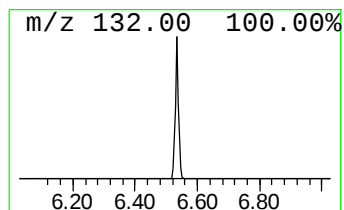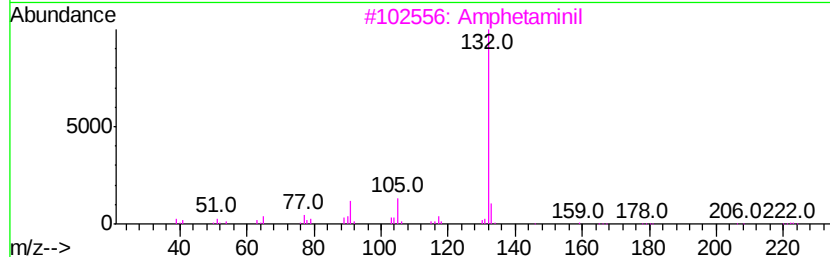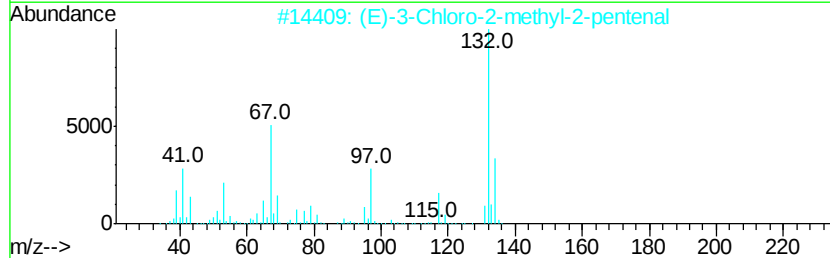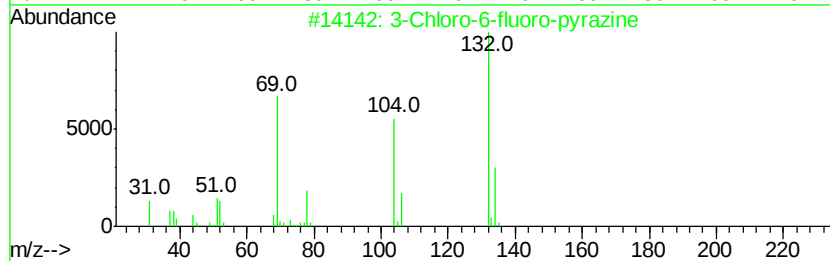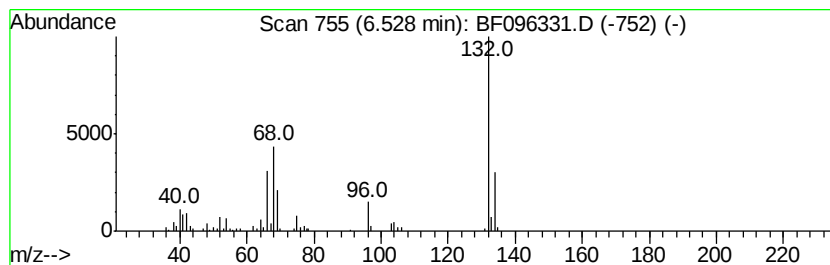

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096331.D
Acq On : 30 Jun 2017 12:23
Operator : SJ/MA
Sample : I3883-08 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G42-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.53	6.53	5.0	ng	226759	1	6.77	913210	20.0