

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
 Data File : BF096341.D
 Acq On : 30 Jun 2017 17:04
 Operator : SJ/MA
 Sample : I3882-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G51-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.951	484	487	496	rVB	41579	44290	3.85%	0.634%
2	5.375	556	559	566	rVB	263312	232097	20.17%	3.325%
3	6.392	729	732	739	rVB	276921	236583	20.56%	3.389%
4	6.539	753	757	760	rBV	264162	231257	20.09%	3.312%
5	6.775	793	797	800	rBV	1002949	867302	75.36%	12.423%
6	6.928	820	823	826	rBV	219183	169220	14.70%	2.424%
7	7.322	887	890	894	rBV	139630	123731	10.75%	1.772%
8	8.057	1010	1015	1018	rBV	1306764	1150899	100.00%	16.485%
9	9.128	1193	1197	1203	rBV	294183	226799	19.71%	3.249%
10	9.522	1261	1264	1266	rBV	35882	29999	2.61%	0.430%
11	9.616	1275	1280	1284	rBV6	12252	19892	1.73%	0.285%
12	9.810	1308	1313	1318	rBV	1111111	1047753	91.04%	15.008%
13	10.586	1442	1445	1449	rBV	120866	110569	9.61%	1.584%
14	10.722	1465	1468	1469	rBV2	15055	14473	1.26%	0.207%
15	10.739	1469	1471	1474	rVB	16610	14201	1.23%	0.203%
16	11.286	1560	1564	1568	rBV	1063027	908704	78.96%	13.016%
17	11.521	1598	1604	1607	rBV6	11489	22275	1.94%	0.319%
18	11.816	1652	1654	1656	rBV3	16444	13564	1.18%	0.194%
19	12.463	1762	1764	1767	rBV4	18040	15516	1.35%	0.222%
20	12.498	1767	1770	1773	rBV3	26573	32271	2.80%	0.462%
21	12.868	1830	1833	1839	rBV	229606	196632	17.09%	2.817%
22	13.921	2008	2012	2015	rBV	825211	784587	68.17%	11.238%
23	15.351	2251	2255	2259	rVB	401807	488780	42.47%	7.001%


Sum of corrected areas: 6981394

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096341.D
Acq On : 30 Jun 2017 17:04
Operator : SJ/MA
Sample : I3882-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G51-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

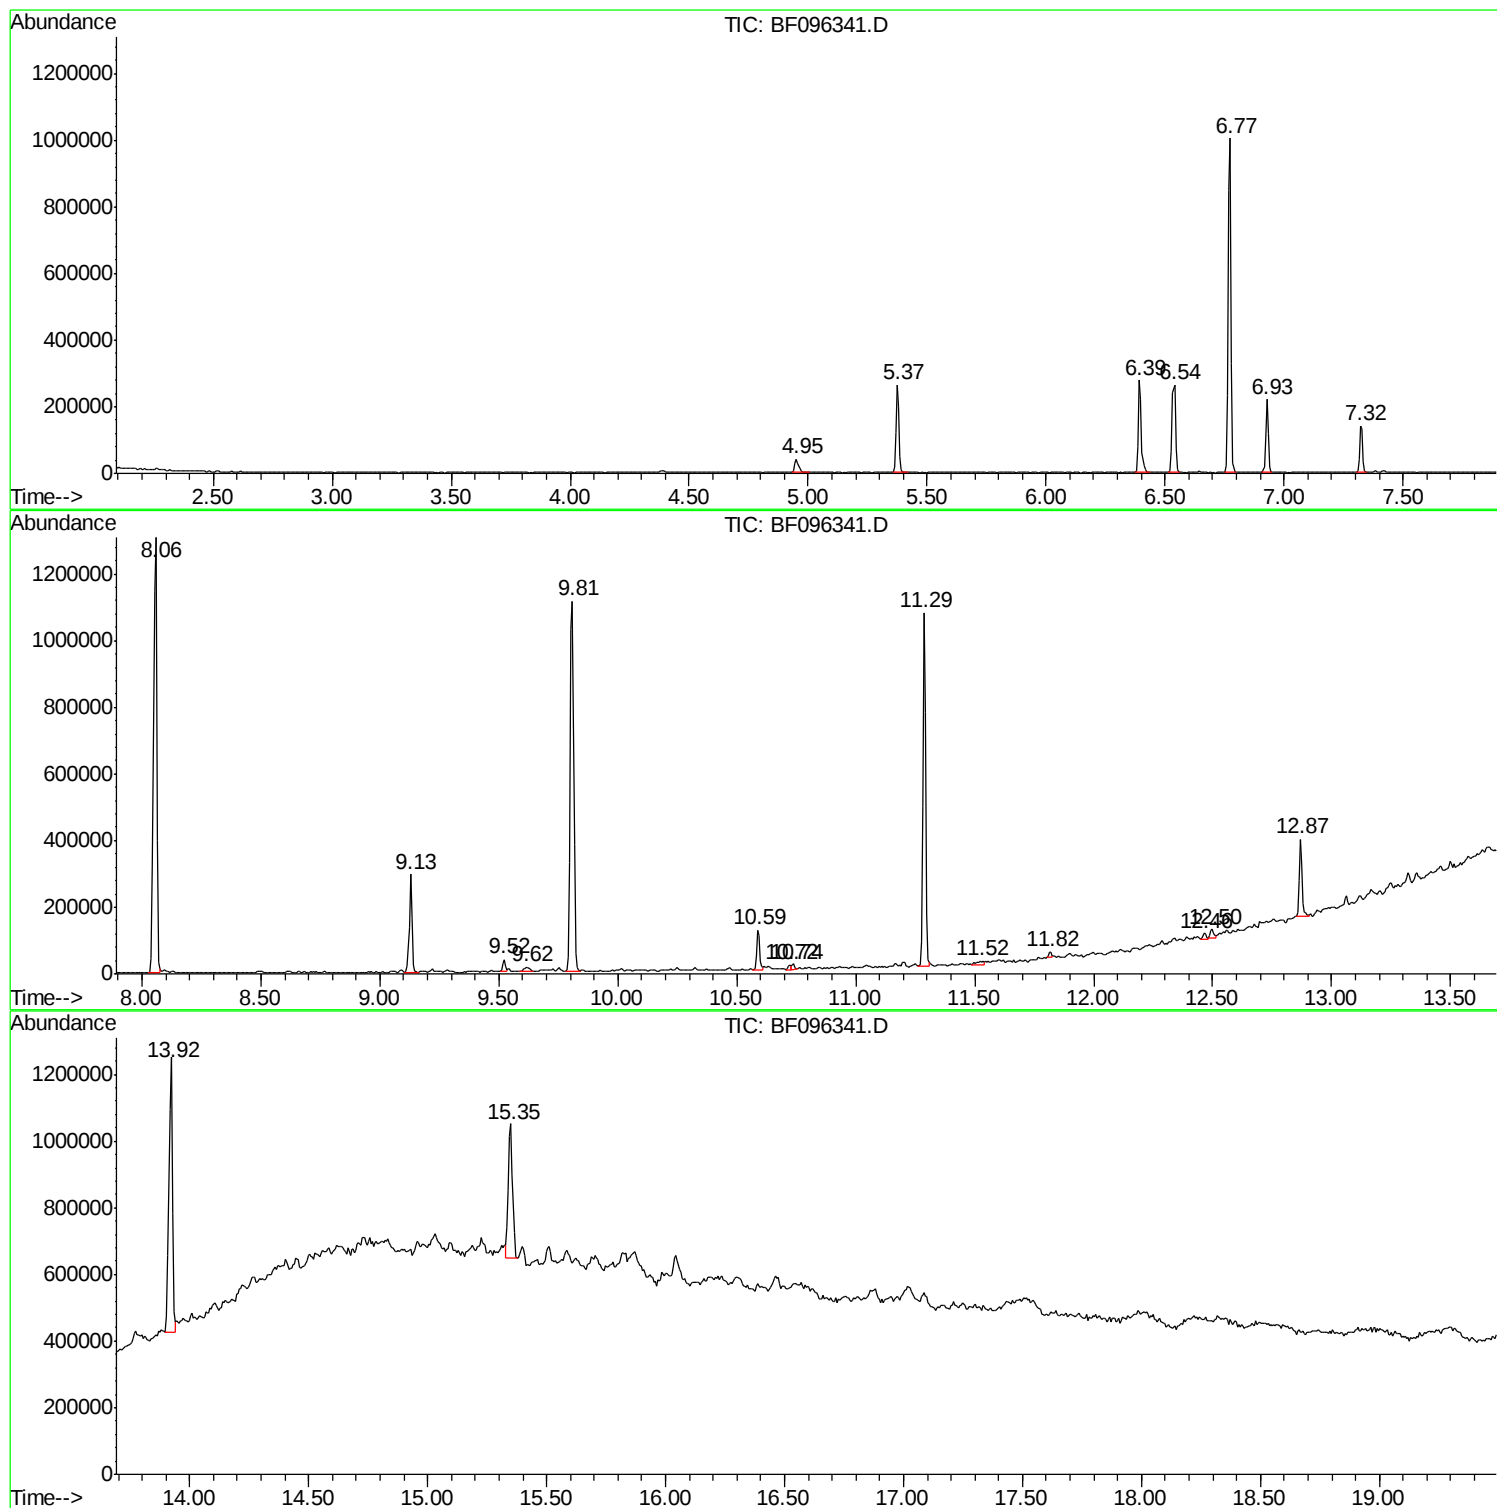

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096341.D
Acq On : 30 Jun 2017 17:04
Operator : SJ/MA
Sample : I3882-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G51-1.5-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3-Chloro-6-fluoro-pyrazine Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.54	5.33 ng	231257	1,4-Dichlorobenzene-d4	6.77

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3			Amphetaminil	250	C17H18N2	017590-01-1	12
4			1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

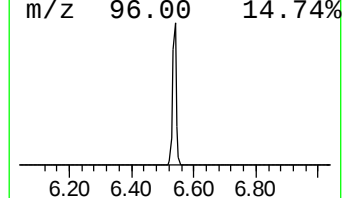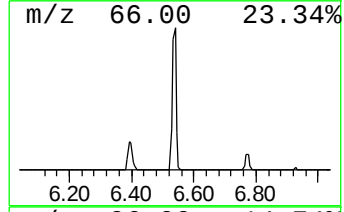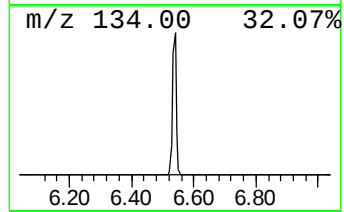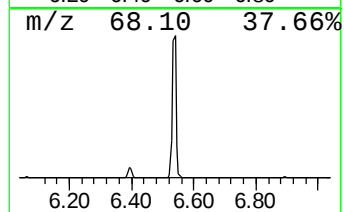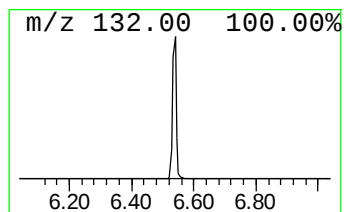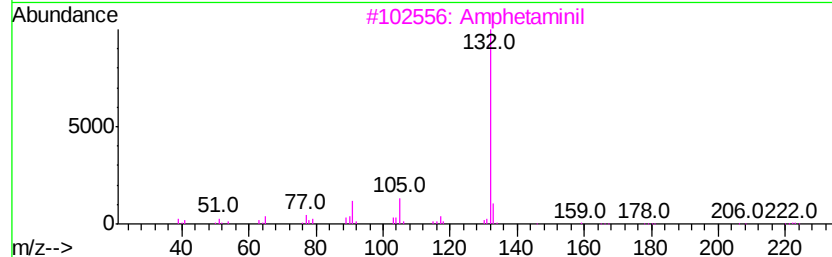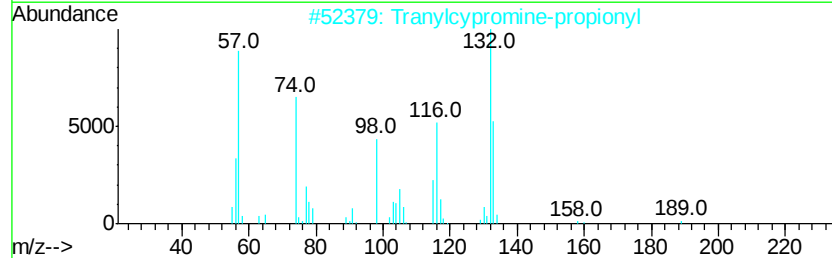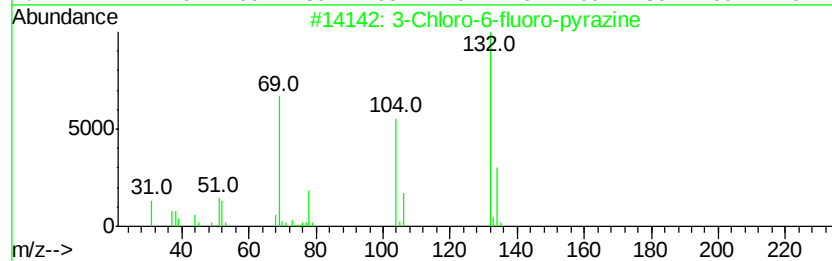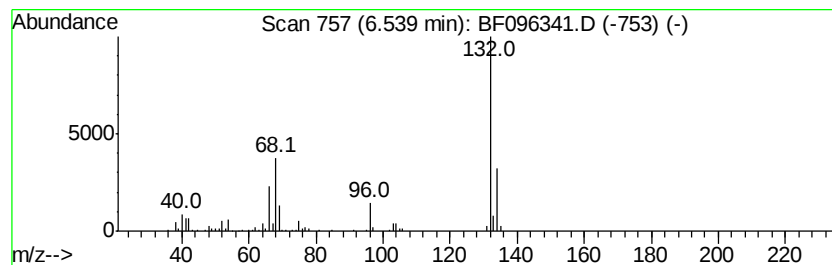

Data Path : Z:\HPCHEM1\BNA F\DATA\BF063017\
Data File : BF096341.D
Acq On : 30 Jun 2017 17:04
Operator : SJ/MA
Sample : I3882-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G51-1.5-3










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1,2-Dichlorobenzene-D4 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.93	3.90 ng	169220	1,4-Dichlorobenzene-d4	6.77

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,2-Dichlorobenzene-D4	150	C6D4Cl2	002199-69-1	96
2			1,4-Dichlorobenzene-D4	150	C6D4Cl2	003855-82-1	96
3			Benzenamine, N,N-dimethyl-4-nitr...	150	C8H10N2O	000138-89-6	16
4			2-Cyclohexene-1,4-dione, 5,6-dic...	370	C15H12Cl2N2O5	324051-46-9	14
5			2-Cyclohexene-1,4-dione, 5,6-dic...	370	C15H12Cl2N2O5	324051-56-1	12

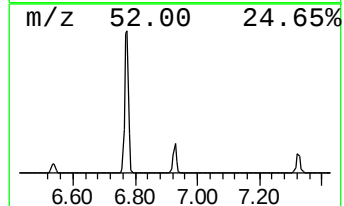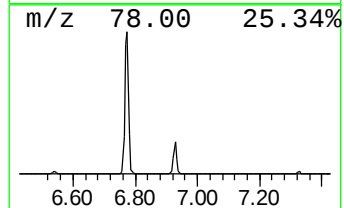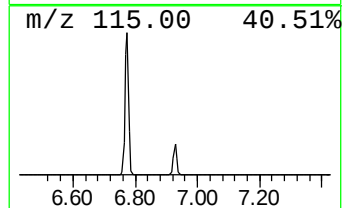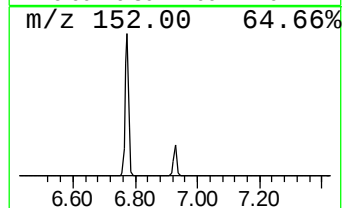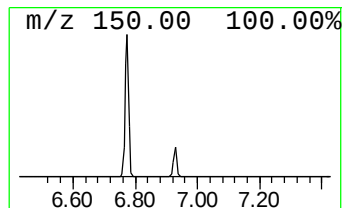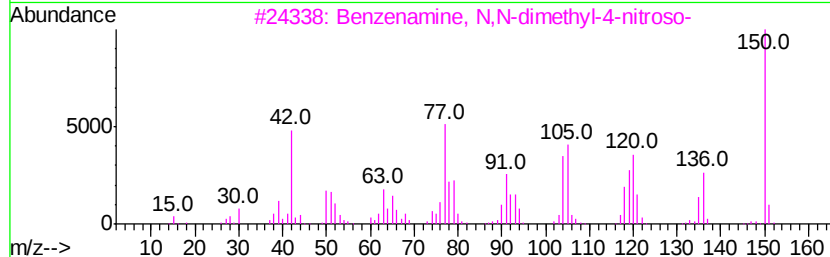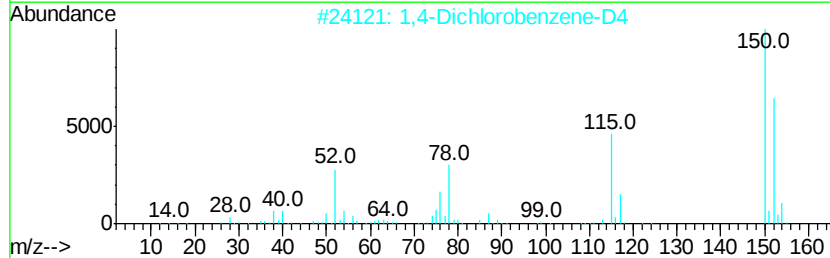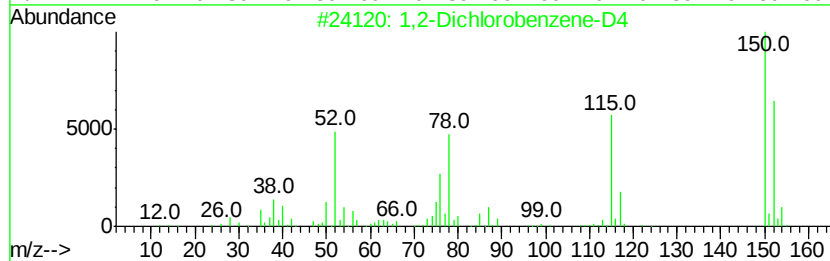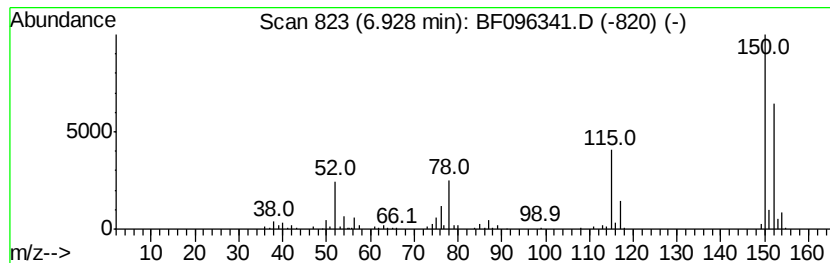

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF063017\
Data File : BF096341.D
Acq On : 30 Jun 2017 17:04
Operator : SJ/MA
Sample : I3882-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G51-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3-Chloro-6-fluoro...	6.54	5.3	ng	231257	1	6.77	867302	20.0
1,2-Dichlorobenze...	6.93	3.9	ng	169220	1	6.77	867302	20.0