


Data Path : Z:\HPCHEM1\BNA_F\Data\BF063017\
 Data File : BF096342.D
 Acq On : 30 Jun 2017 17:57
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF062717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 15:41:49 2017

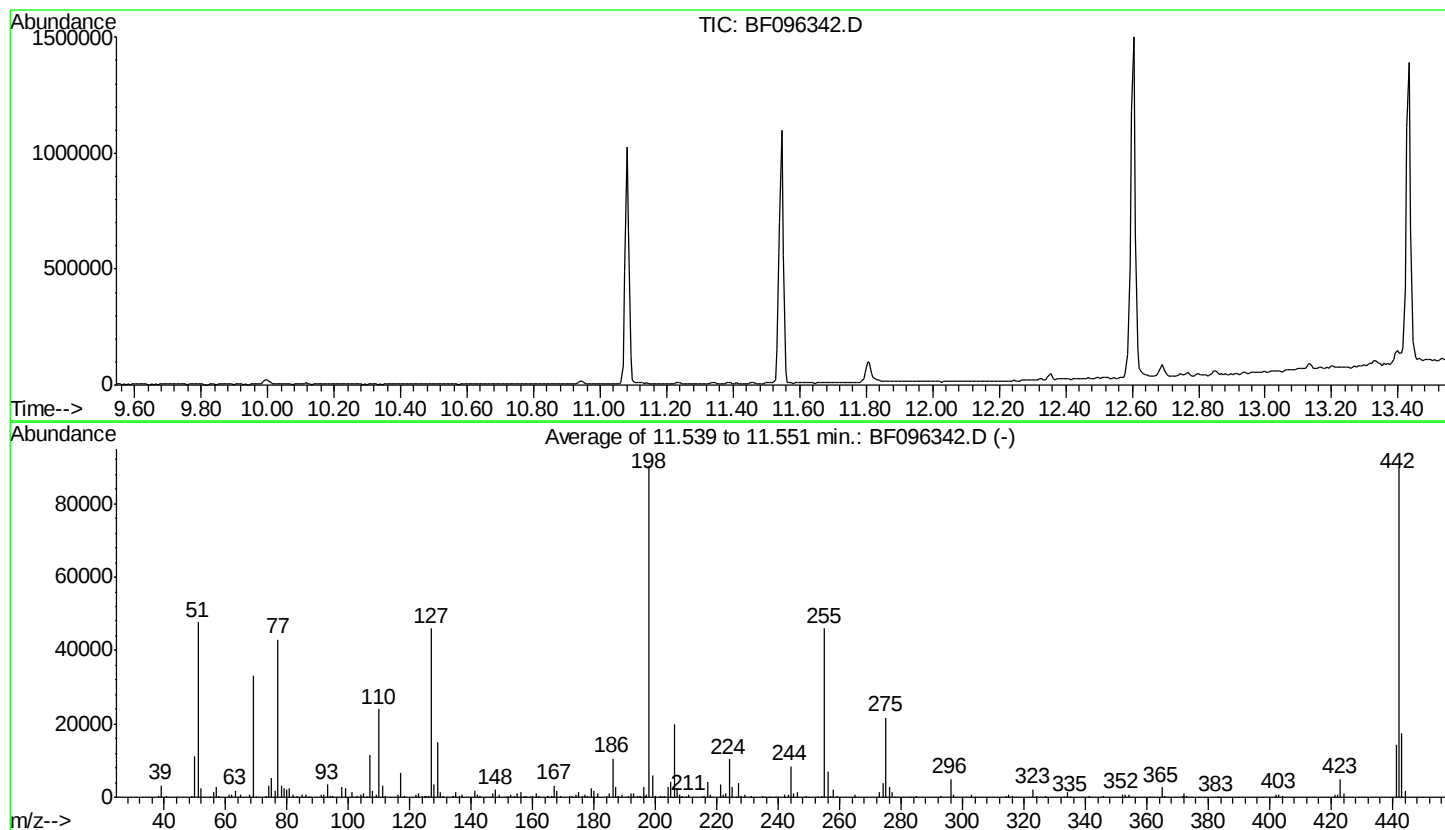

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.8	47781	PASS
68	69	0.00	2	1.8	596	PASS
69	198	0.00	100	36.9	33340	PASS
70	69	0.00	2	0.6	186	PASS
127	198	10	80	50.8	45952	PASS
197	198	0.00	2	0.7	609	PASS
198	198	100	100	100.0	90410	PASS
199	198	5	9	6.7	6032	PASS
275	198	10	60	24.0	21706	PASS
365	198	1	100	3.1	2793	PASS
441	442	0.01	24	15.9	14286	PASS
442	198	50	100	99.5	89981	PASS
443	442	15	24	19.5	17533	PASS