

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063021\
 Data File : BF124493.D
 Acq On : 30 Jun 2021 15:09
 Operator : JU/CG
 Sample : PB137373BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137373BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.328	547	551	565	rBV	1360059	1279653	67.20%	12.757%
2	6.351	720	725	739	rBV	1088801	1214785	63.79%	12.110%
3	6.692	780	783	791	rBB	285324	243570	12.79%	2.428%
4	7.263	875	880	883	rBV	881235	829123	43.54%	8.266%
5	7.969	997	1000	1006	rBV	322869	311228	16.34%	3.103%
6	9.051	1179	1184	1187	rBV	2071618	1781186	93.53%	17.757%
7	9.722	1295	1298	1302	rBV	423845	383372	20.13%	3.822%
8	10.522	1430	1434	1444	rBV	1185042	1120695	58.85%	11.172%
9	11.210	1548	1551	1560	rBV	453270	398164	20.91%	3.969%
10	12.804	1817	1822	1825	rBV	2123016	1904319	100.00%	18.985%
11	13.857	1998	2001	2007	rVB	368330	305710	16.05%	3.048%
12	15.286	2240	2244	2257	rBV	201298	259054	13.60%	2.583%




Sum of corrected areas: 10030859

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063021\
Data File : BF124493.D
Acq On : 30 Jun 2021 15:09
Operator : JU/CG
Sample : PB137373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137373BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

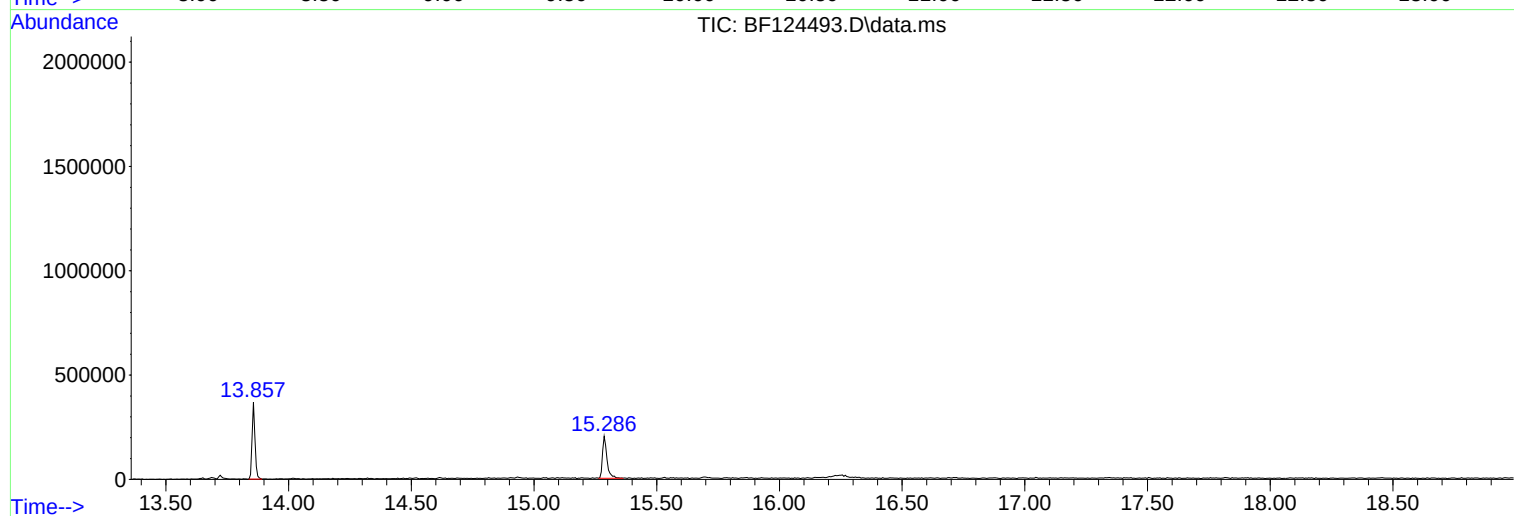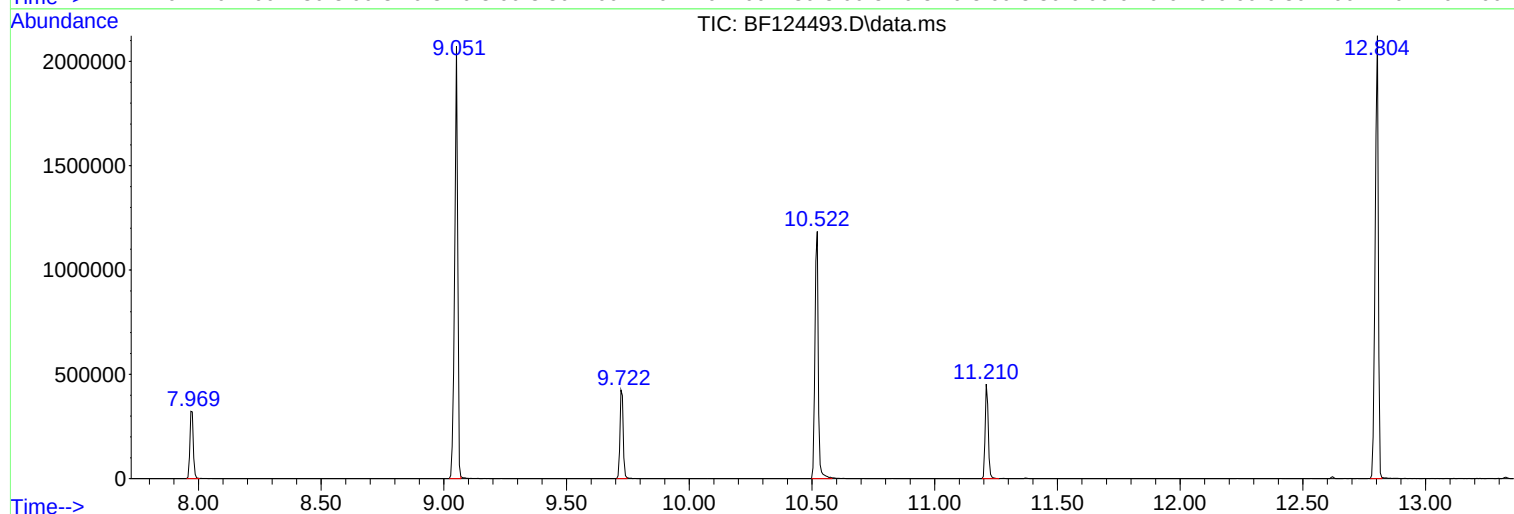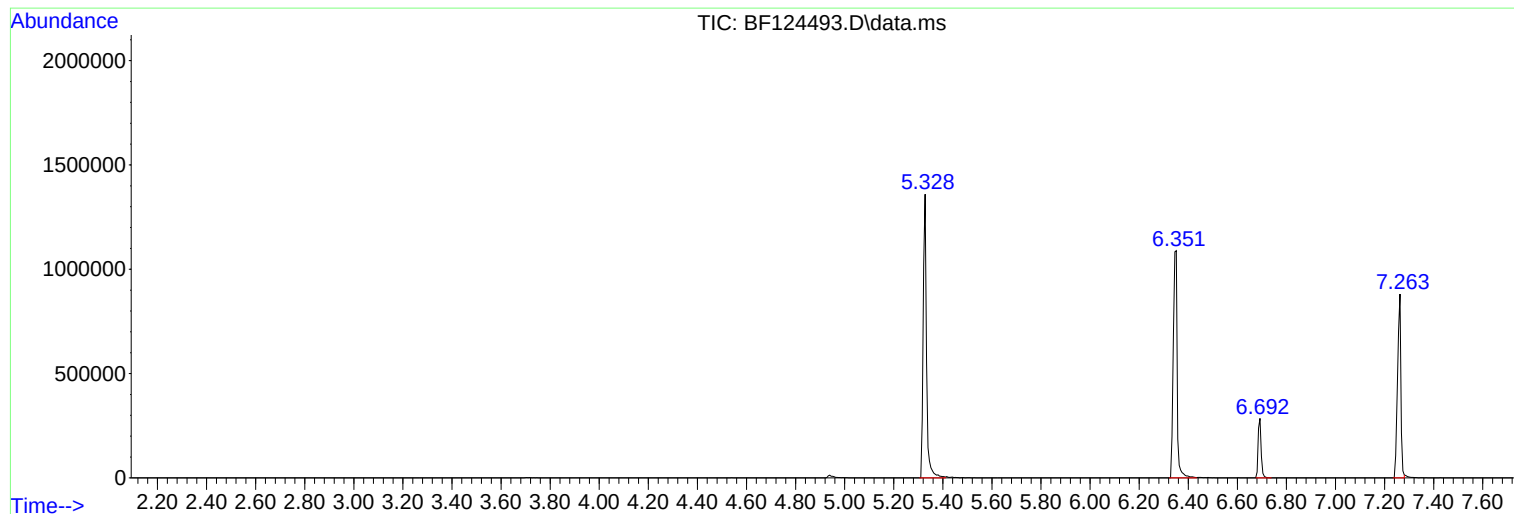

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063021\
Data File : BF124493.D
Acq On : 30 Jun 2021 15:09
Operator : JU/CG
Sample : PB137373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137373BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063021\
Data File : BF124493.D
Acq On : 30 Jun 2021 15:09
Operator : JU/CG
Sample : PB137373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137373BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------