
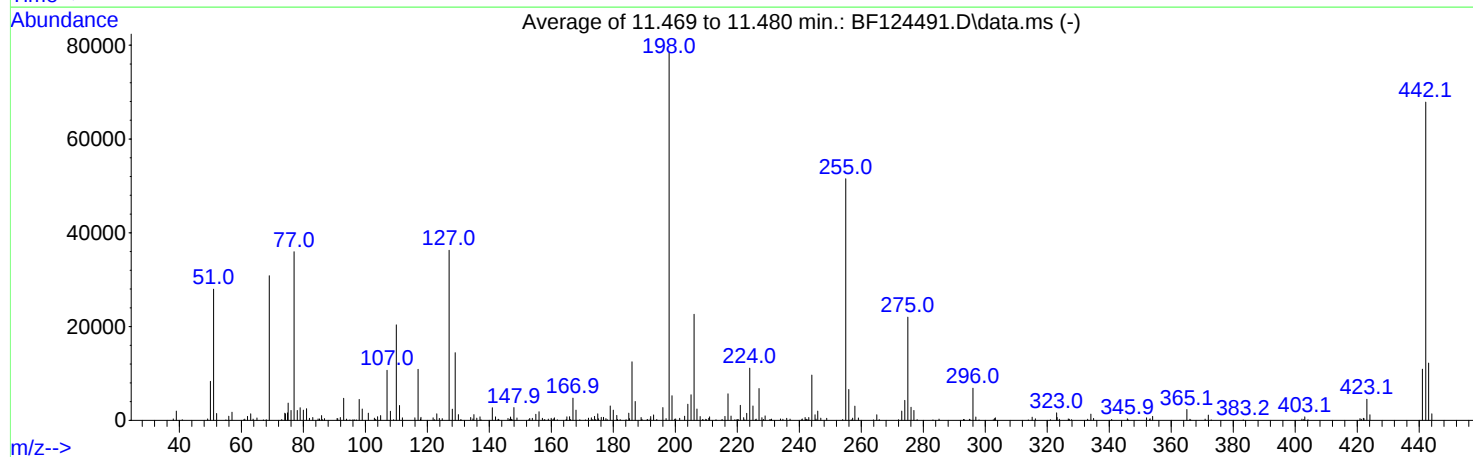


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063021\
 Data File : BF124491.D
 Acq On : 30 Jun 2021 14:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 14:15:13 2021

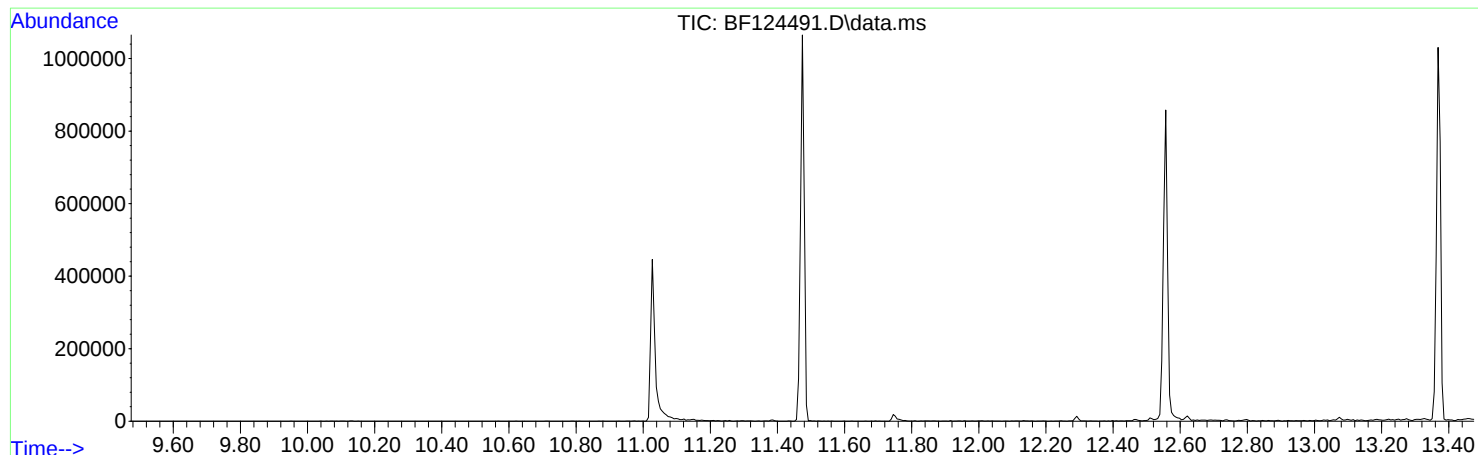




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	27968	PASS
68	69	0.00	2	0.4	133	PASS
69	198	0.00	100	39.3	30862	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.3	36291	PASS
197	198	0.00	2	0.5	395	PASS
198	198	100	100	100.0	78448	PASS
199	198	5	9	6.7	5244	PASS
275	198	10	60	28.0	22003	PASS
365	198	1	100	2.9	2314	PASS
441	198	0.01	100	13.9	10931	PASS
442	442	50	100	100.0	67872	PASS
443	442	15	24	18.0	12214	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063021\
Data File : BF124491.D
Acq On : 30 Jun 2021 14:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 14:33:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 12:49:33 2021
Response via : Initial Calibration

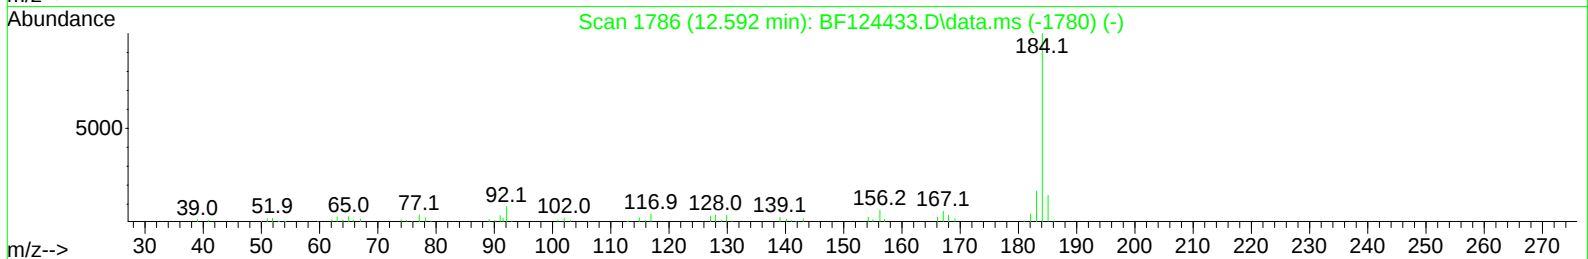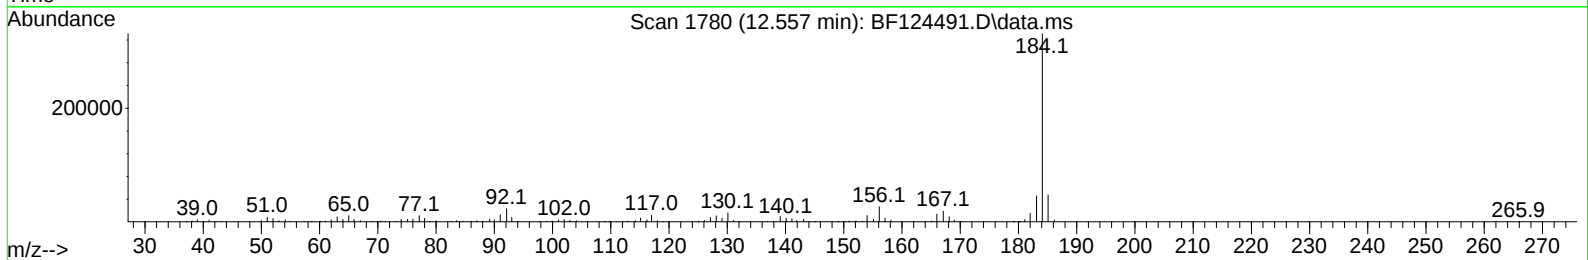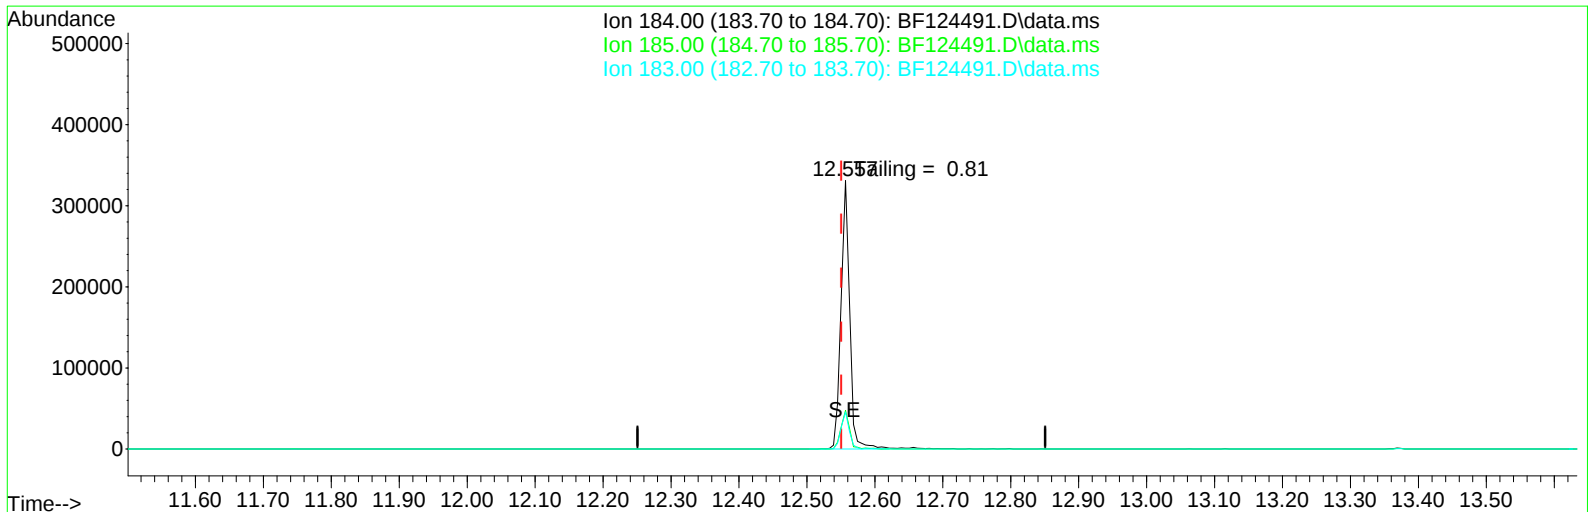

TIC: BF124491.D\data.ms

(77) Benzidine

12.557min (+ 0.006) 0.00 ng




response 295972

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.41
183.00	9.80	13.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063021\
Data File : BF124491.D
Acq On : 30 Jun 2021 14:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 14:33:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 12:49:33 2021
Response via : Initial Calibration

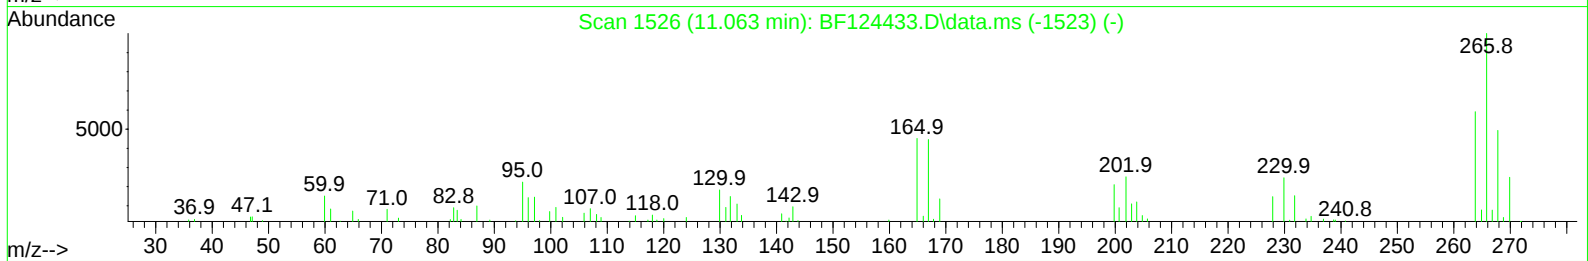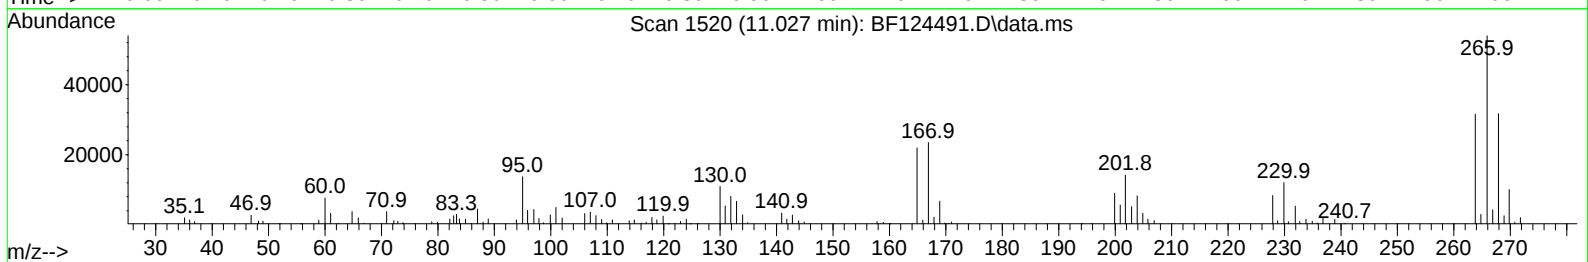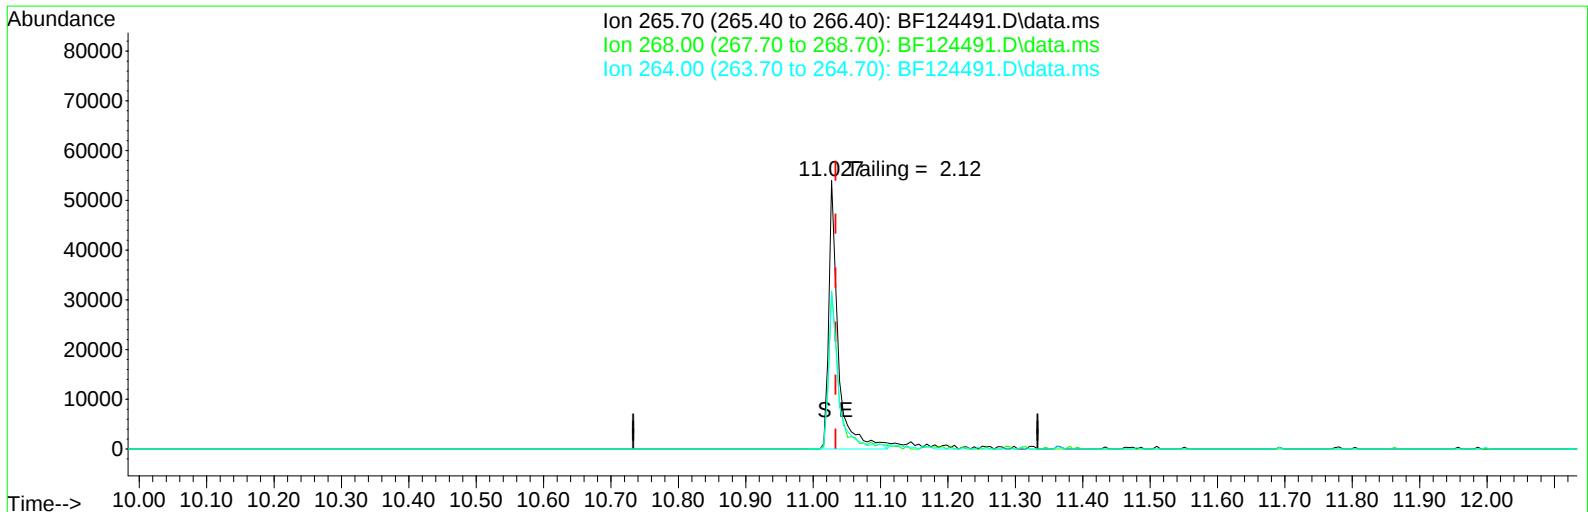

TIC: BF124491.D\data.ms

(70) Pentachlorophenol (C)

11.027min (-0.006) 0.00 ng

response 54683

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	58.82
264.00	65.70	58.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2021	BNA_F	<u>BF124491.D</u>
Compound Name	Response	Retention Time
DDT	161830	13.36
DDD	2003	13.07
DDE	500	12.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2503	164333	1.52