
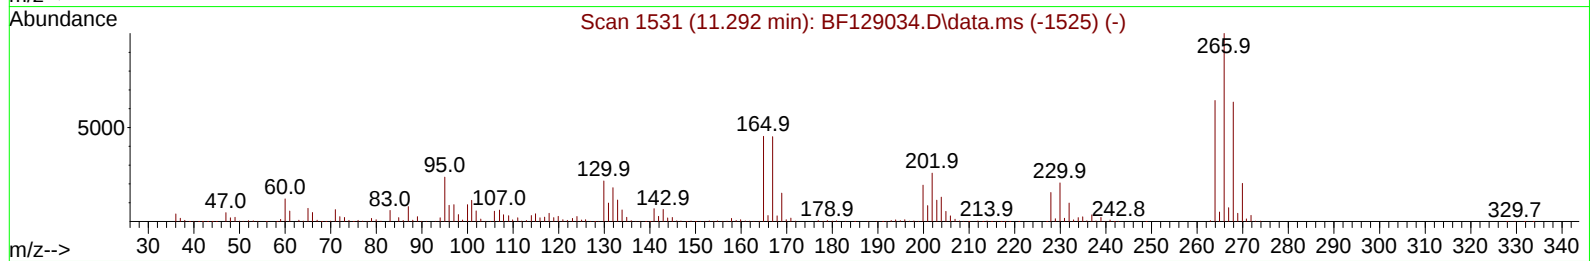
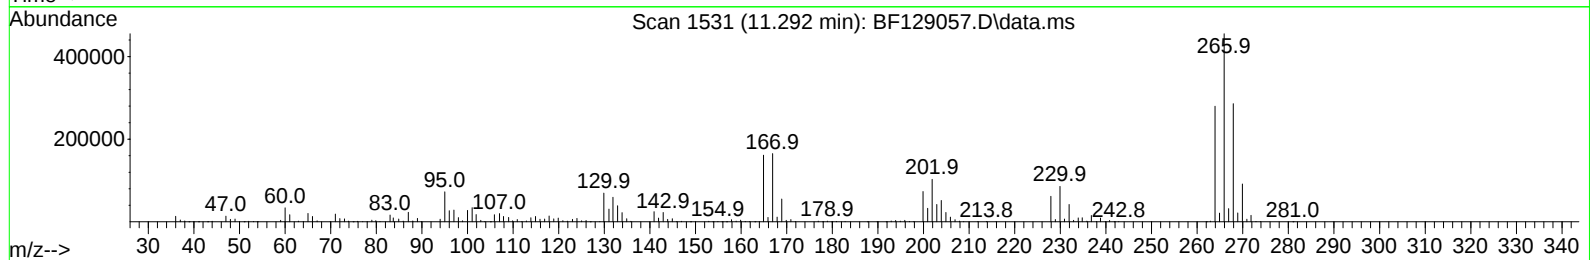


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129057.D
 Acq On : 30 Jun 2022 14:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 08:55:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

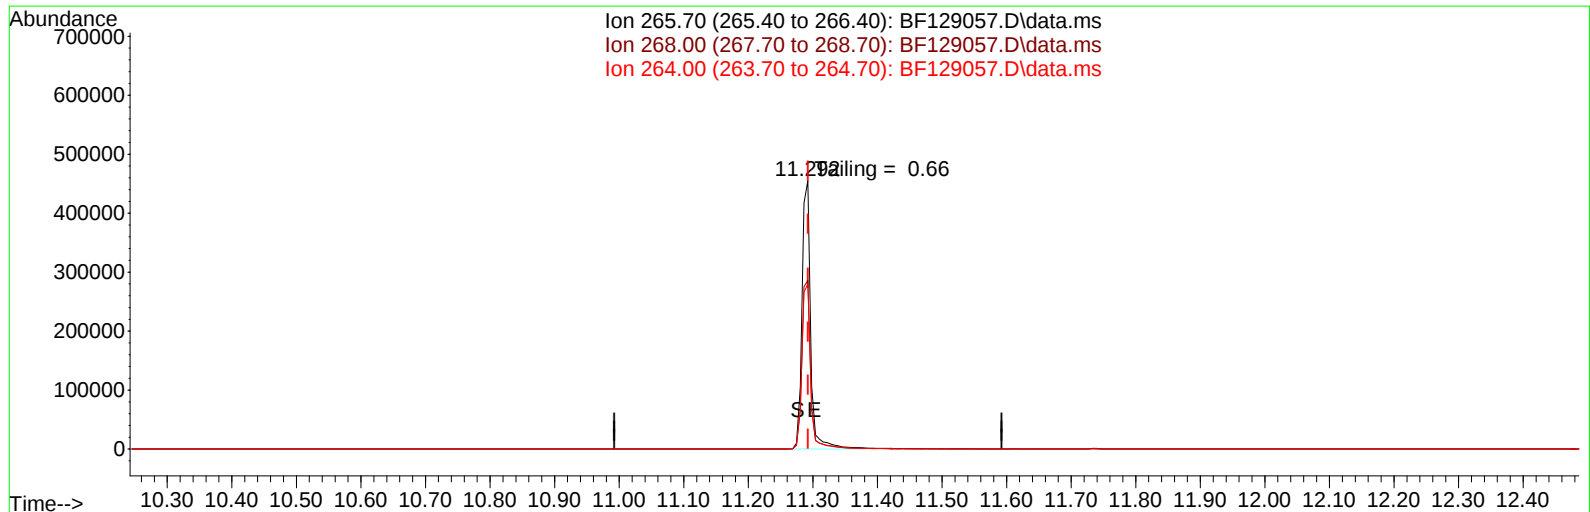

TIC: BF129057.D\data.ms

(70) Pentachlorophenol (C)




11.292min (-0.000) 192430.21 ng

response 427645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.83
264.00	61.80	61.45
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\  
Data File : BF129057.D  
Acq On    : 30 Jun 2022  14:24  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 01 08:55:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

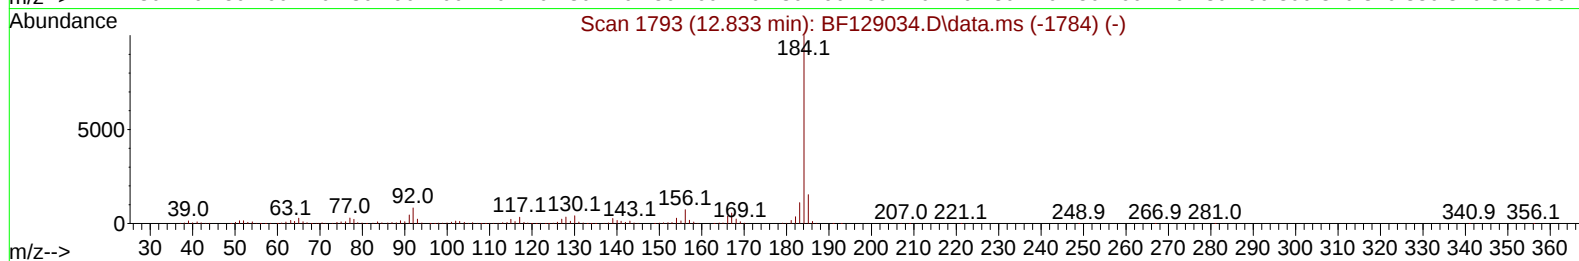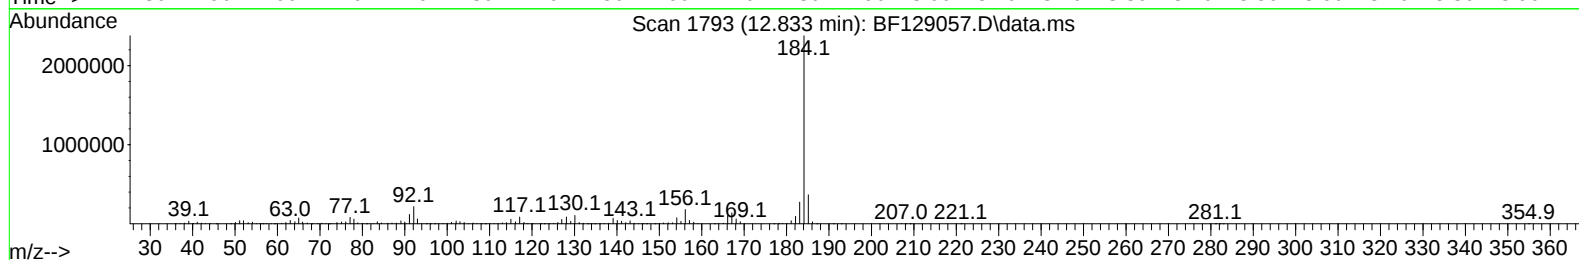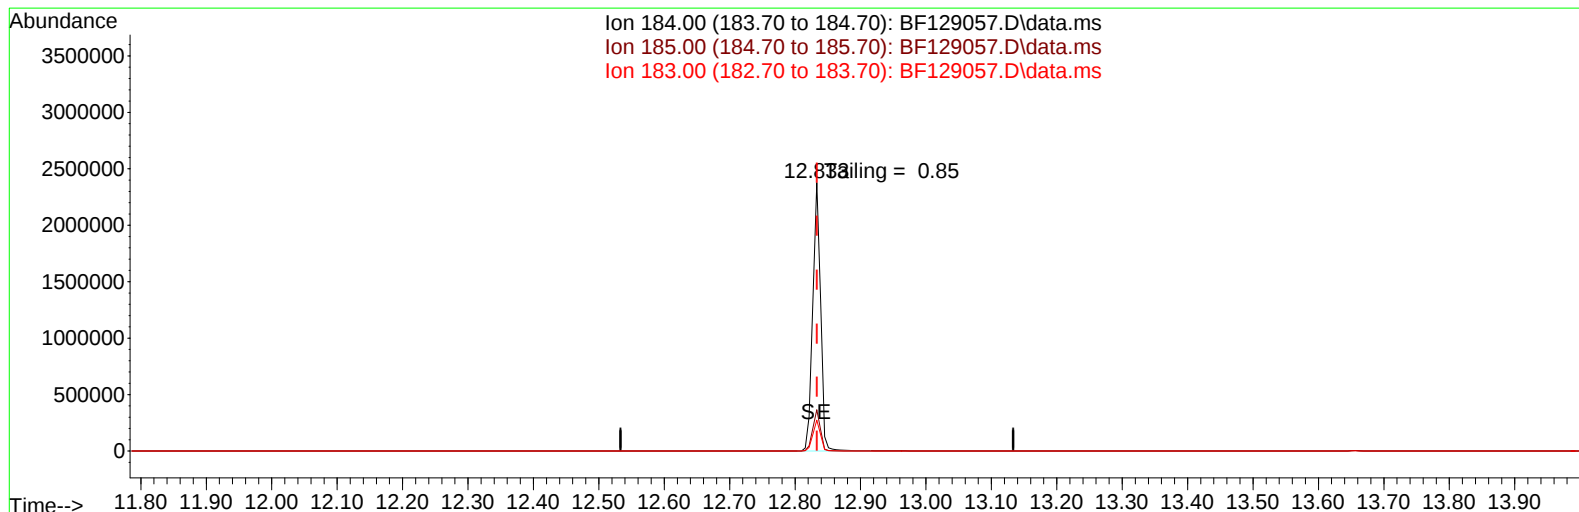

TIC: BF129057.D\data.ms

(77) Benzidine

12.833min (-0.000) 441893.12 ng

response **1990730**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	15.40
--------	-------	-------

183.00	11.60	11.54
--------	-------	-------

0.00 0.00 0.00