

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129049.D
 Acq On : 30 Jun 2022 10:28
 Operator : CG\JU
 Sample : PB145806BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145806BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.375	6	15	23	rVB	253649	353717	2.70%	0.444%
2	5.593	557	562	565	rBV	8924312	9933400	75.88%	12.465%
3	6.581	724	730	733	rBV	8255866	9991712	76.32%	12.539%
4	6.957	790	794	797	rBV	3038808	2365546	18.07%	2.969%
5	7.522	884	890	893	rBV	6451904	6618213	50.55%	8.305%
6	8.240	1007	1012	1015	rBV	3700733	3227510	24.65%	4.050%
7	9.316	1189	1195	1198	rBV	12273850	12576228	96.07%	15.782%
8	9.998	1305	1311	1315	rBV	4340642	3661545	27.97%	4.595%
9	10.792	1439	1446	1449	rBV	8521901	7879217	60.19%	9.888%
10	11.492	1559	1565	1568	rBV	4598144	3807936	29.09%	4.779%
11	13.086	1831	1836	1839	rBV	13205920	13091361	100.00%	16.428%
12	14.139	2011	2015	2019	rBV	3702670	3245671	24.79%	4.073%
13	14.239	2028	2032	2037	rBV	137478	143145	1.09%	0.180%
14	15.668	2269	2275	2286	rBV	2186489	2792277	21.33%	3.504%




Sum of corrected areas: 79687478

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129049.D
Acq On : 30 Jun 2022 10:28
Operator : CG\JU
Sample : PB145806BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145806BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

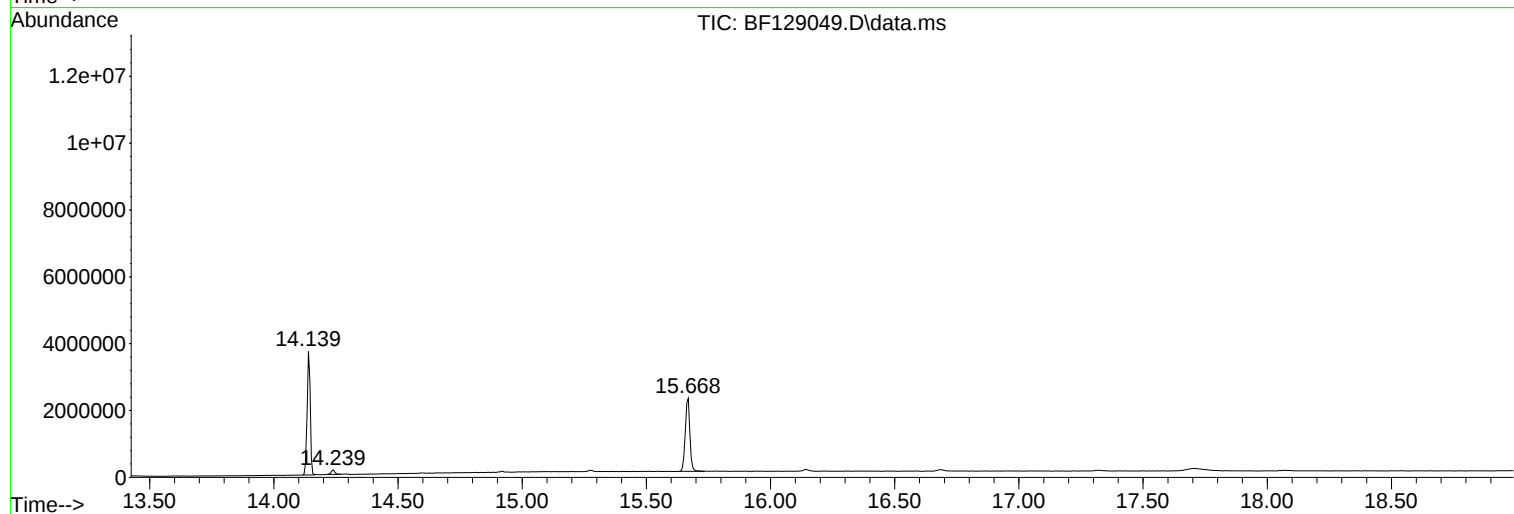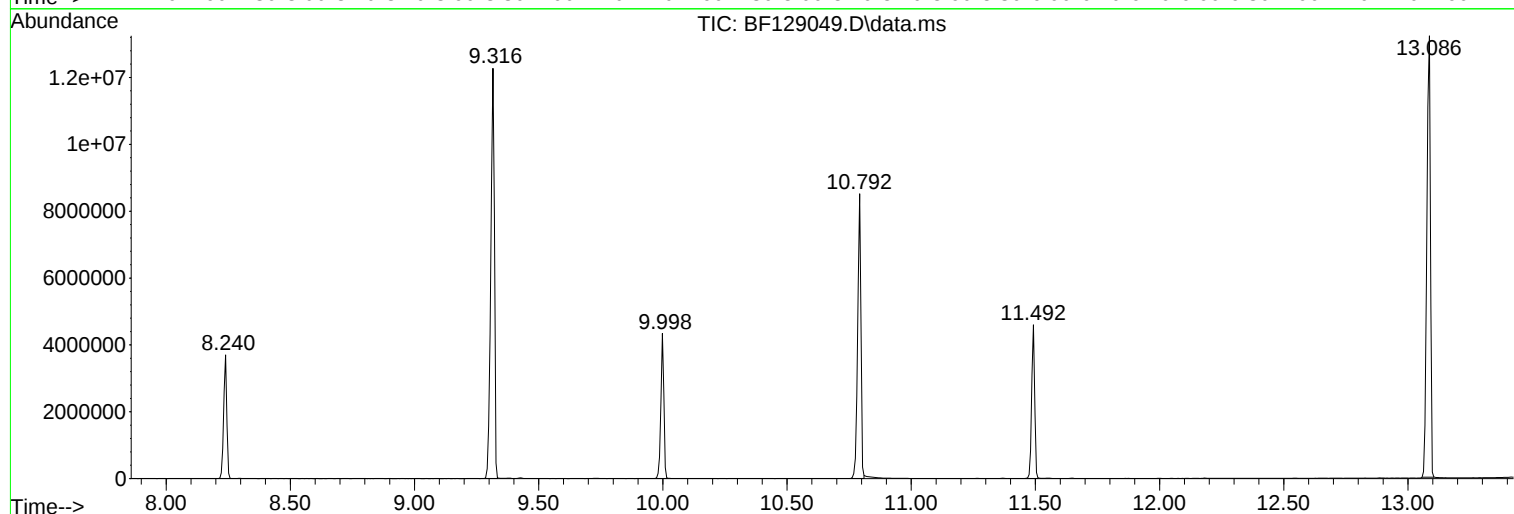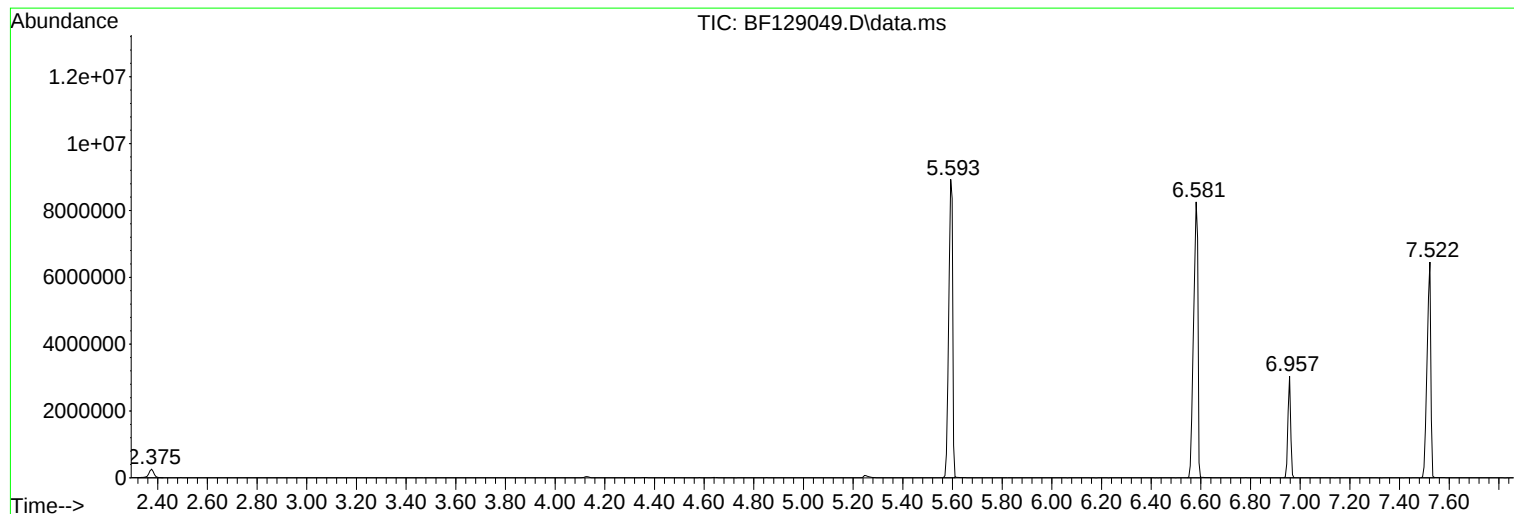

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129049.D
Acq On : 30 Jun 2022 10:28
Operator : CG\JU
Sample : PB145806BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145806BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.375	2.99 ng	353717	1,4-Dichlorobenzene-d4	6.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	23
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17

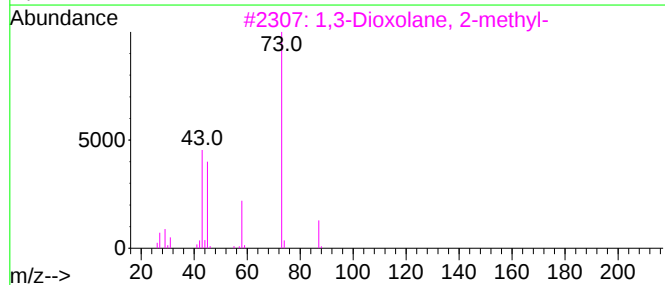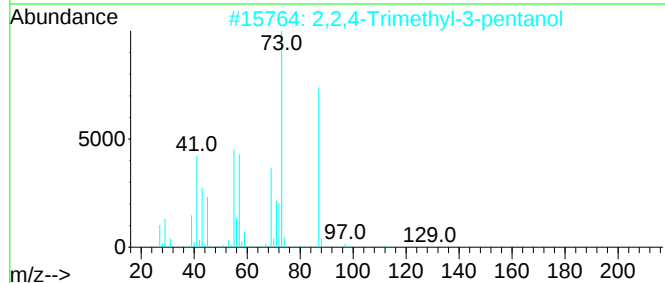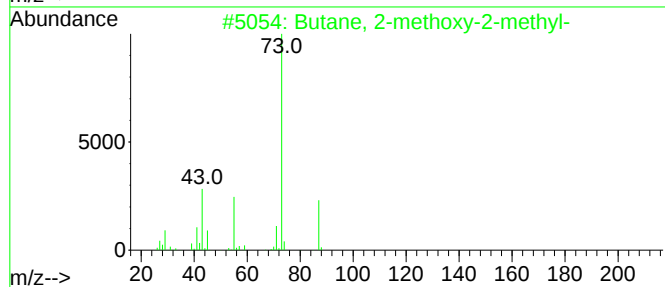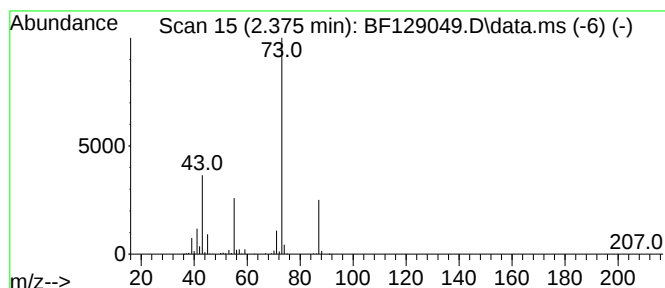

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129049.D
Acq On : 30 Jun 2022 10:28
Operator : CG\JU
Sample : PB145806BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145806BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.375	3.0	ng	353717	1	6.957	2365550	20.0