

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129053.D
 Acq On : 30 Jun 2022 12:26
 Operator : CG\JU
 Sample : PB145921BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145921BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.363	5	13	20	rVB	242125	341491	2.59%	0.429%
2	5.592	557	562	565	rBV	9110395	9923057	75.40%	12.466%
3	6.580	724	730	733	rBV	8334995	9916612	75.35%	12.458%
4	6.957	790	794	797	rBV	2935584	2370513	18.01%	2.978%
5	7.522	884	890	893	rBV	6181403	6648763	50.52%	8.353%
6	8.239	1007	1012	1015	rBV	3647916	3225002	24.51%	4.051%
7	9.316	1189	1195	1198	rBV	12231241	12535291	95.25%	15.748%
8	9.998	1305	1311	1314	rBV	4407459	3650642	27.74%	4.586%
9	10.792	1439	1446	1449	rBV	8328749	7665600	58.25%	9.630%
10	11.492	1559	1565	1568	rBV	4585779	3786627	28.77%	4.757%
11	13.086	1830	1836	1839	rBV	13390718	13160071	100.00%	16.532%
12	14.139	2011	2015	2019	rBV	3729153	3223866	24.50%	4.050%
13	14.239	2027	2032	2036	rBV	121578	145166	1.10%	0.182%
14	15.662	2269	2274	2284	rBV	2139168	2852197	21.67%	3.583%
15	16.139	2351	2355	2361	rVB	97646	156599	1.19%	0.197%




Sum of corrected areas: 79601497

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129053.D
Acq On : 30 Jun 2022 12:26
Operator : CG\JU
Sample : PB145921BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

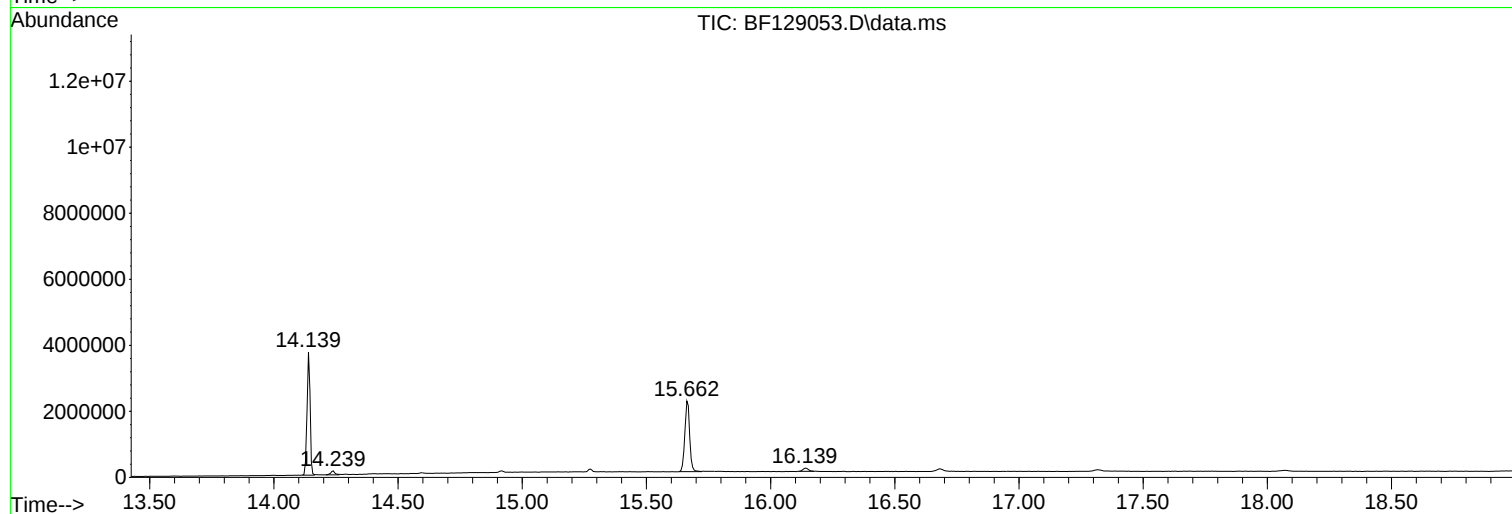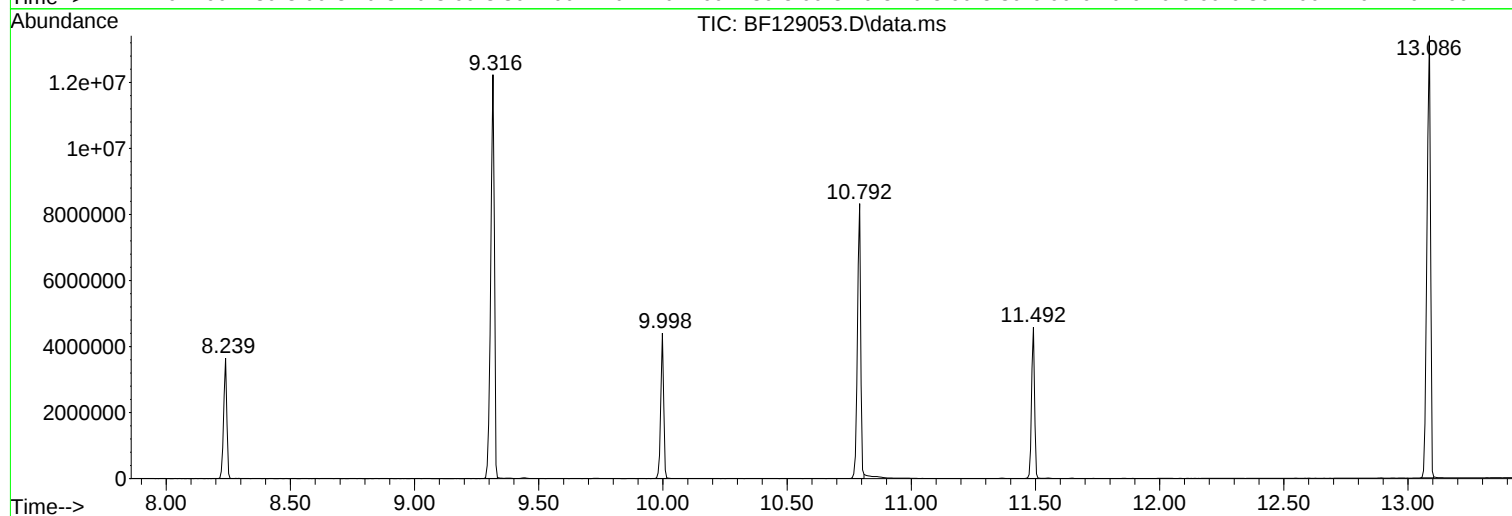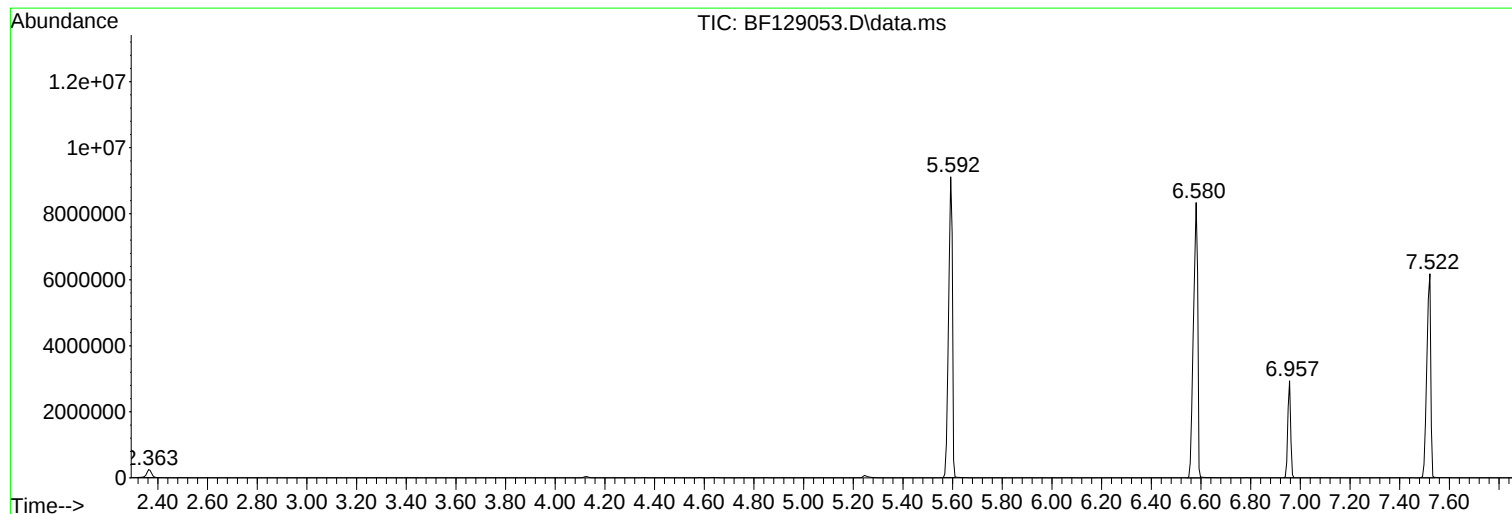

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129053.D
Acq On : 30 Jun 2022 12:26
Operator : CG\JU
Sample : PB145921BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145921BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.363	2.88 ng	341491	1,4-Dichlorobenzene-d4	6.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	27
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

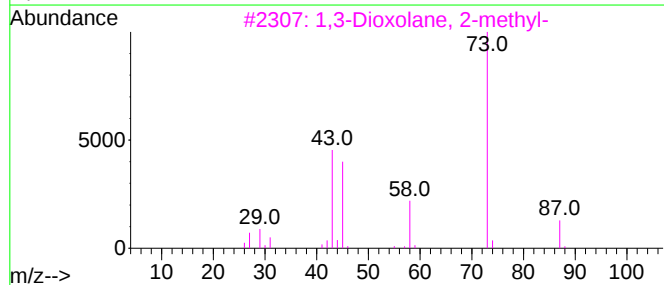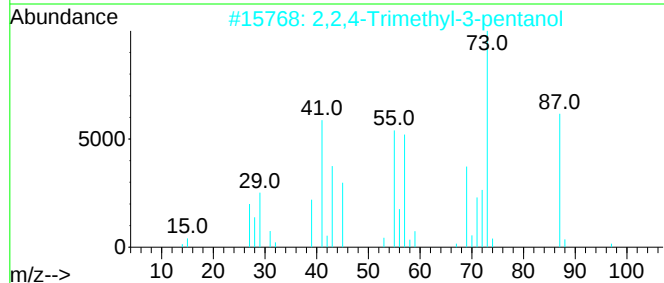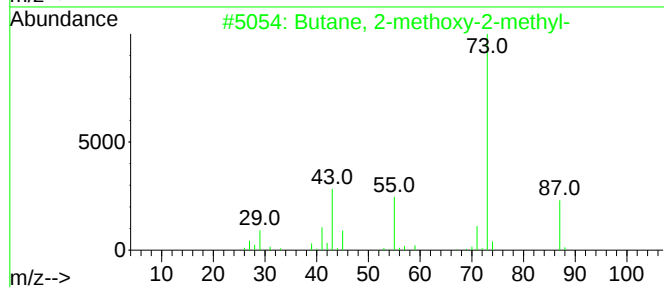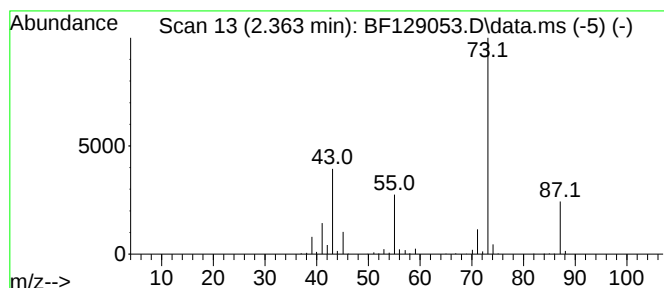

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129053.D
Acq On : 30 Jun 2022 12:26
Operator : CG\JU
Sample : PB145921BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.363	2.9	ng	341491	1	6.957	2370510	20.0