

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129056.D
 Acq On : 30 Jun 2022 13:54
 Operator : CG\JU
 Sample : PB145775BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145775BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.369	6	14	21	rVB	241836	347002	2.66%	0.430%
2	5.592	557	562	565	rBV	9207055	10182605	78.04%	12.625%
3	6.581	724	730	733	rBV	8328073	10220066	78.33%	12.671%
4	6.957	790	794	797	rBV	3056411	2435928	18.67%	3.020%
5	7.522	884	890	893	rBV	6558326	6793275	52.06%	8.423%
6	8.239	1007	1012	1015	rBV	3807925	3306360	25.34%	4.099%
7	9.316	1189	1195	1198	rBV	12654300	12674582	97.14%	15.714%
8	9.998	1305	1311	1315	rBV	4497540	3755503	28.78%	4.656%
9	10.792	1439	1446	1449	rBV	8566187	7748489	59.38%	9.607%
10	11.492	1559	1565	1568	rBV	4582978	3821080	29.28%	4.738%
11	13.086	1831	1836	1839	rBV	12894864	13048116	100.00%	16.177%
12	14.139	2011	2015	2019	rBV	3623669	3078526	23.59%	3.817%
13	14.239	2027	2032	2038	rBV	113205	155267	1.19%	0.193%
14	15.662	2269	2274	2282	rBV	1993331	2692687	20.64%	3.338%
15	16.139	2351	2355	2366	rVB	134673	225117	1.73%	0.279%
16	16.680	2443	2447	2454	rVB	101770	171421	1.31%	0.213%




Sum of corrected areas: 80656024

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129056.D
Acq On : 30 Jun 2022 13:54
Operator : CG\JU
Sample : PB145775BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145775BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

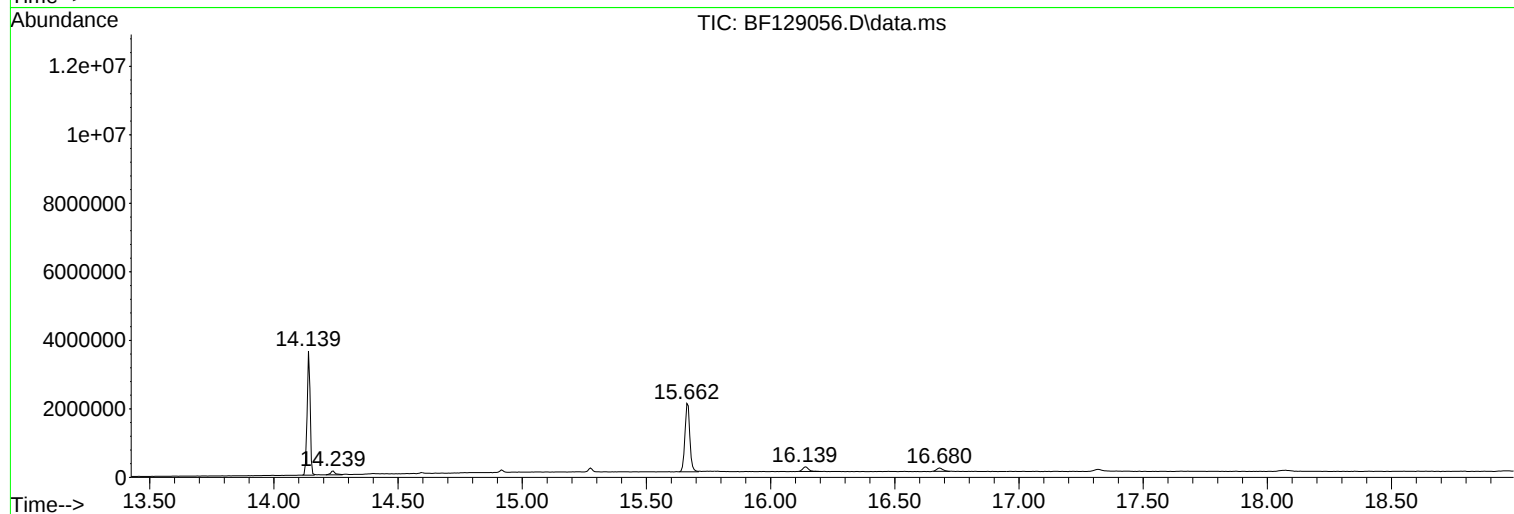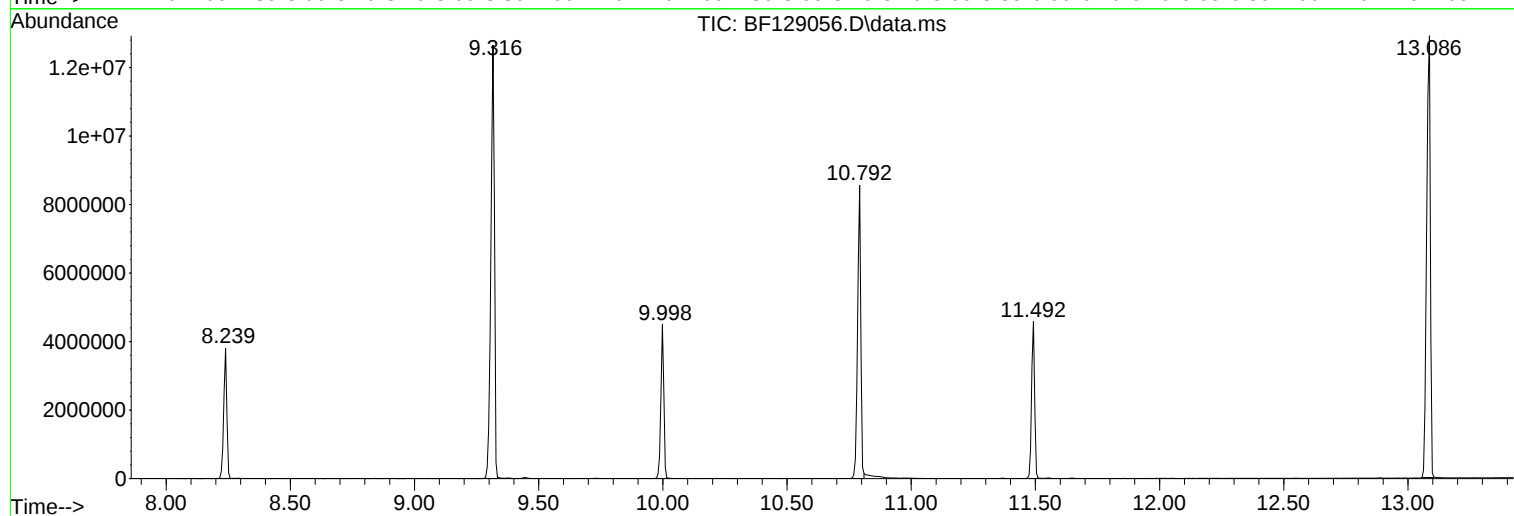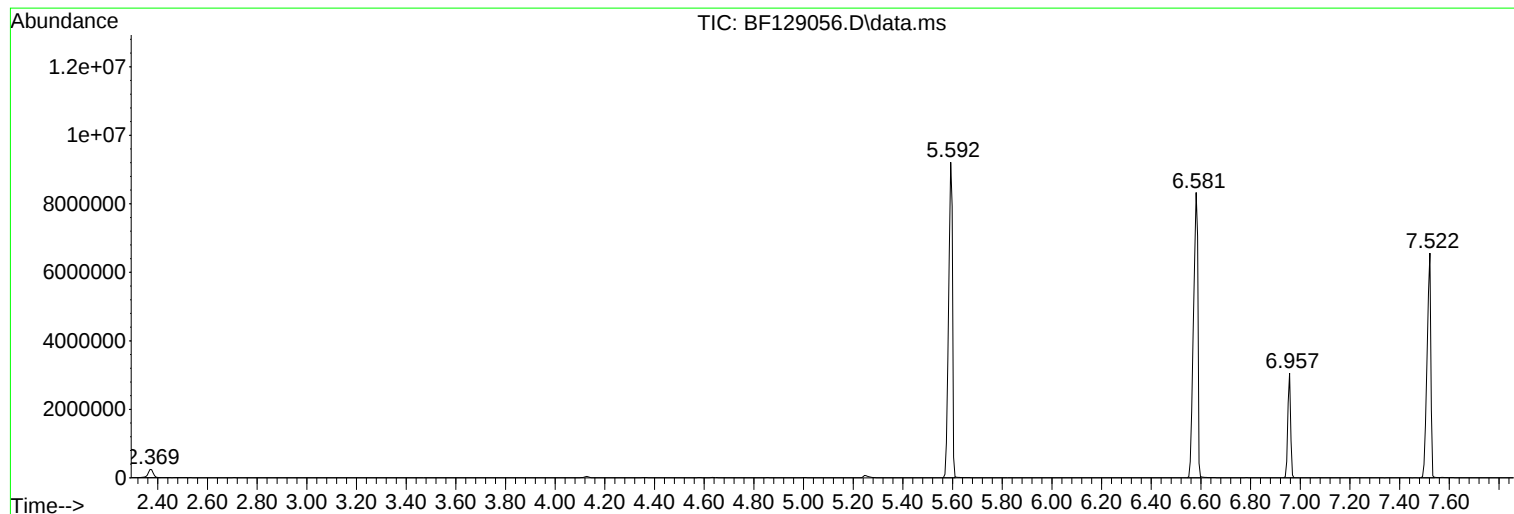

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129056.D
Acq On : 30 Jun 2022 13:54
Operator : CG\JU
Sample : PB145775BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145775BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.369	2.85 ng	347002	1,4-Dichlorobenzene-d4	6.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17

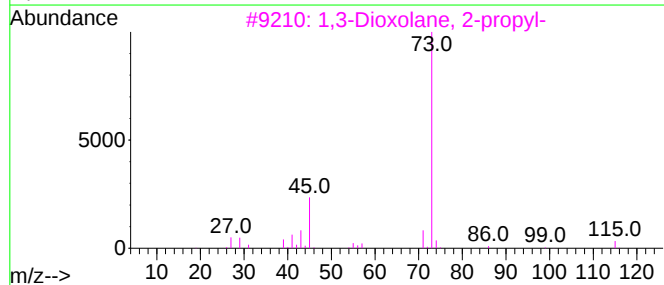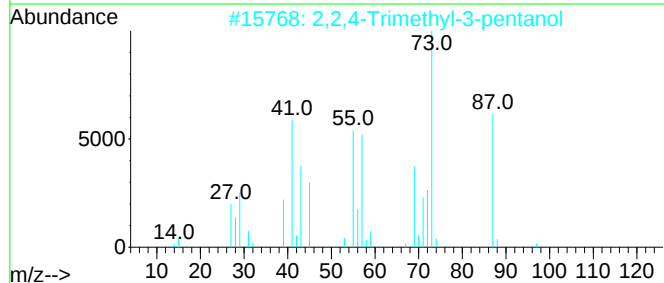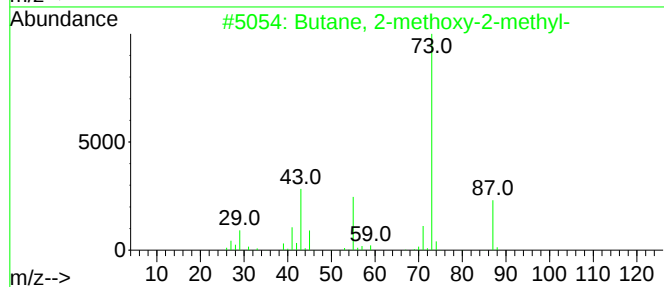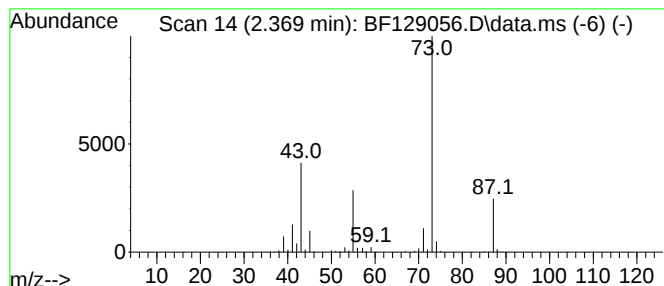

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129056.D
Acq On : 30 Jun 2022 13:54
Operator : CG\JU
Sample : PB145775BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145775BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.369	2.9	ng	347002	1	6.957	2435930	20.0