

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129059.D
 Acq On : 30 Jun 2022 15:24
 Operator : CG\JU
 Sample : PB145848BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145848BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.375	6	15	26	rVB	252582	370502	2.73%	0.444%
2	5.593	557	562	565	rBV	9361149	10406777	76.62%	12.473%
3	6.581	724	730	733	rBV	8551464	10422670	76.74%	12.492%
4	6.957	790	794	797	rBV	3081674	2504980	18.44%	3.002%
5	7.522	884	890	893	rBV	6371959	6973048	51.34%	8.357%
6	8.239	1007	1012	1015	rBV	3724340	3403571	25.06%	4.079%
7	9.316	1189	1195	1198	rBV	12746253	13103318	96.48%	15.704%
8	9.998	1305	1311	1314	rBV	4517879	3855870	28.39%	4.621%
9	10.792	1439	1446	1449	rBV	8518917	7971389	58.69%	9.554%
10	11.492	1559	1565	1568	rBV	4746481	3980570	29.31%	4.771%
11	13.086	1830	1836	1839	rBV	13146947	13582078	100.00%	16.278%
12	14.139	2011	2015	2019	rBV	3832188	3258052	23.99%	3.905%
13	15.274	2204	2208	2216	rVB	149024	166354	1.22%	0.199%
14	15.663	2269	2274	2284	rBV	2145938	2927843	21.56%	3.509%
15	16.139	2351	2355	2363	rVB	179313	260738	1.92%	0.312%
16	16.680	2442	2447	2456	rVB	142425	249470	1.84%	0.299%




Sum of corrected areas: 83437230

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129059.D
Acq On : 30 Jun 2022 15:24
Operator : CG\JU
Sample : PB145848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145848BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

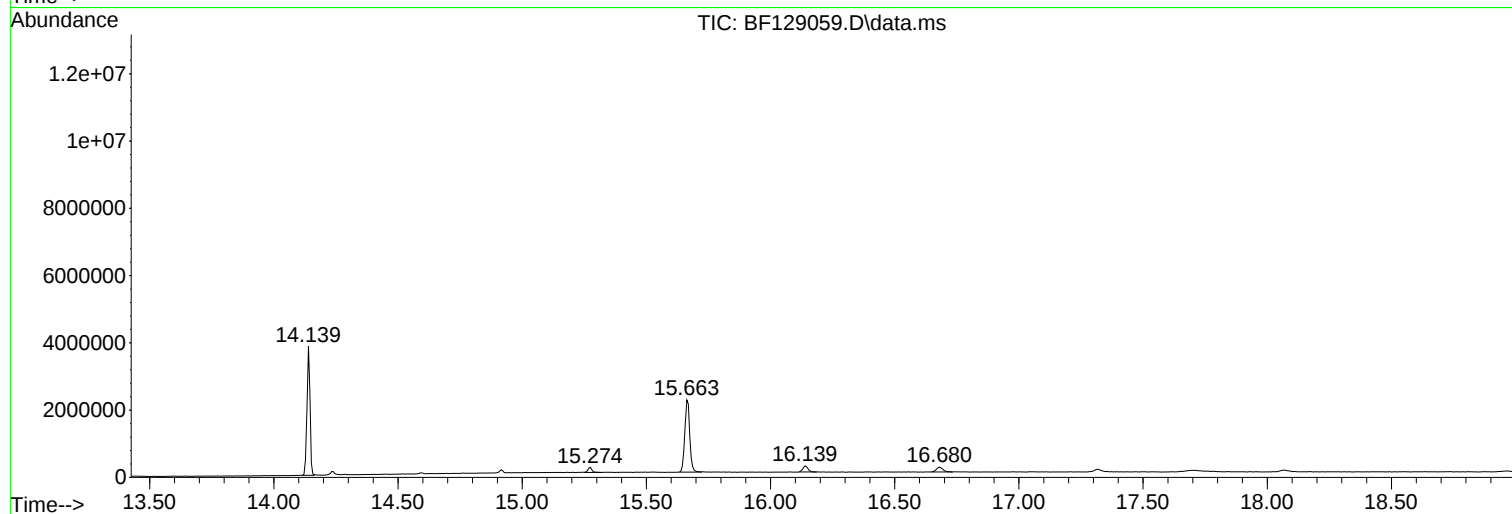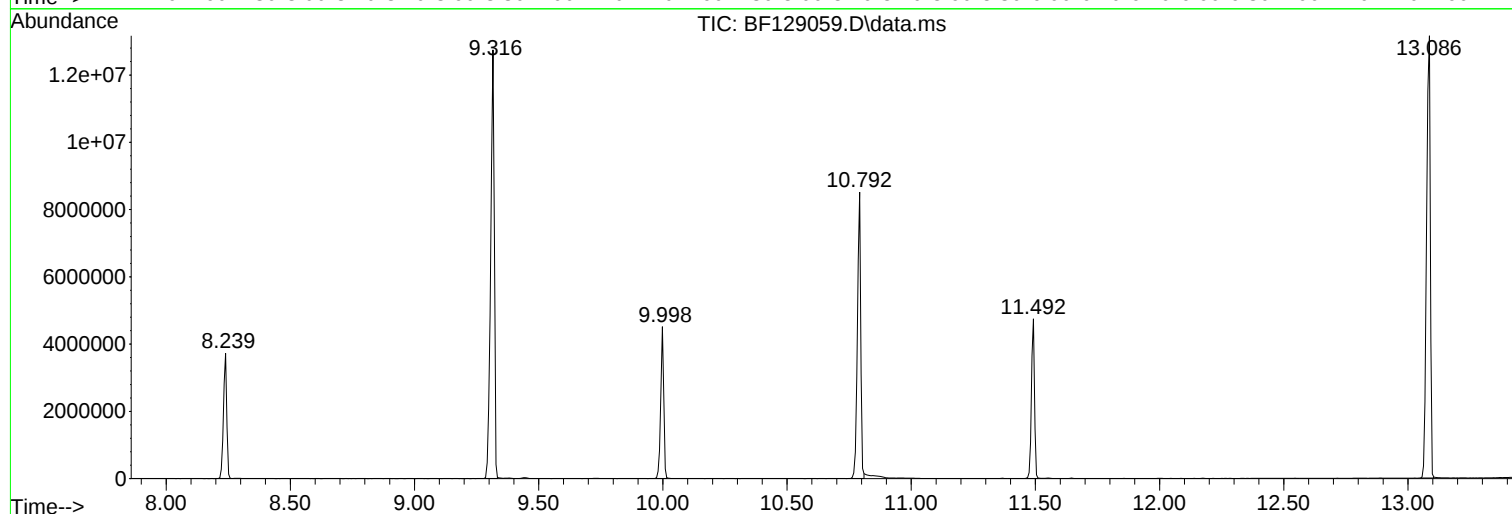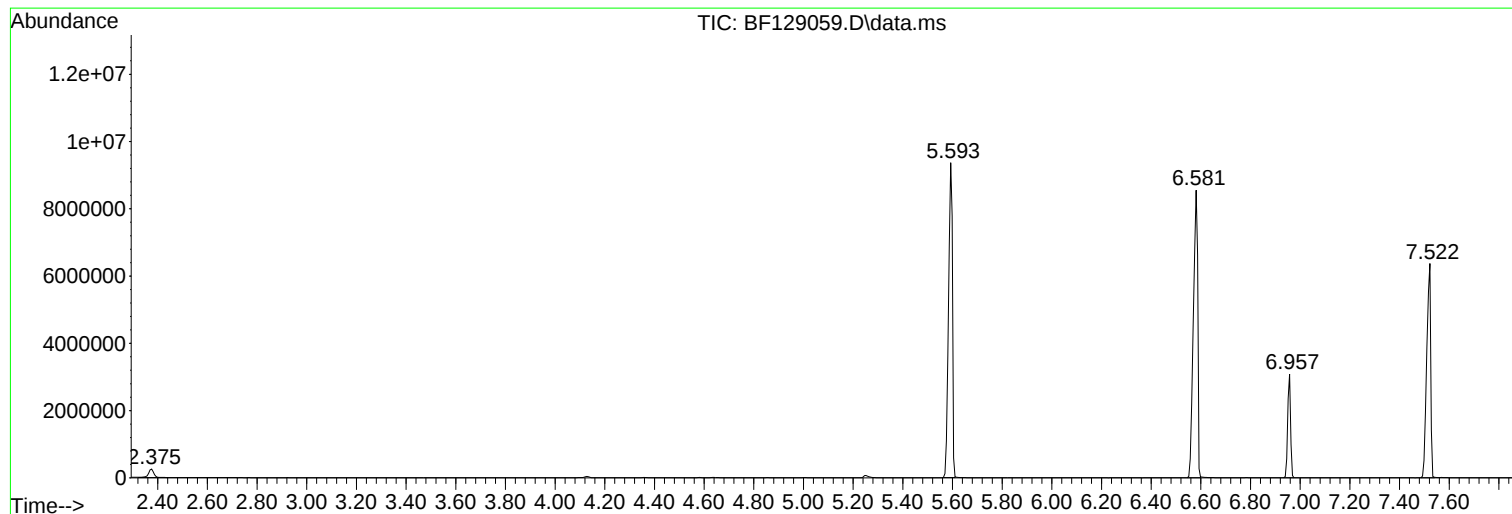

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129059.D
Acq On : 30 Jun 2022 15:24
Operator : CG\JU
Sample : PB145848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145848BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.375	2.96 ng	370502	1,4-Dichlorobenzene-d4	6.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

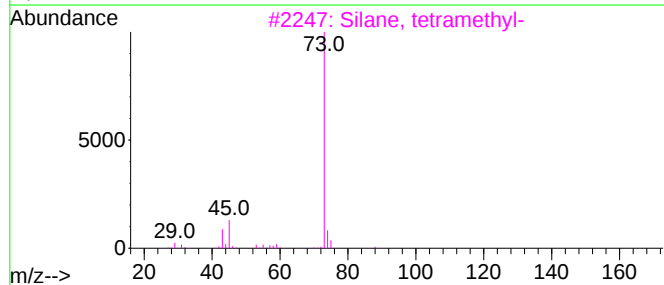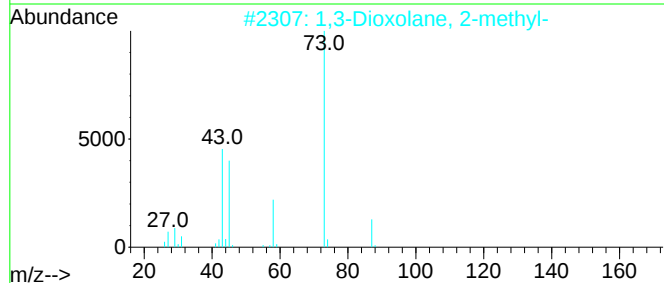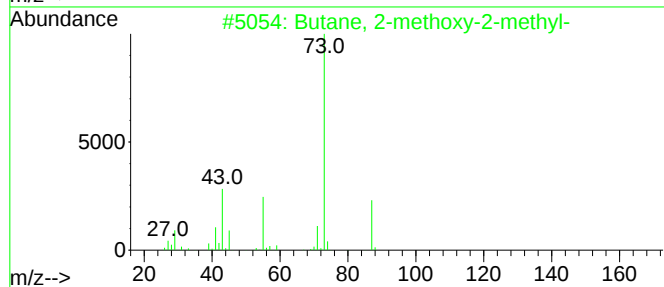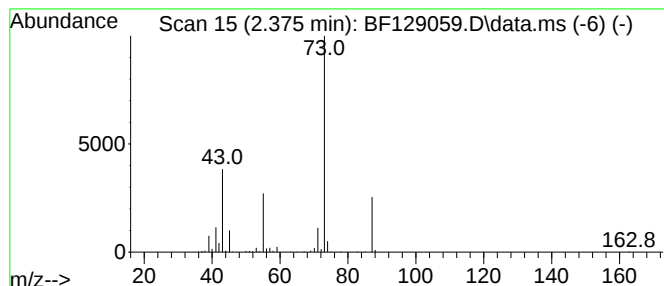

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129059.D
Acq On : 30 Jun 2022 15:24
Operator : CG\JU
Sample : PB145848BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145848BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.375	3.0	ng	370502	1	6.957	2504980	20.0