

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129060.D
 Acq On : 30 Jun 2022 15:56
 Operator : CG\JU
 Sample : N3434-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B2203-35

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.352	3	11	20	rVB	2454300	3220538	31.91%	4.433%
2	5.593	556	562	565	rBV	7990812	8423583	83.48%	11.595%
3	6.581	724	730	733	rBV	7816913	8446023	83.70%	11.626%
4	6.957	790	794	797	rBV	2863947	2324139	23.03%	3.199%
5	7.516	884	889	892	rBV	5138795	5575993	55.26%	7.675%
6	8.239	1007	1012	1015	rBV	3617425	3091065	30.63%	4.255%
7	9.316	1189	1195	1198	rBV	10941411	10050905	99.60%	13.835%
8	9.998	1305	1311	1314	rBV	4209671	3474718	34.43%	4.783%
9	10.792	1438	1446	1449	rBV	6904795	6718805	66.58%	9.248%
10	11.492	1560	1565	1568	rBV	4080506	3597444	35.65%	4.952%
11	12.004	1645	1652	1655	rBV	294324	298811	2.96%	0.411%
12	12.792	1780	1786	1797	rBV	112327	167028	1.66%	0.230%
13	13.080	1830	1835	1838	rBV	10520881	10090995	100.00%	13.890%
14	13.557	1911	1916	1921	rBV	139332	161609	1.60%	0.222%
15	14.021	1990	1995	2005	rBV	115144	278942	2.76%	0.384%
16	14.139	2011	2015	2019	rBV	3745621	3169369	31.41%	4.363%
17	14.233	2026	2031	2036	rBV	210622	261249	2.59%	0.360%
18	14.915	2141	2147	2155	rBV2	149856	241103	2.39%	0.332%
19	15.274	2204	2208	2213	rVB	135320	167697	1.66%	0.231%
20	15.662	2269	2274	2285	rVB	2146170	2889909	28.64%	3.978%




Sum of corrected areas: 72649925

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129060.D
Acq On : 30 Jun 2022 15:56
Operator : CG\JU
Sample : N3434-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B2203-35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

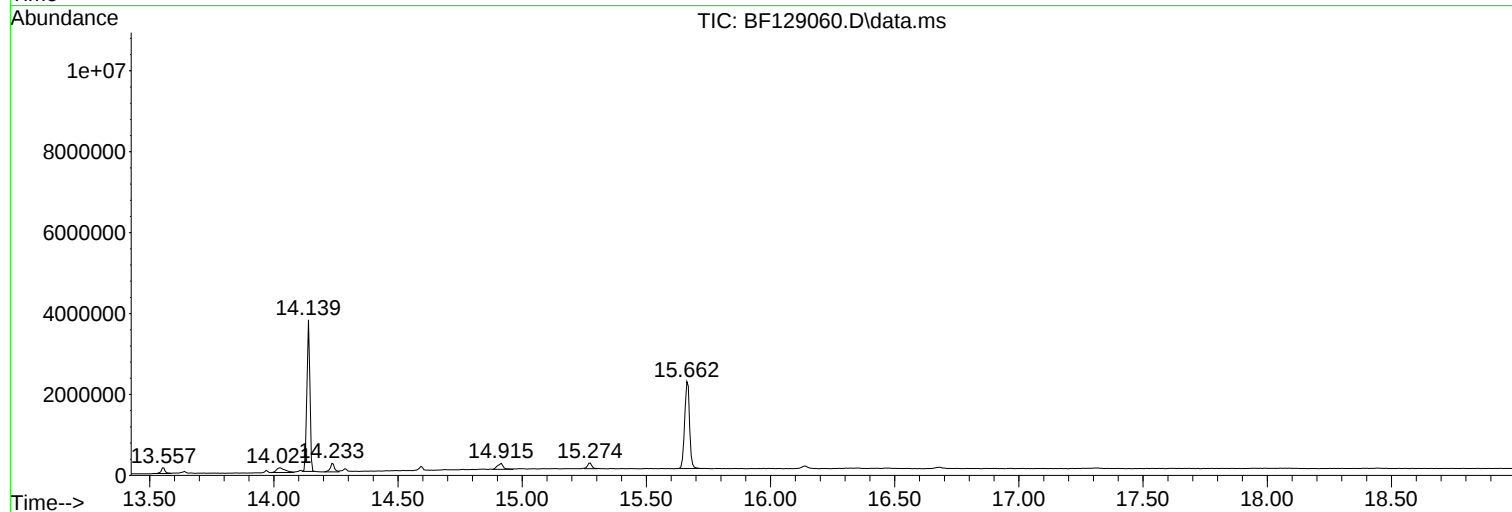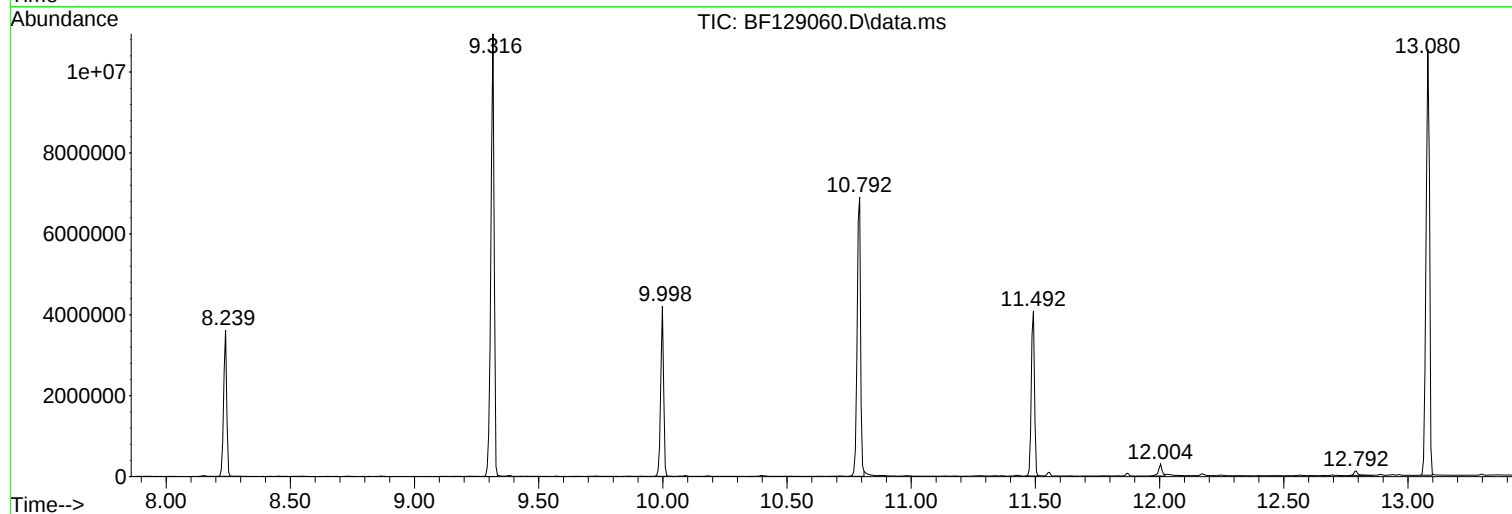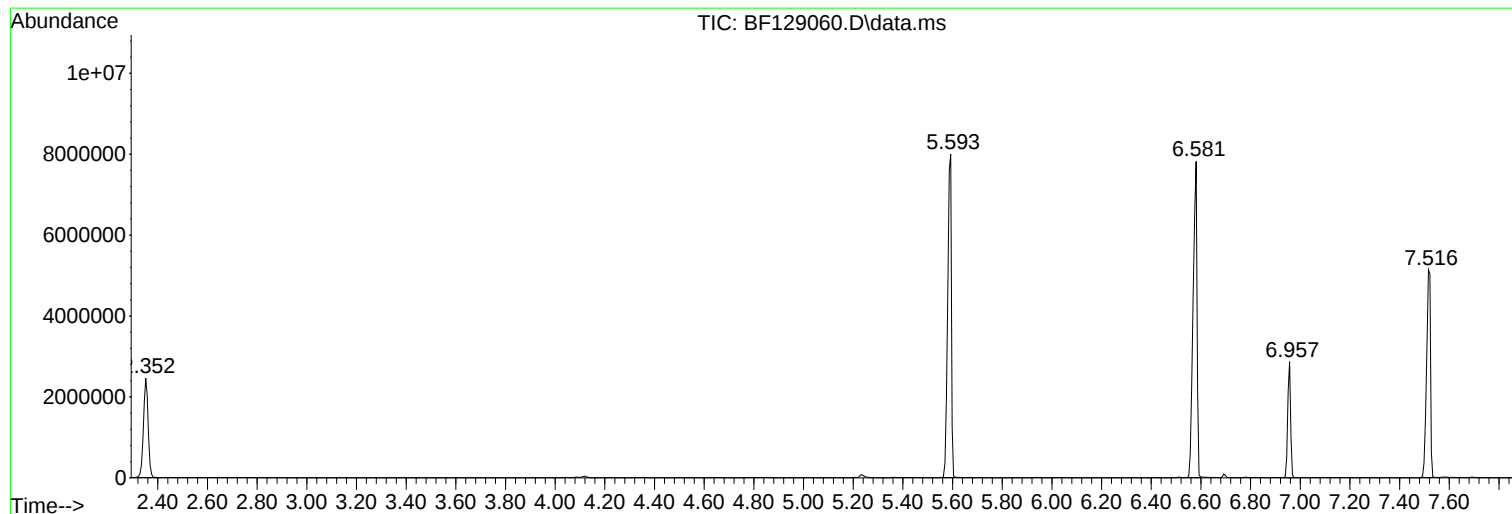

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129060.D
Acq On : 30 Jun 2022 15:56
Operator : CG\JU
Sample : N3434-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B2203-35










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.352	27.71 ng	3220540	1,4-Dichlorobenzene-d4	6.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12

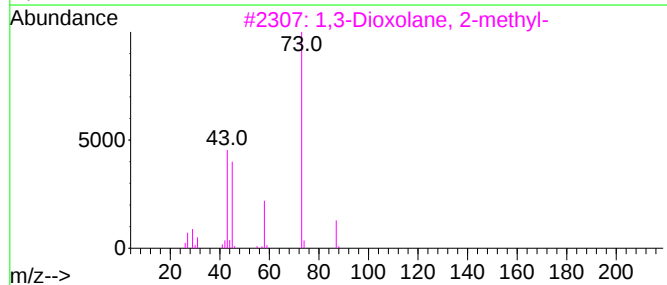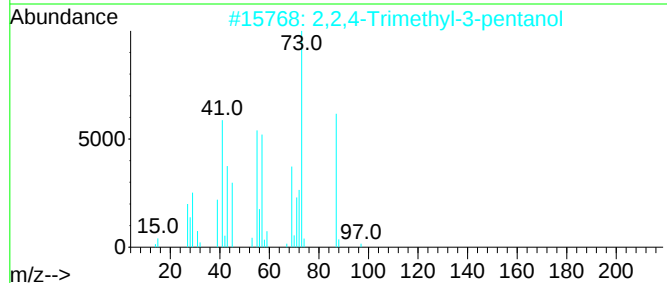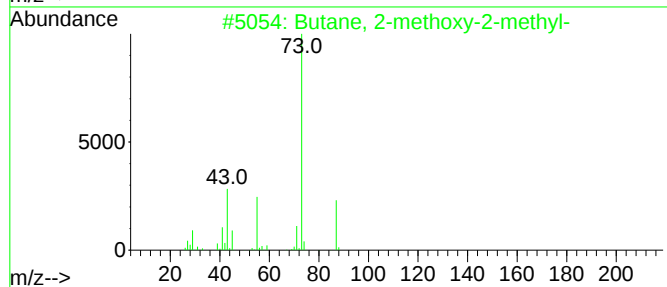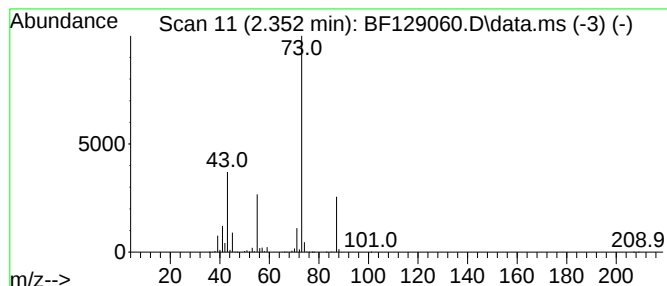

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129060.D
Acq On : 30 Jun 2022 15:56
Operator : CG\JU
Sample : N3434-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B2203-35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.352	27.7	ng	3220540	1	6.957	2324140	20.0