


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129047.D
 Acq On : 30 Jun 2022 09:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

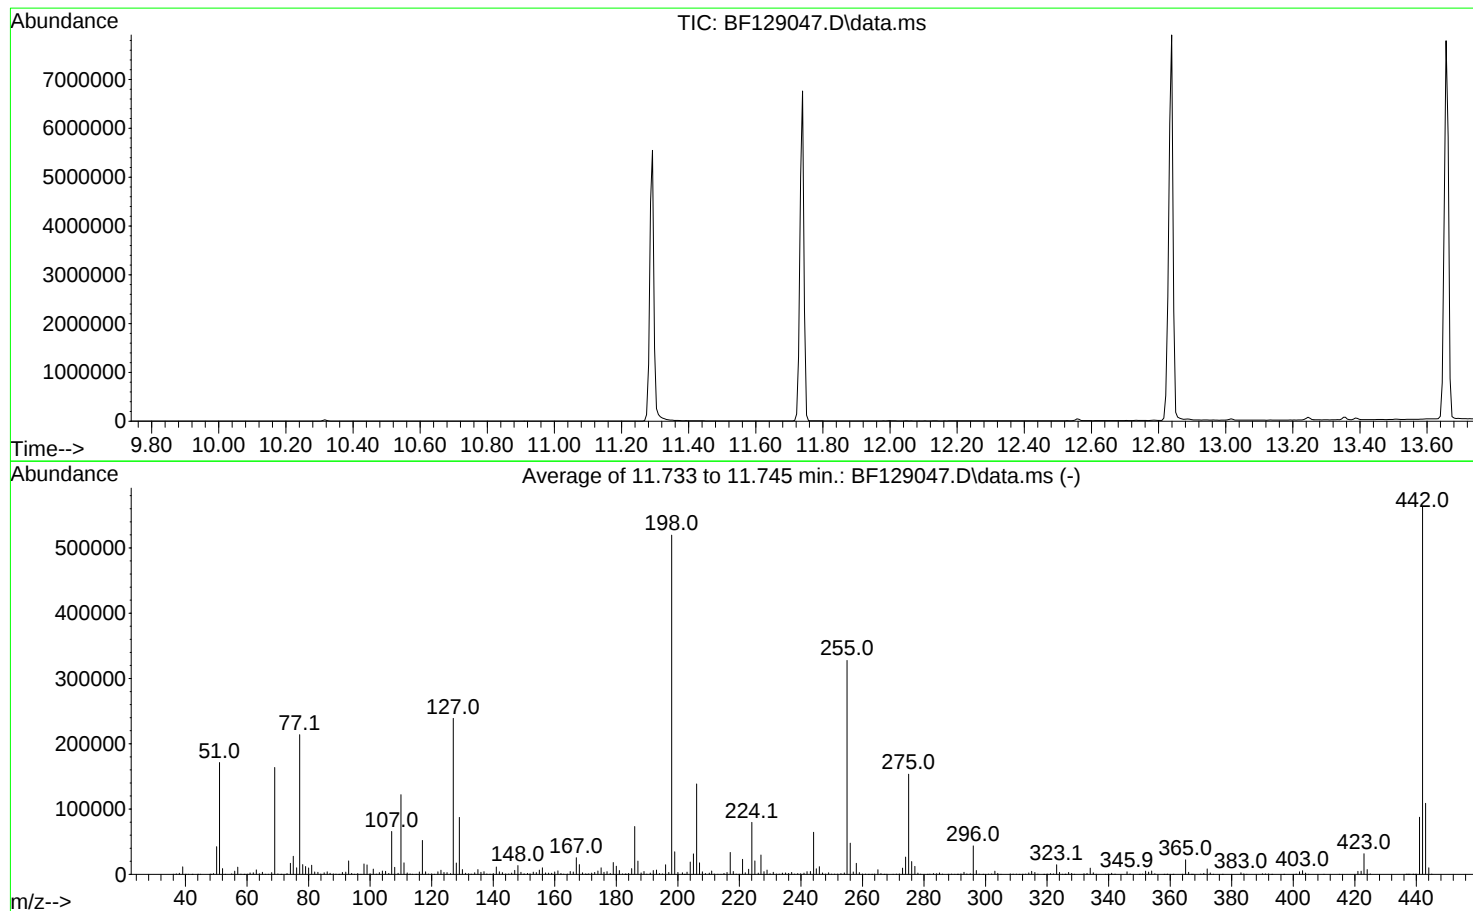




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	171301	PASS
68	69	0.00	2	1.7	2703	PASS
69	198	0.00	100	31.5	163619	PASS
70	69	0.00	2	0.4	717	PASS
127	198	10	80	46.0	238877	PASS
197	198	0.00	2	0.6	2890	PASS
198	198	100	100	100.0	519595	PASS
199	198	5	9	6.7	34601	PASS
275	198	10	60	29.5	153499	PASS
365	198	1	100	4.3	22365	PASS
441	198	0.01	100	16.9	87637	PASS
442	442	50	100	100.0	563456	PASS
443	442	15	24	19.3	108880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129047.D
 Acq On : 30 Jun 2022 09:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 01 08:53:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

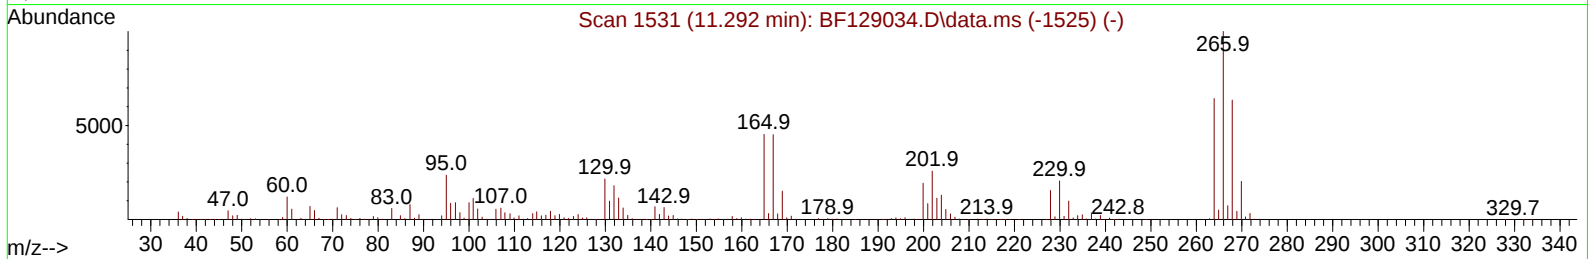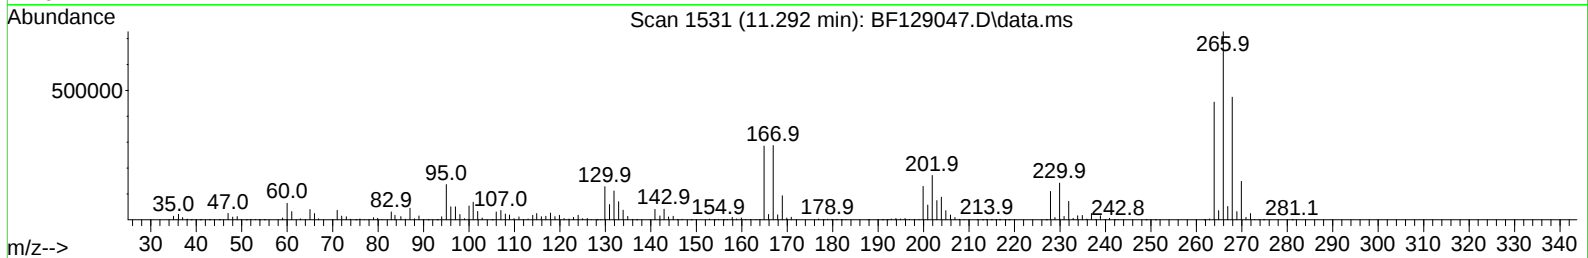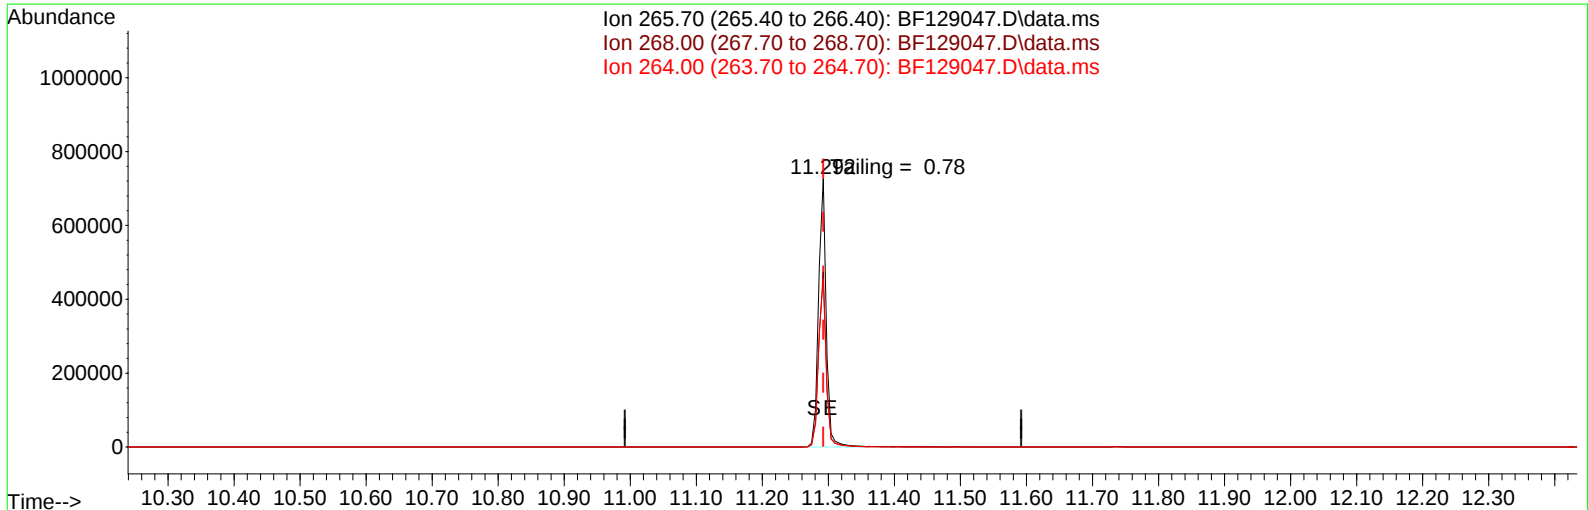

TIC: BF129047.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 525423.01 ng




response 593101

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.18
264.00	61.80	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129047.D
 Acq On : 30 Jun 2022 09:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 01 08:53:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

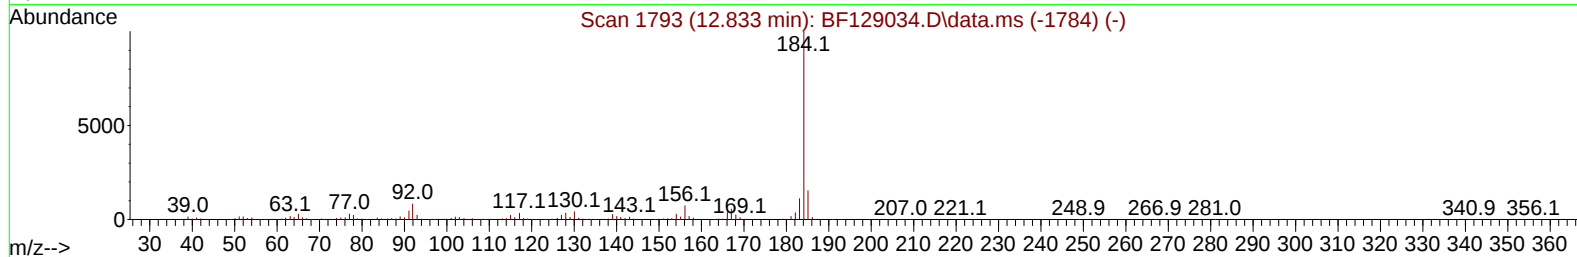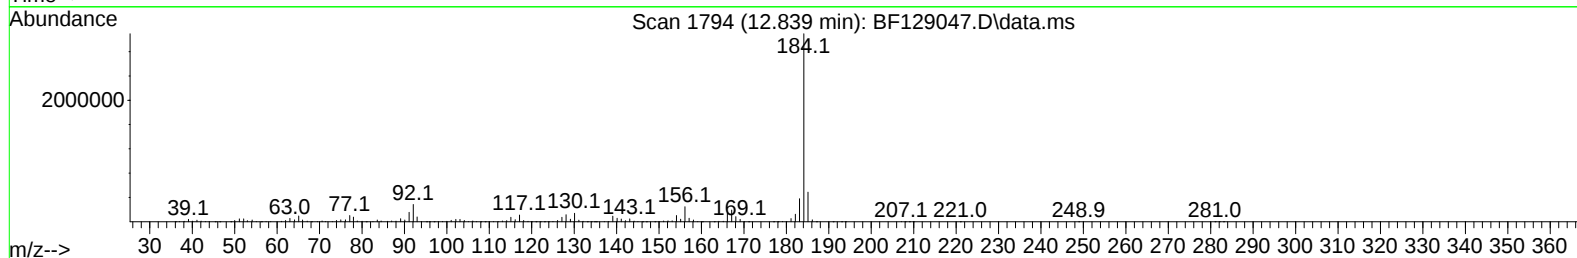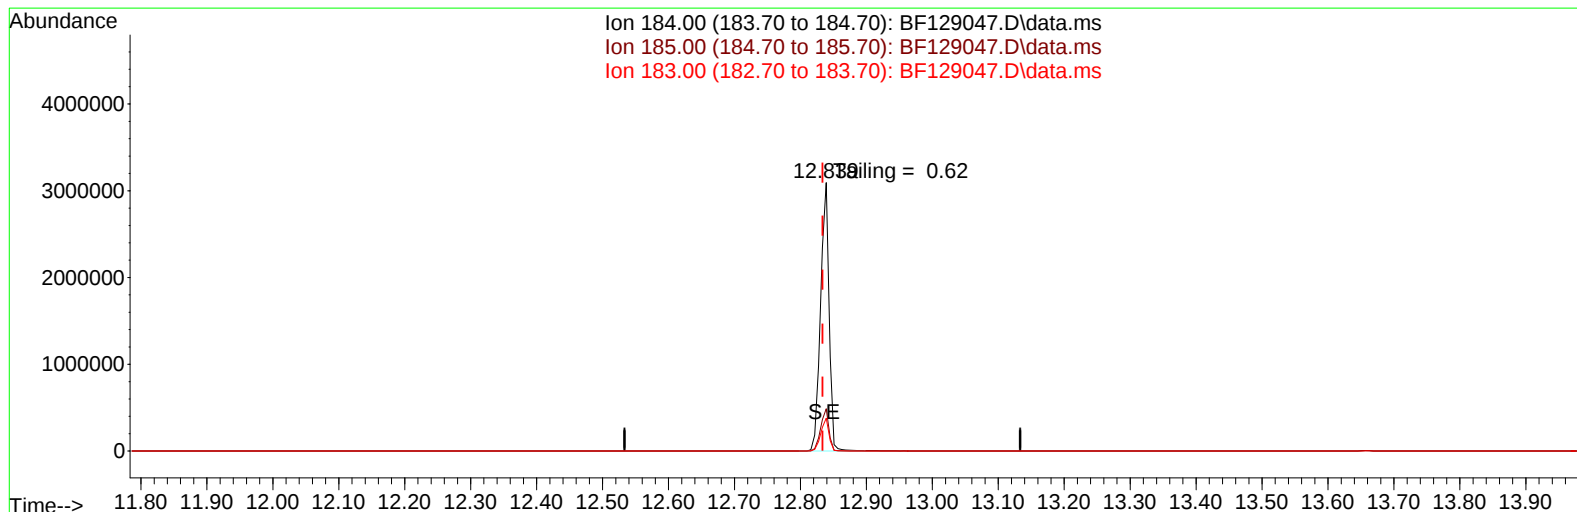

TIC: BF129047.D\data.ms

(77) Benzidine

12.839min (+ 0.006) 401790.97 ng

response 2790226

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.74
183.00	11.60	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2022	BNA_F	<u>BF129047.D</u>
Compound Name	Response	Retention Time
DDT	1319283	13.657
DDD	13247	13.357
DDE	2947	13.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16194	1335477	1.21

Instrument :
BNA_F
ClientSampleId :
DFTPP