
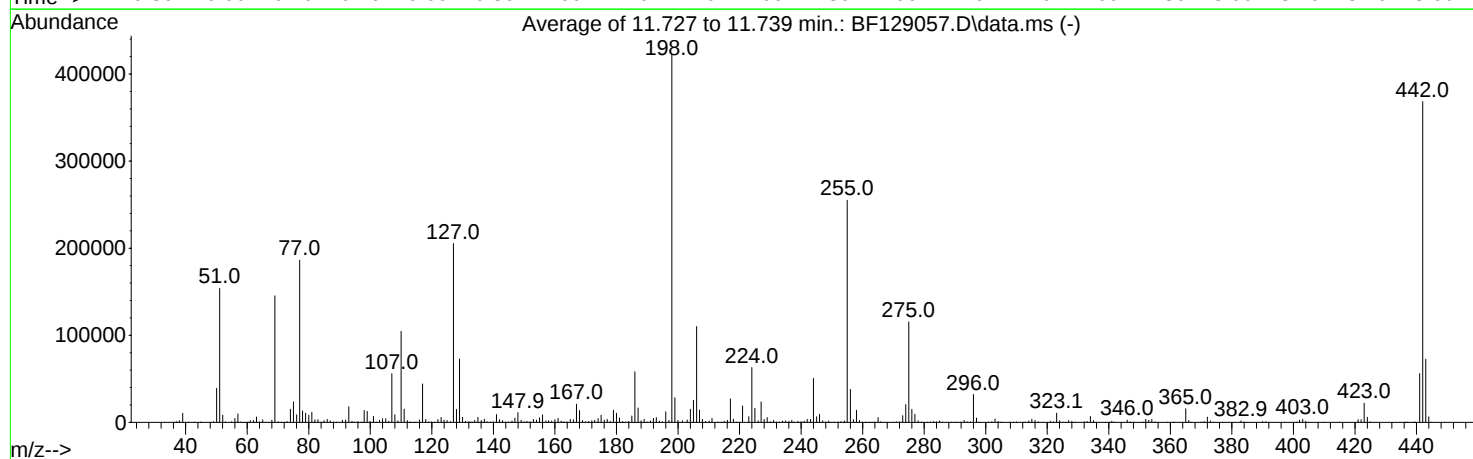


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
 Data File : BF129057.D
 Acq On : 30 Jun 2022 14:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

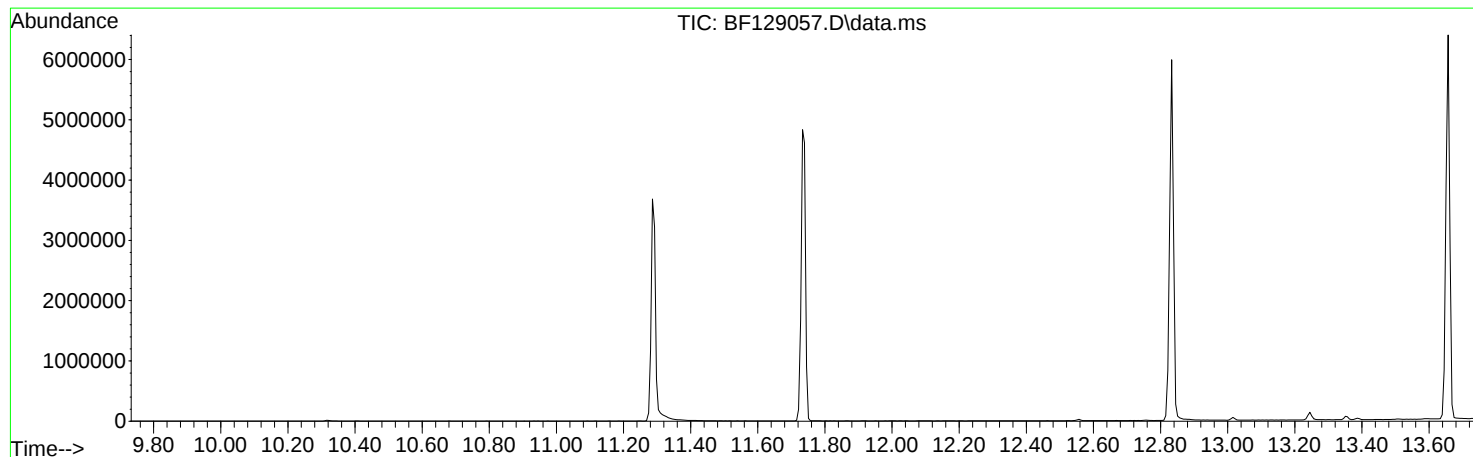




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	153881	PASS
68	69	0.00	2	1.8	2608	PASS
69	198	0.00	100	34.4	145331	PASS
70	69	0.00	2	0.5	798	PASS
127	198	10	80	48.7	205531	PASS
197	198	0.00	2	0.5	2244	PASS
198	198	100	100	100.0	422443	PASS
199	198	5	9	6.7	28301	PASS
275	198	10	60	27.3	115373	PASS
365	198	1	100	3.7	15641	PASS
441	198	0.01	100	13.3	56062	PASS
442	442	50	100	100.0	368488	PASS
443	442	15	24	19.7	72681	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129057.D
Acq On : 30 Jun 2022 14:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 01 08:55:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

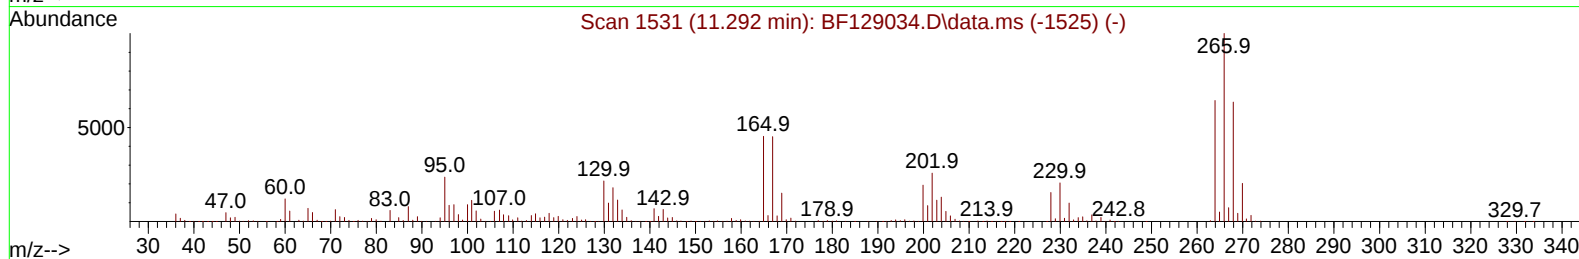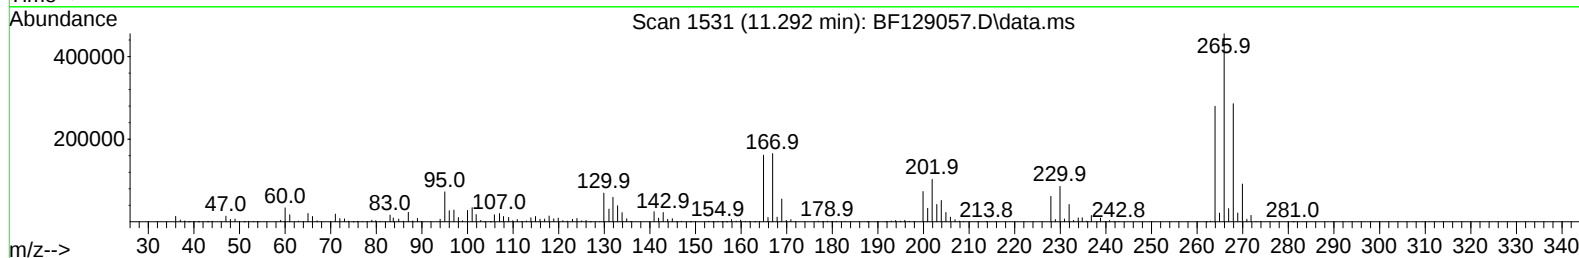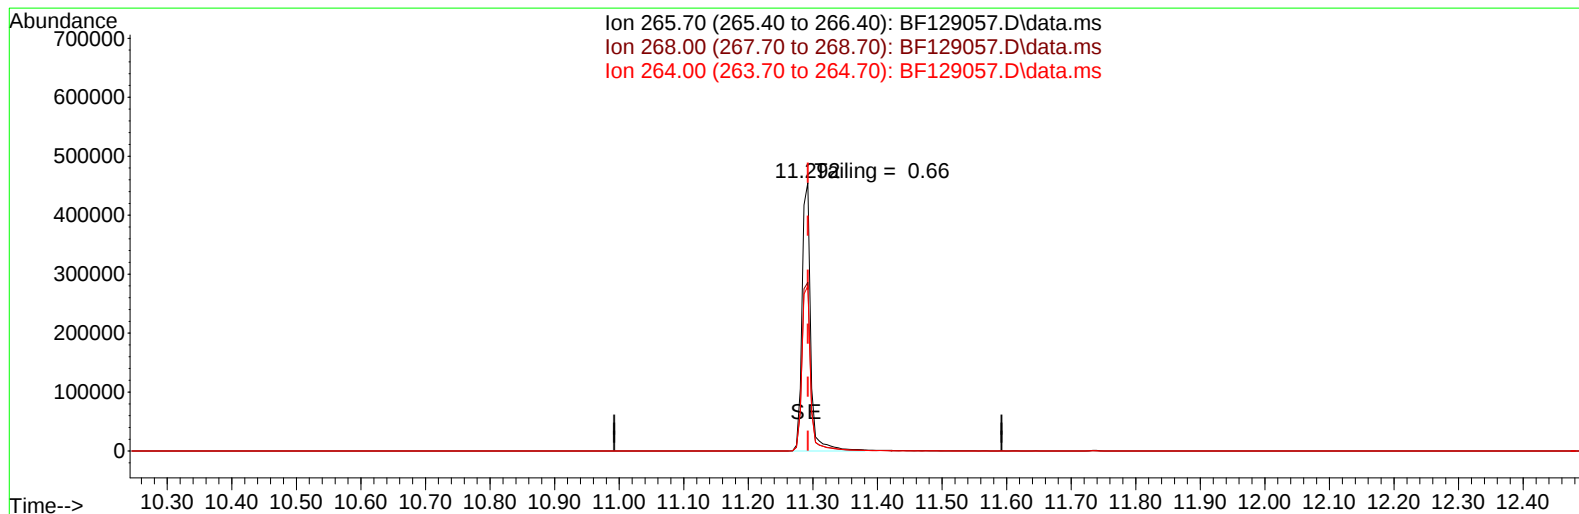

TIC: BF129057.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 192430.21 ng




response 427645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.83
264.00	61.80	61.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063022\
Data File : BF129057.D
Acq On : 30 Jun 2022 14:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 01 08:55:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

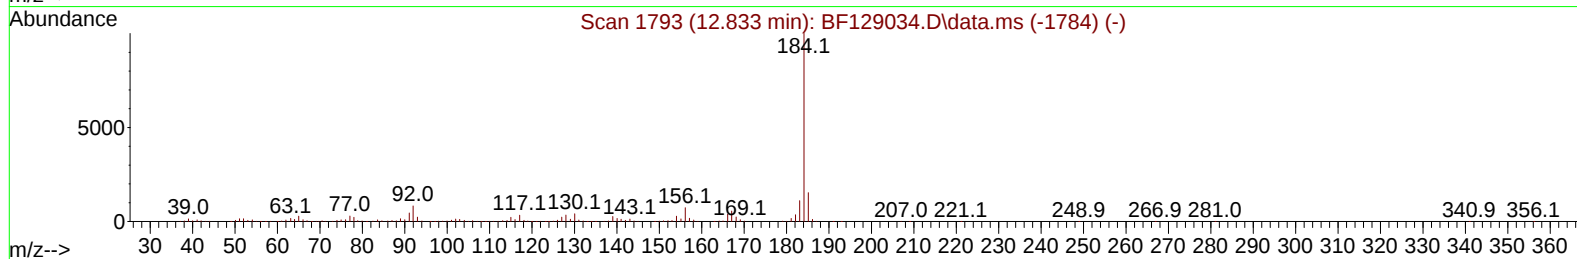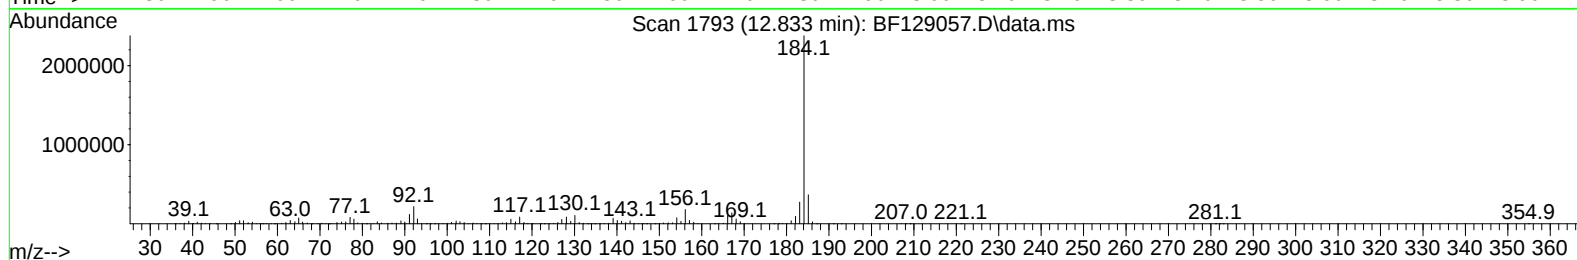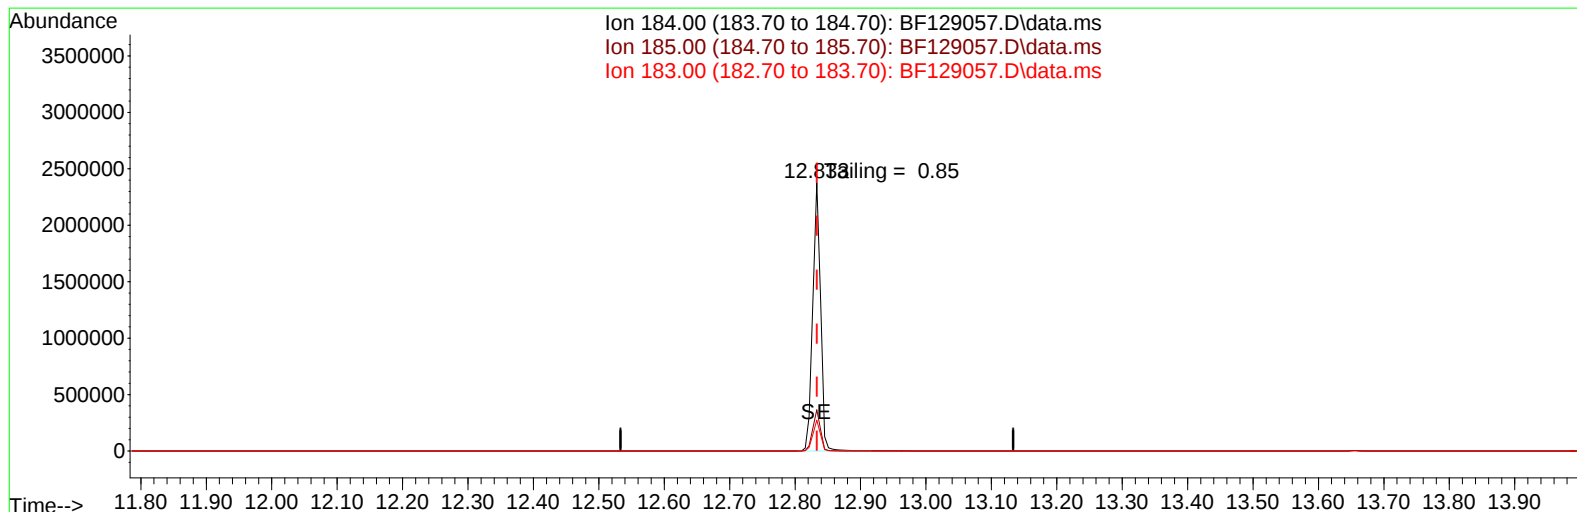

TIC: BF129057.D\data.ms

(77) Benzidine

12.833min (-0.000) 441893.12 ng

response 1990730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.40
183.00	11.60	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2022	BNA_F	<u>BF129057.D</u>
Compound Name	Response	Retention Time
DDT	980949	13.657
DDD	12414	13.351
DDE	4625	13.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17039	997988	1.71

Instrument :
BNA_F
ClientSampleId :
DFTPP