
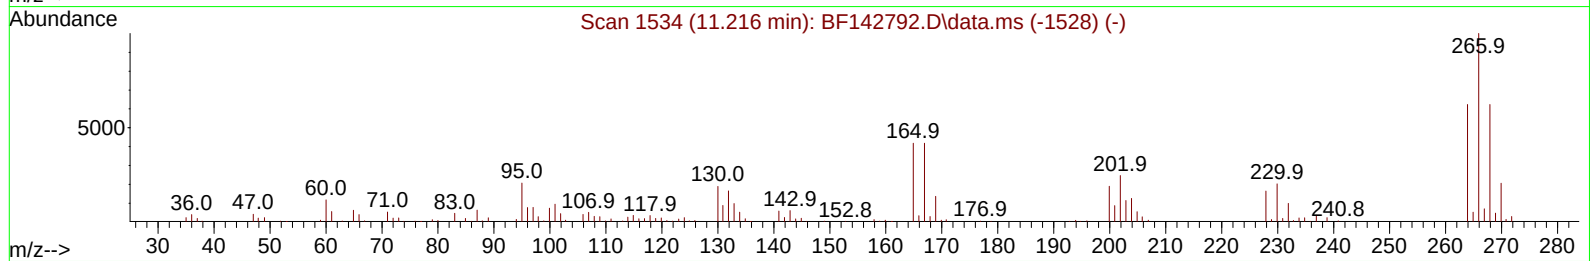
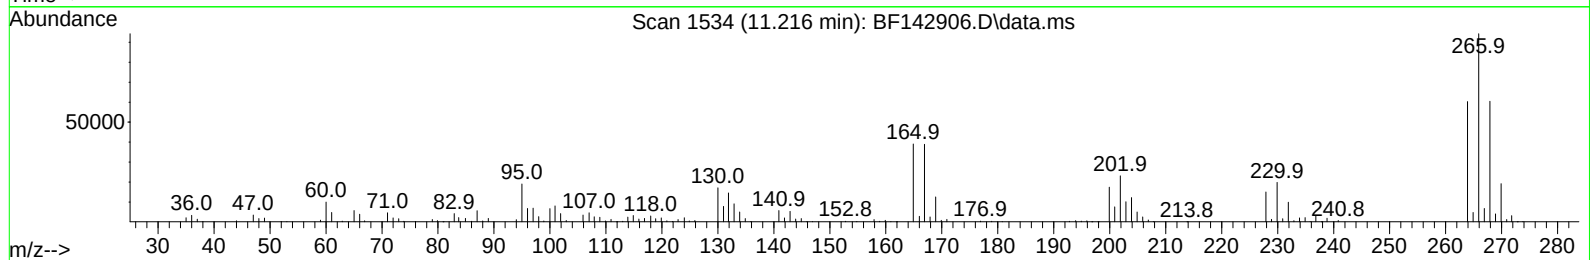


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142906.D
Acq On : 30 Jun 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 12:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

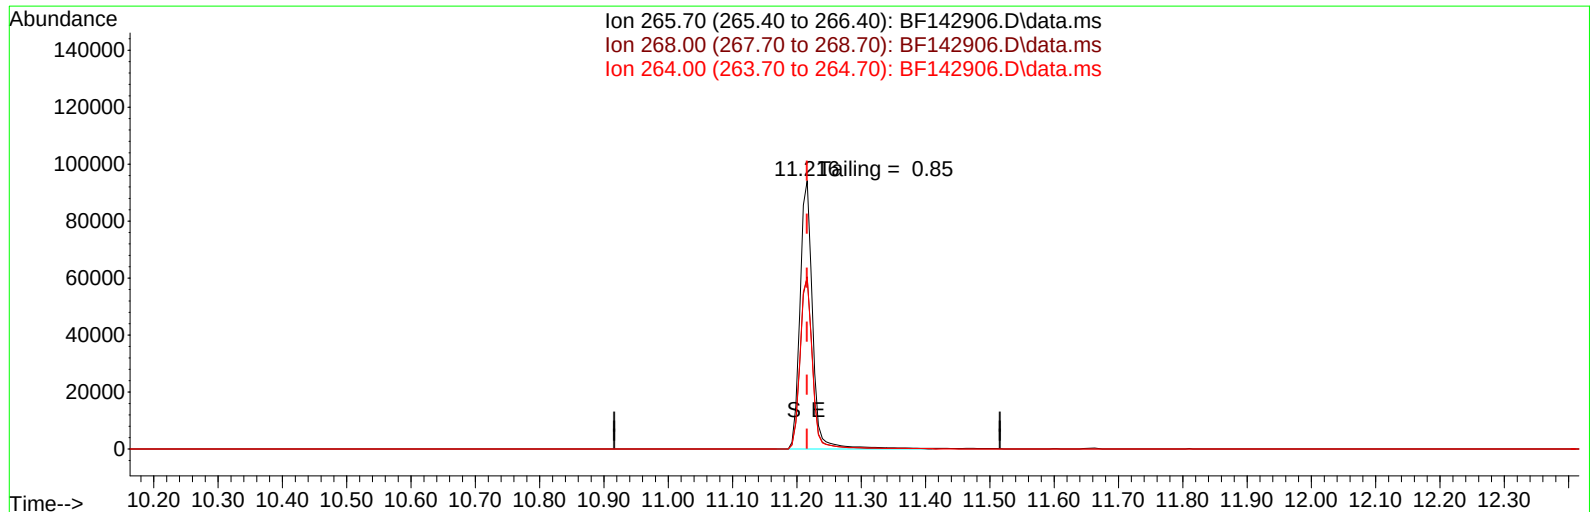

TIC: BF142906.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.000) 31918.23 ng

response 129732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.13
264.00	62.40	63.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142906.D
Acq On : 30 Jun 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 12:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

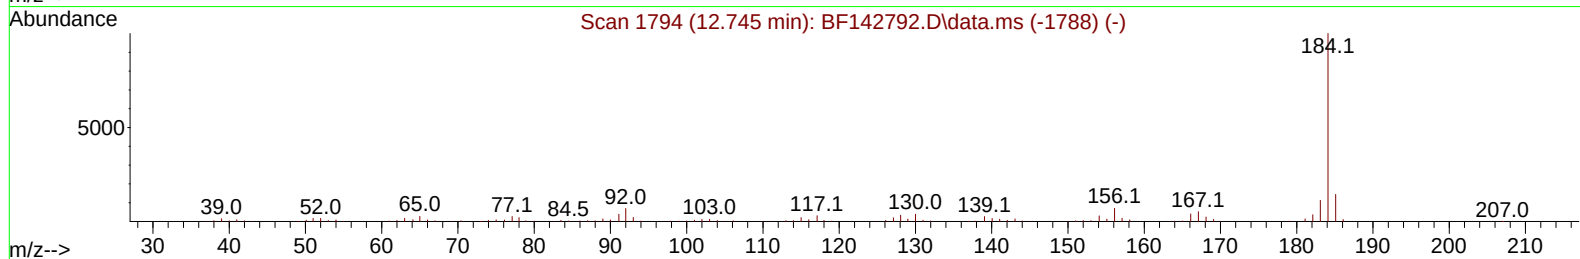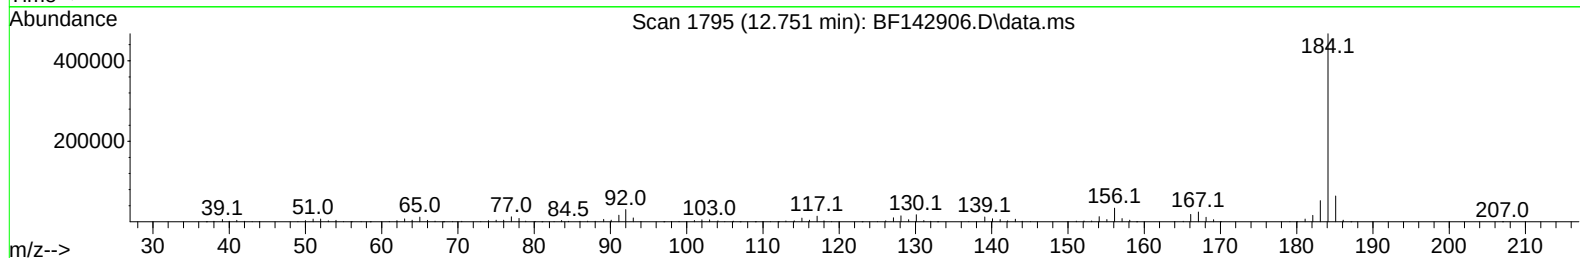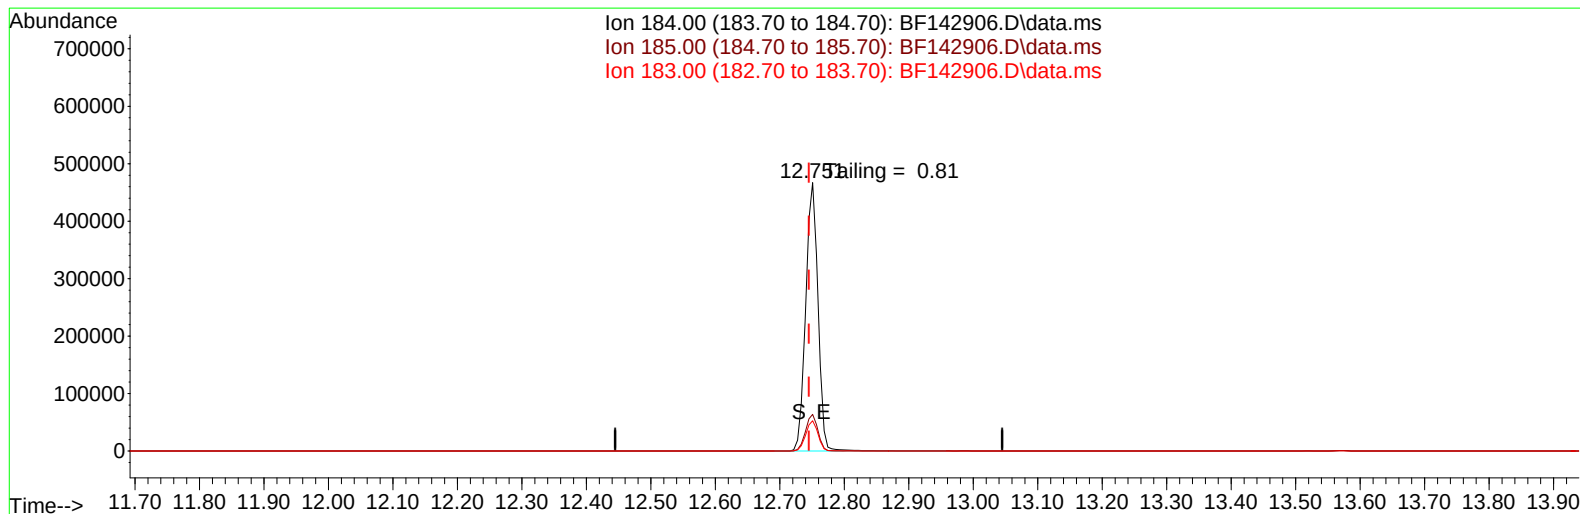

TIC: BF142906.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 620836

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.70
183.00	11.20	11.28
0.00	0.00	0.00