
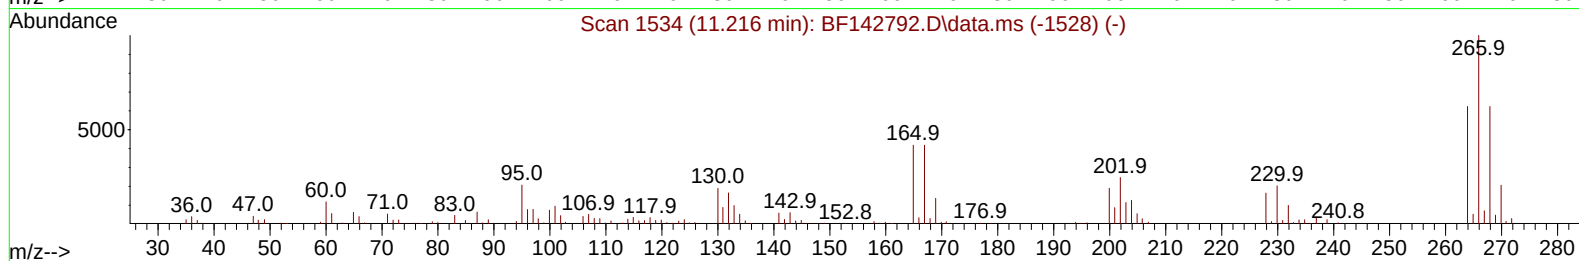
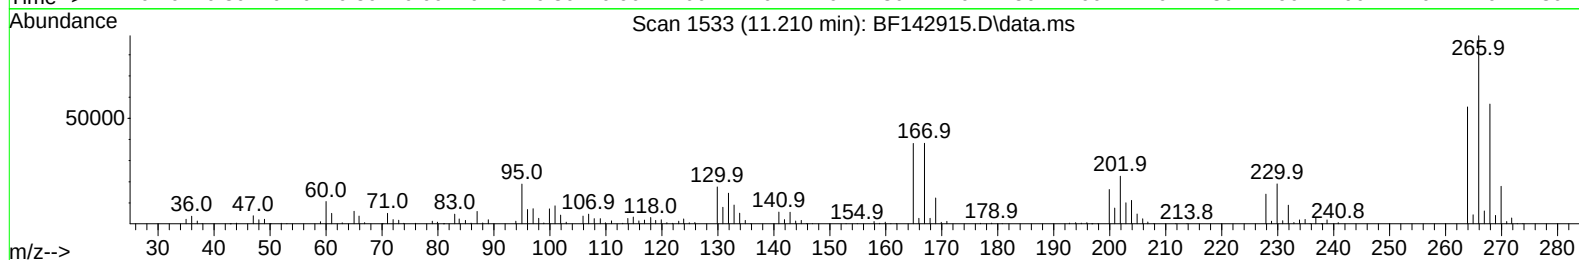


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142915.D
Acq On : 30 Jun 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 15:46:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

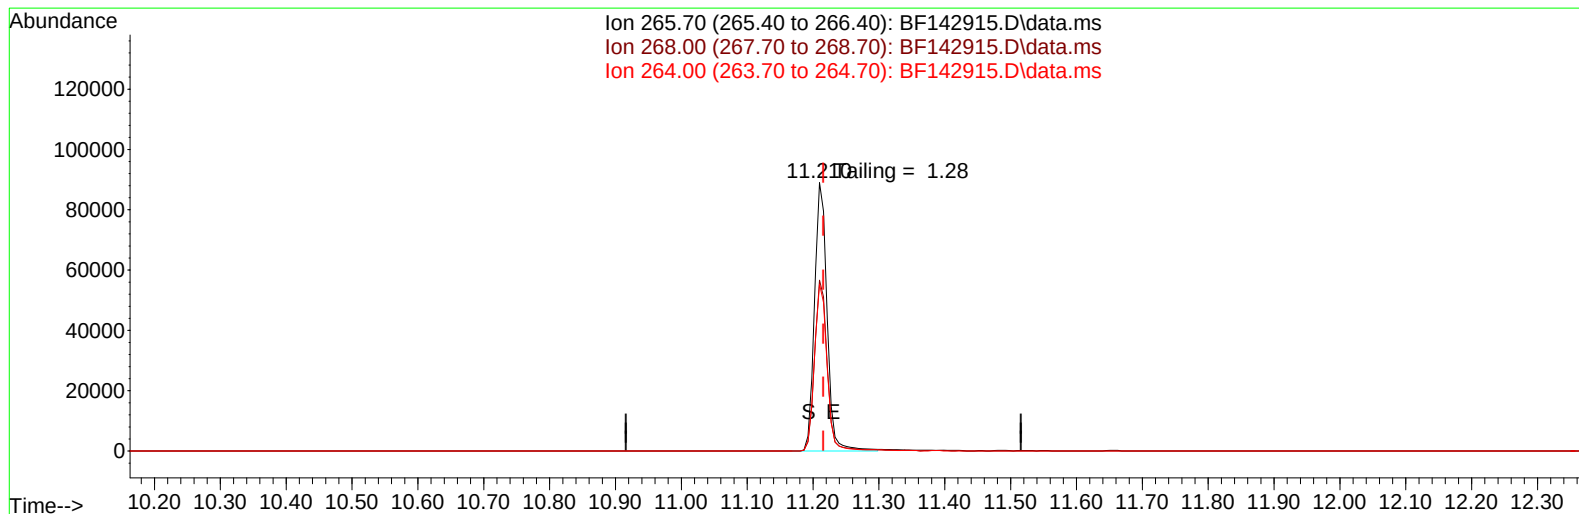

TIC: BF142915.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 37500.34 ng

response 119337

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.69
264.00	62.40	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142915.D
Acq On : 30 Jun 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 15:46:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

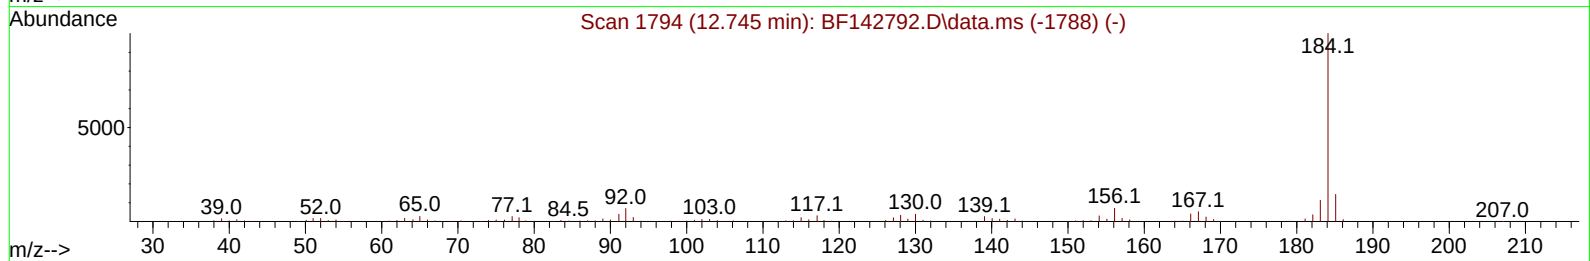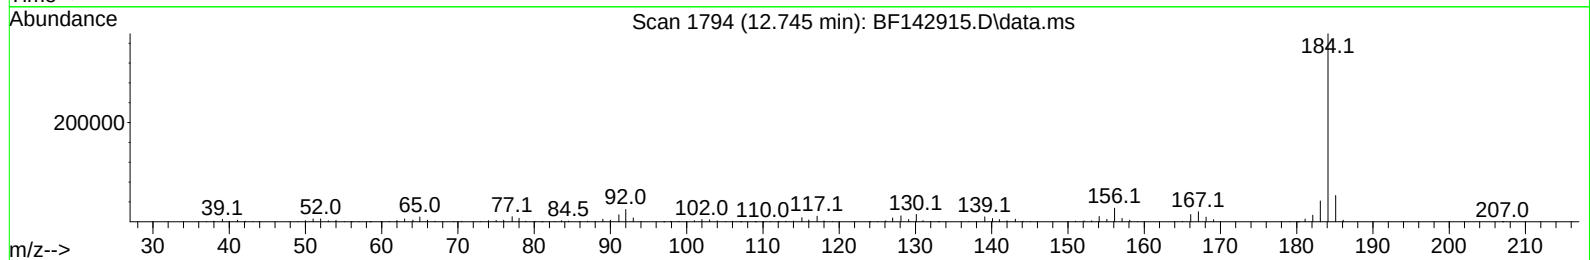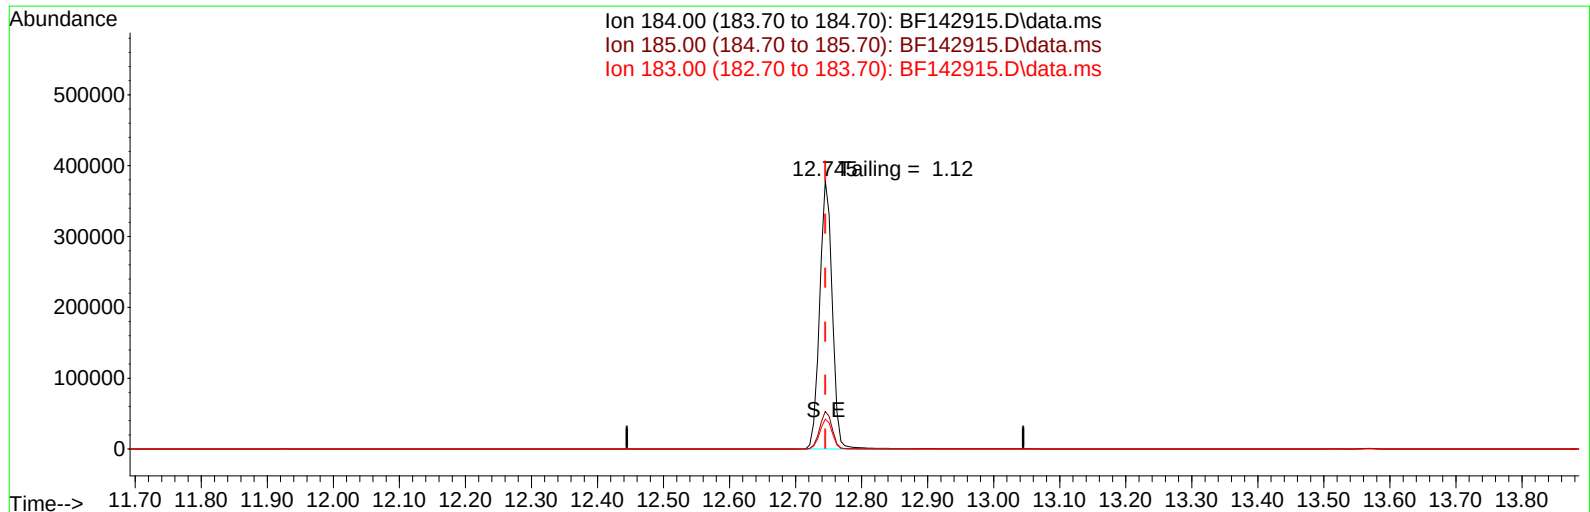

TIC: BF142915.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 501451

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.02
183.00	11.20	11.14
0.00	0.00	0.00