


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142906.D
Acq On : 30 Jun 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

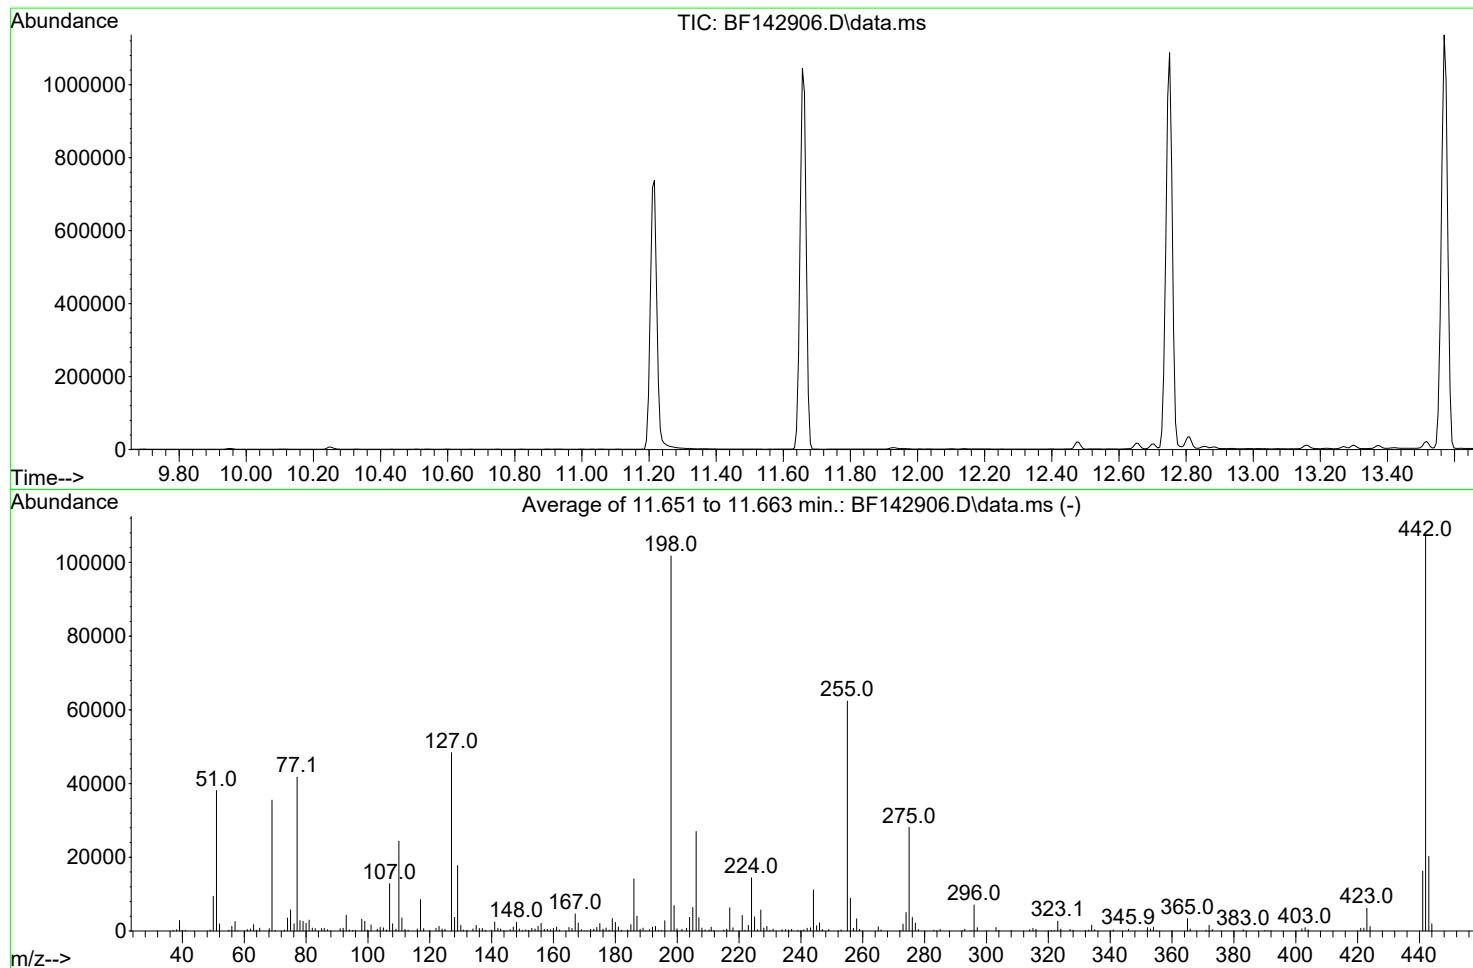

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	666	PASS
69	69	100	100	100.0	35523	PASS
70	69	0.00	2	0.6	196	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101768	PASS
199	198	5	9	6.8	6914	PASS
365	198	1	100	3.4	3411	PASS
441	443	0.01	150	80.4	16252	PASS
442	442	100	100	100.0	107117	PASS
443	442	15	24	18.9	20219	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/30/2025	BNA_F	<u>BF142906.D</u>
Compound Name	Response	Retention Time
DDT	303517	13.569
DDD	5711	13.298
DDE	396	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6107	309624	1.97

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142906.D
Acq On : 30 Jun 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 12:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

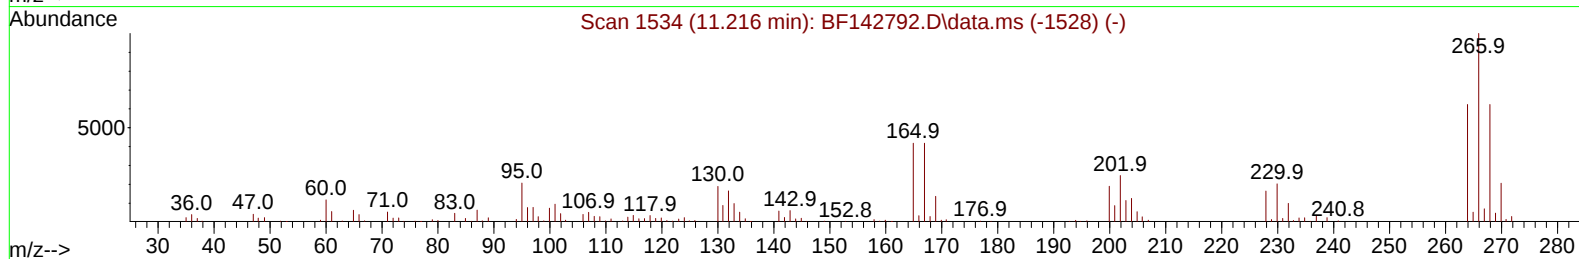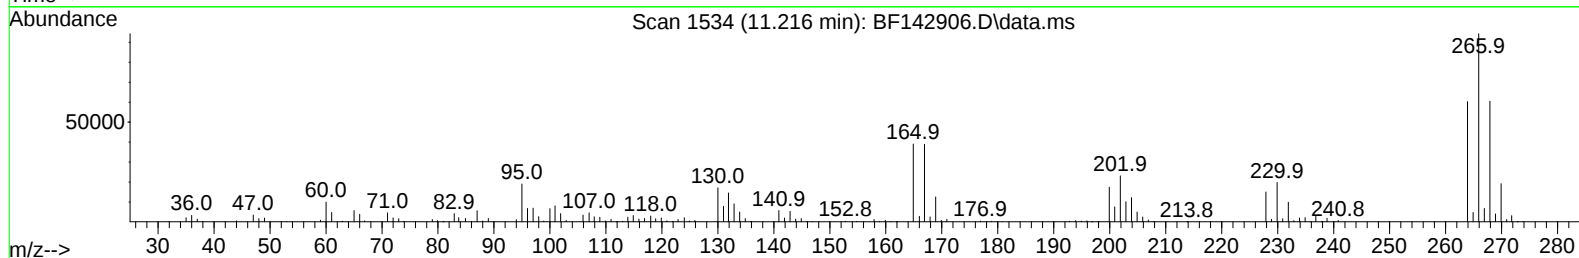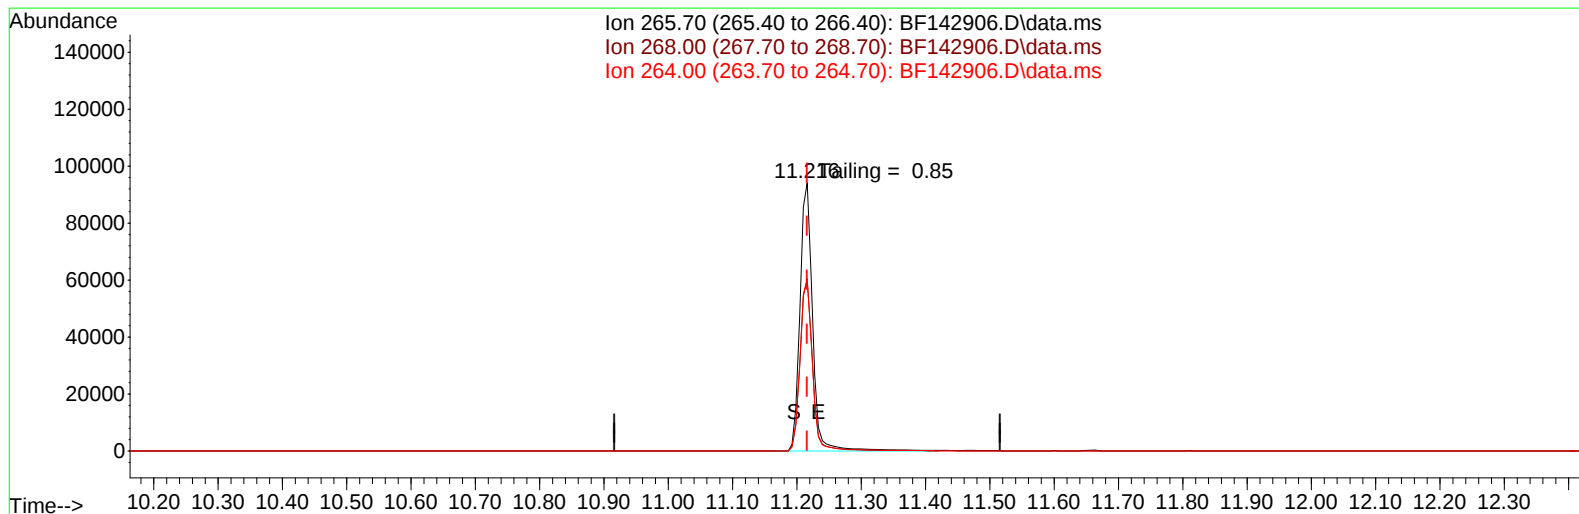

TIC: BF142906.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 31918.23 ng




response 129732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.13
264.00	62.40	63.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142906.D
Acq On : 30 Jun 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 12:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

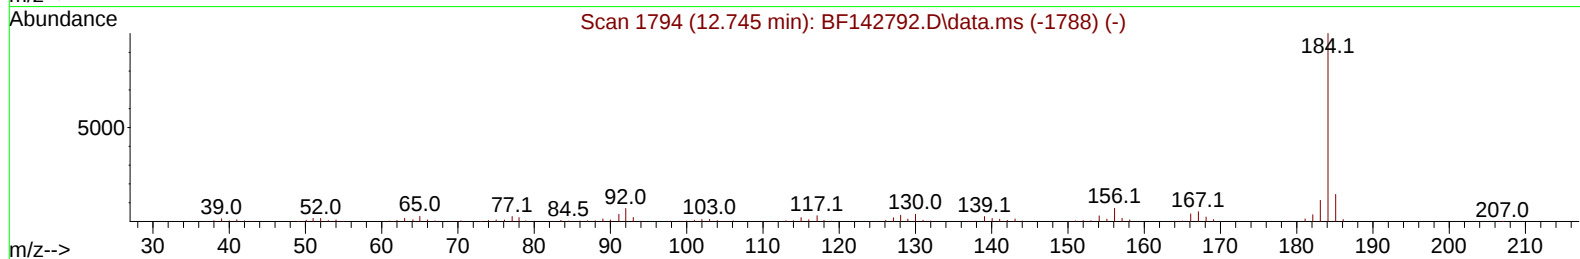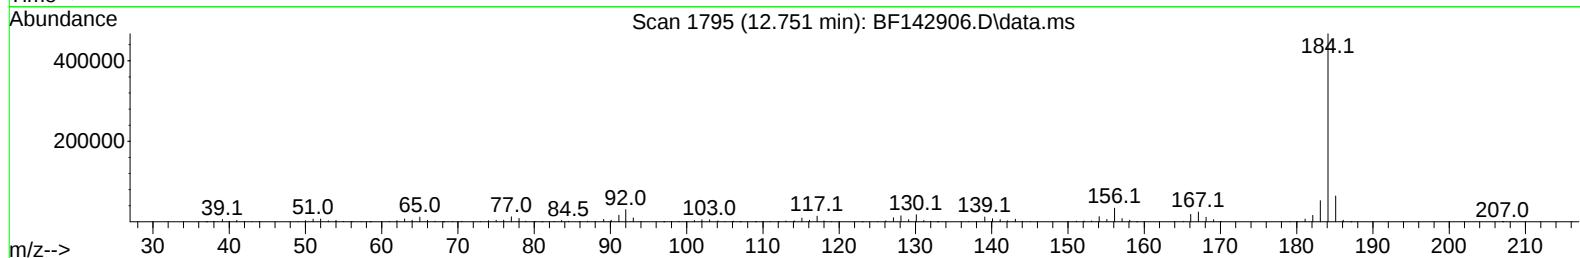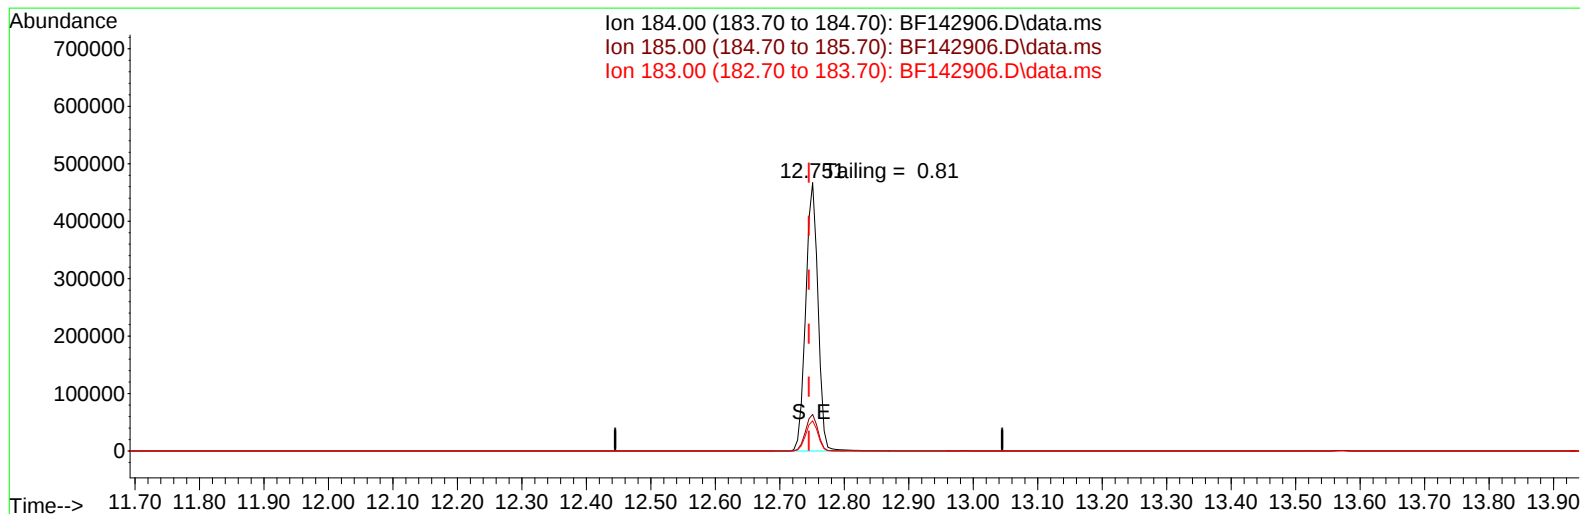

TIC: BF142906.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 620836

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.70
183.00	11.20	11.28
0.00	0.00	0.00