


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142915.D
Acq On : 30 Jun 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

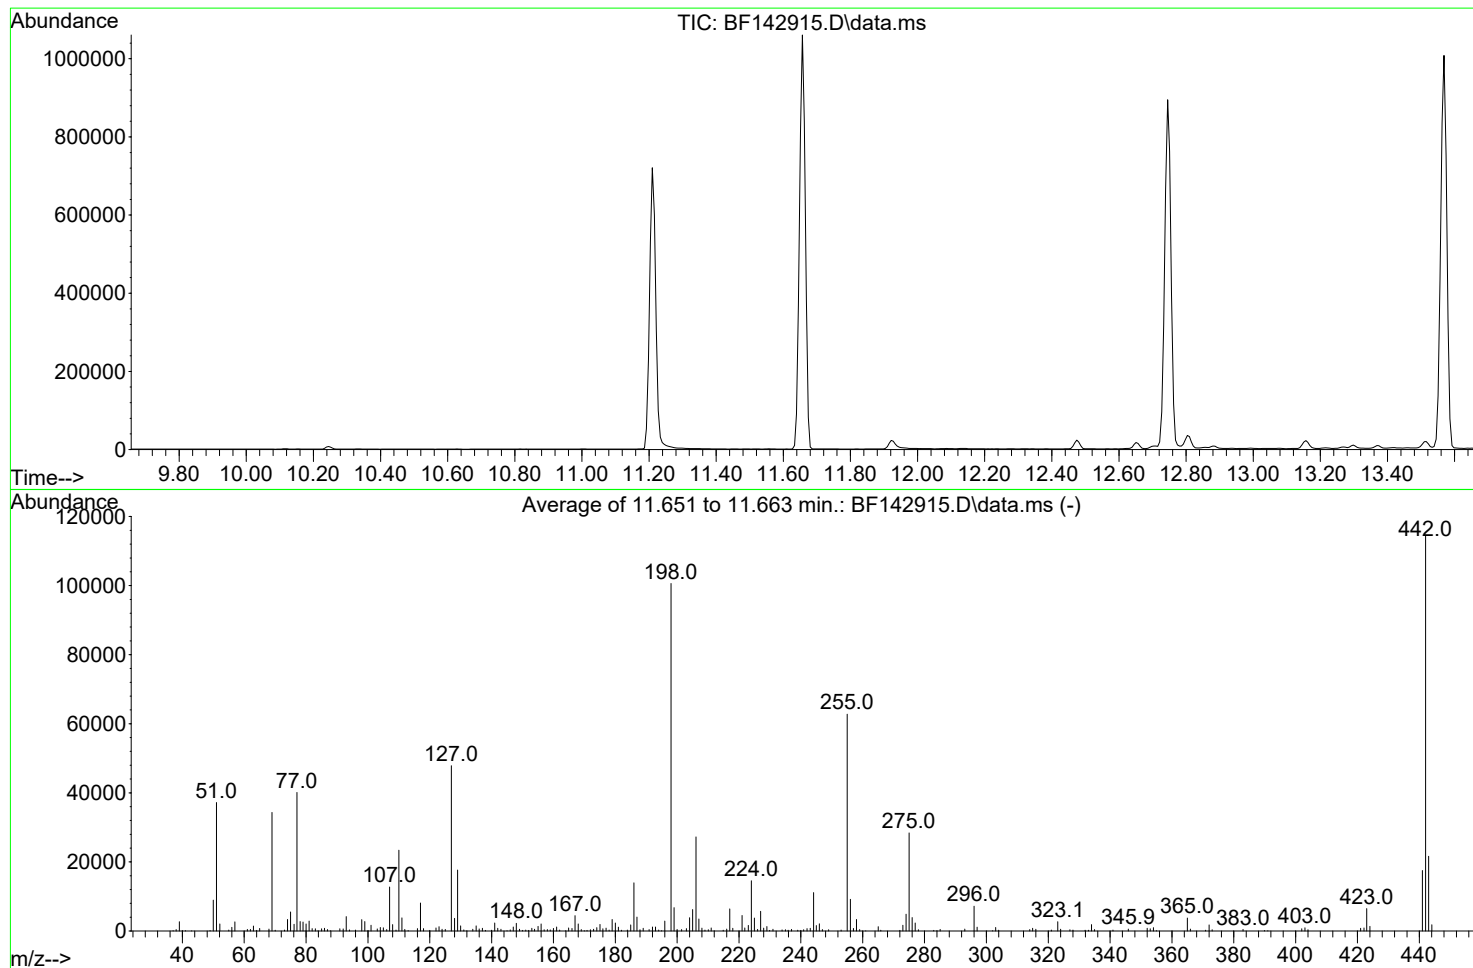

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	577	PASS
69	69	100	100	100.0	34325	PASS
70	69	0.00	2	0.7	230	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100621	PASS
199	198	5	9	6.7	6787	PASS
365	198	1	100	3.8	3778	PASS
441	443	0.01	150	81.0	17513	PASS
442	442	100	100	100.0	114307	PASS
443	442	15	24	18.9	21622	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/30/2025	BNA_F	<u>BF142906.D</u>
Compound Name	Response	Retention Time
DDT	261830	13.568
DDD	4976	13.298
DDE	417	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5393	267223	2.02

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142915.D
Acq On : 30 Jun 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 15:46:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

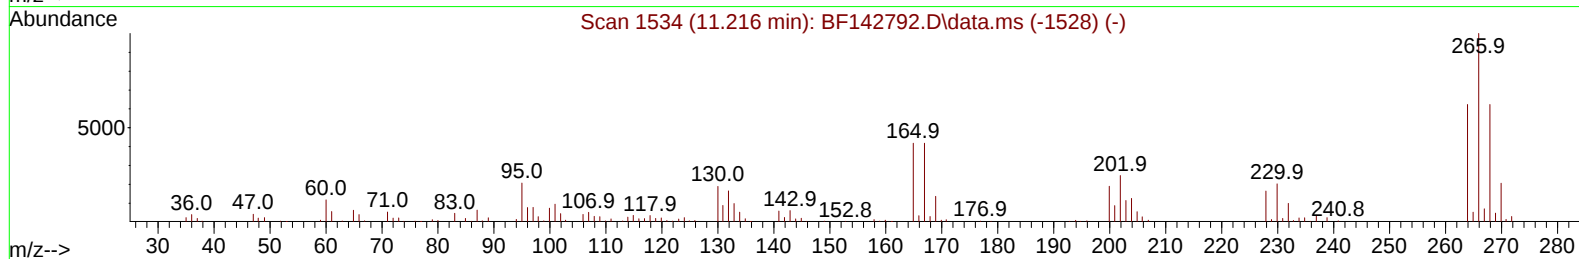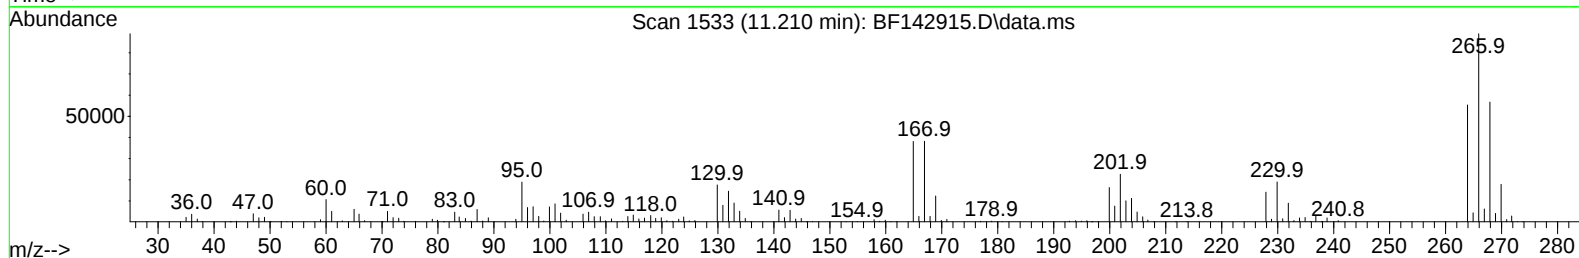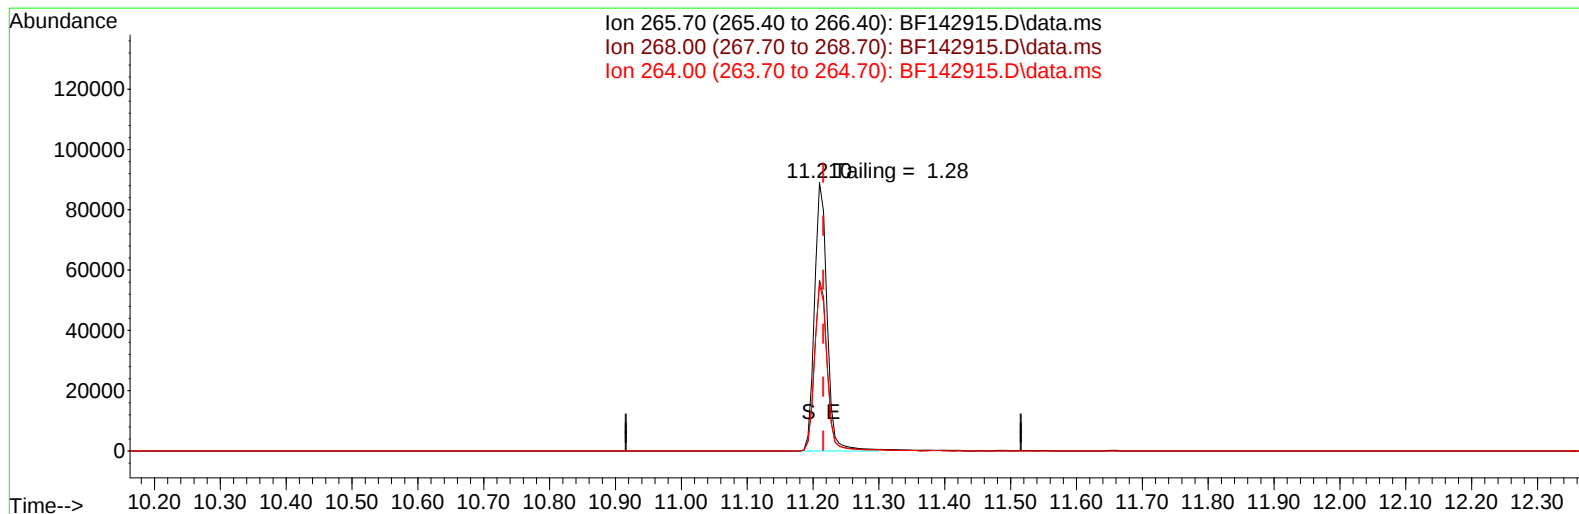

TIC: BF142915.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 37500.34 ng




response 119337

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.69
264.00	62.40	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142915.D
Acq On : 30 Jun 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 15:46:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

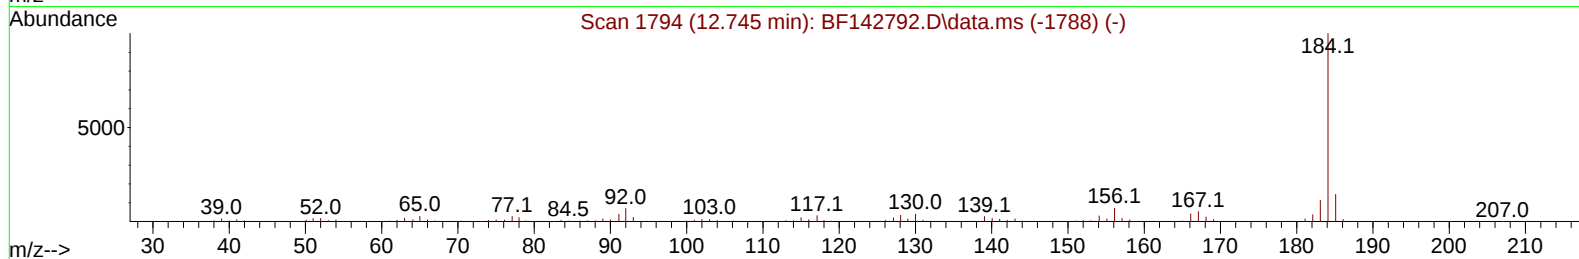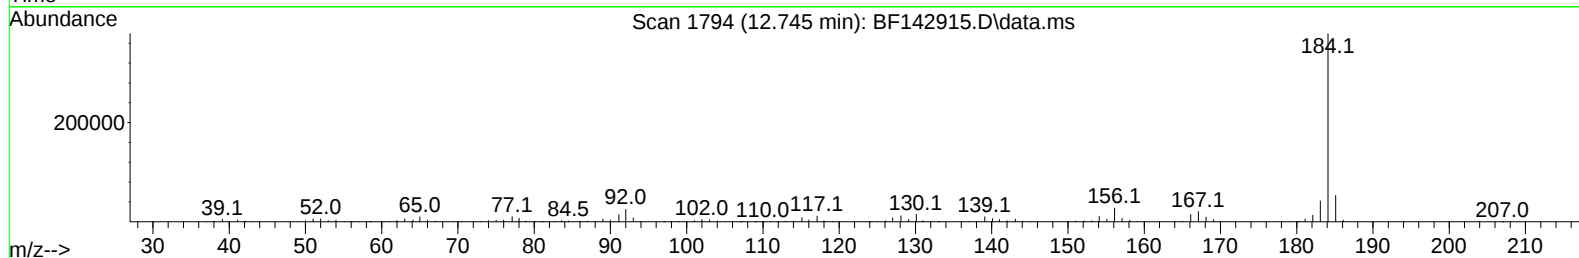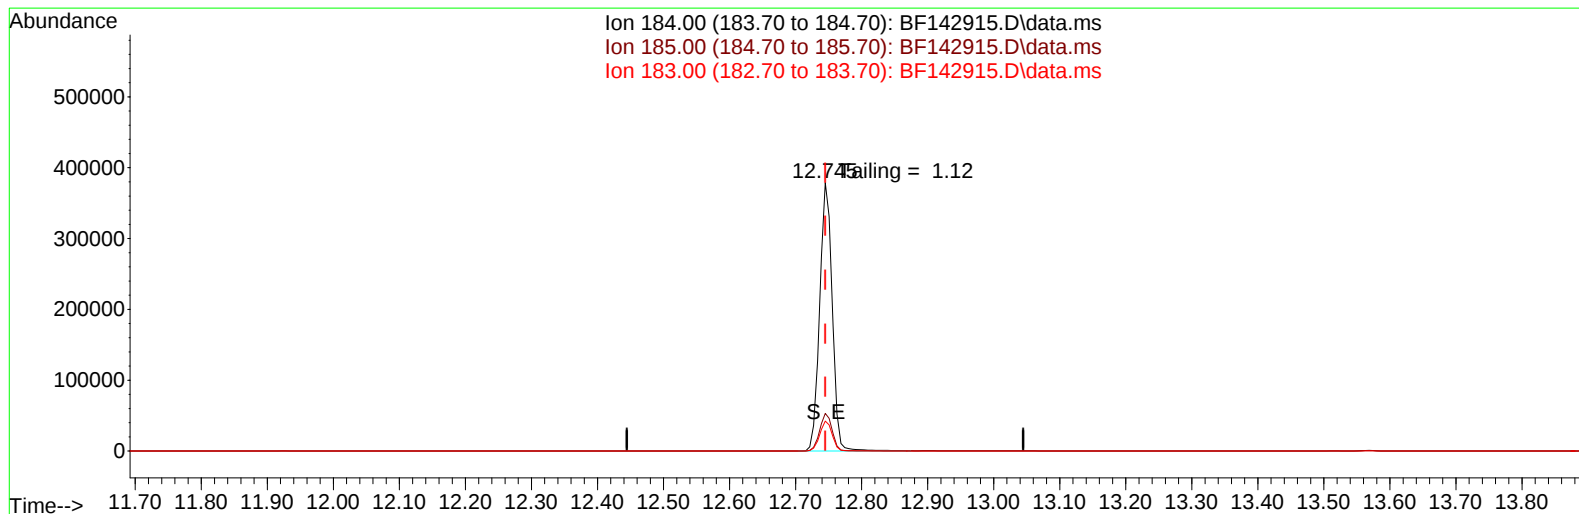

TIC: BF142915.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 501451

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.02
183.00	11.20	11.14
0.00	0.00	0.00