
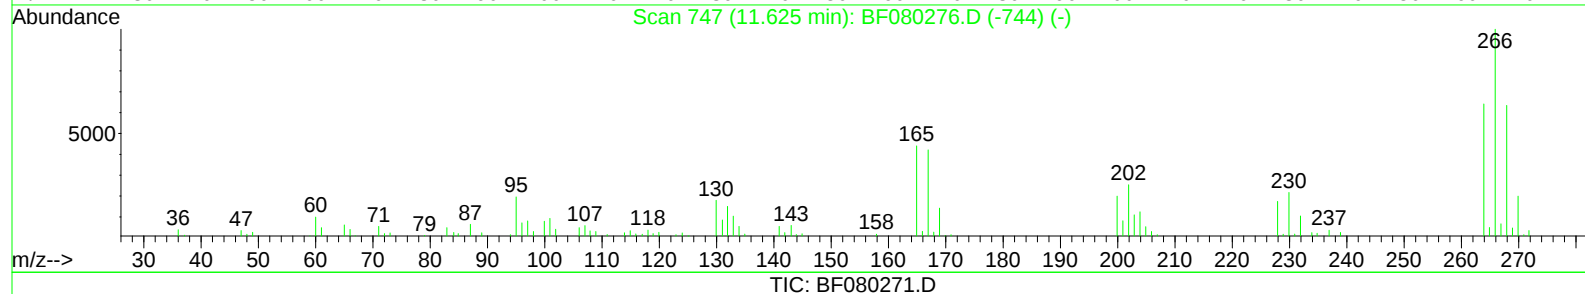
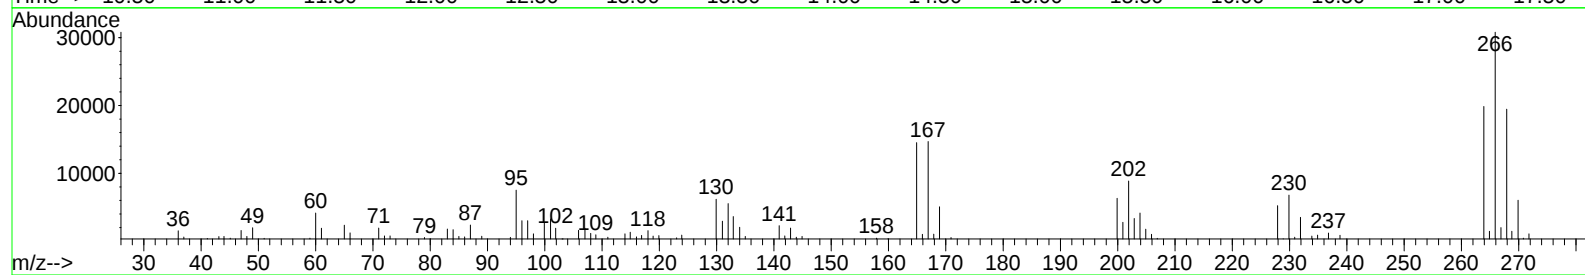


Data Path : Z:\HPCHEM1\BNA F\Data\BF070115\
Data File : BF080271.D
Acq On : 1 Jul 2015 14:00
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 15:54:28 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 19 06:05:07 2015
Response via : Initial Calibration

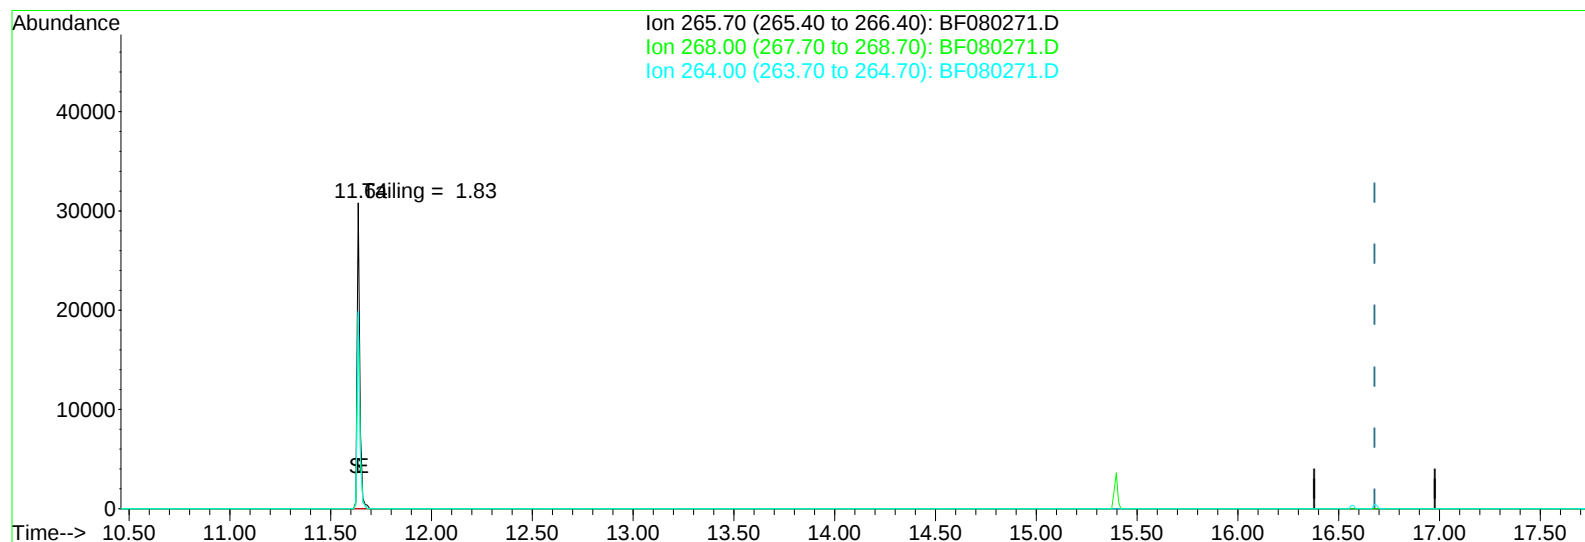

(69) Pentachlorophenol (C)




11.636min (-5.041) 0.00ng m

response 26840

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	63.13
264.00	63.40	64.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF070115\
Data File : BF080271.D
Acq On : 1 Jul 2015 14:00
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 15:54:28 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 19 06:05:07 2015
Response via : Initial Calibration

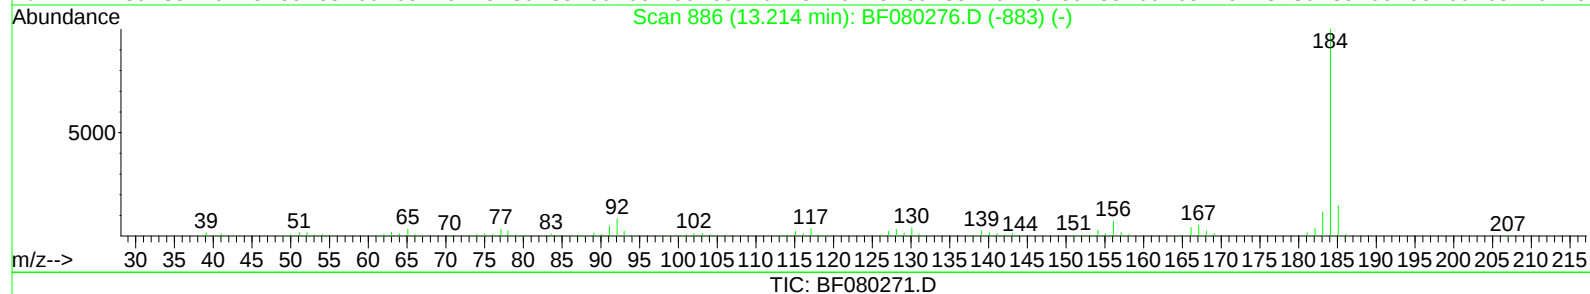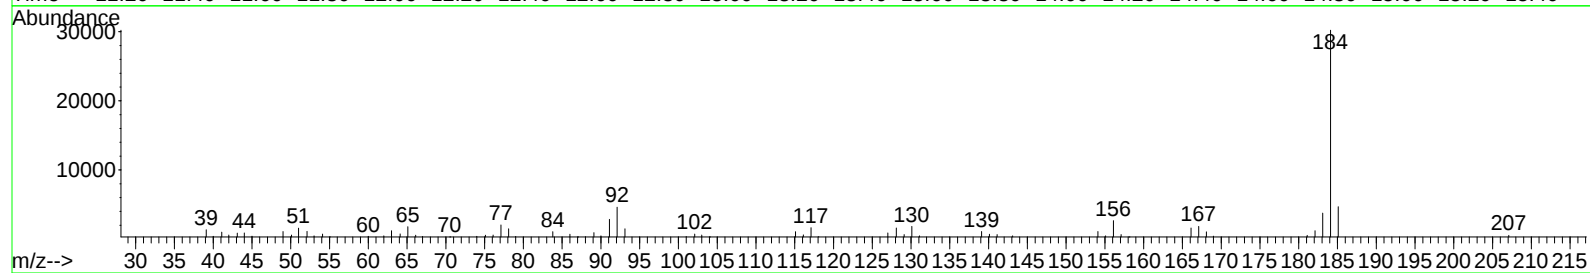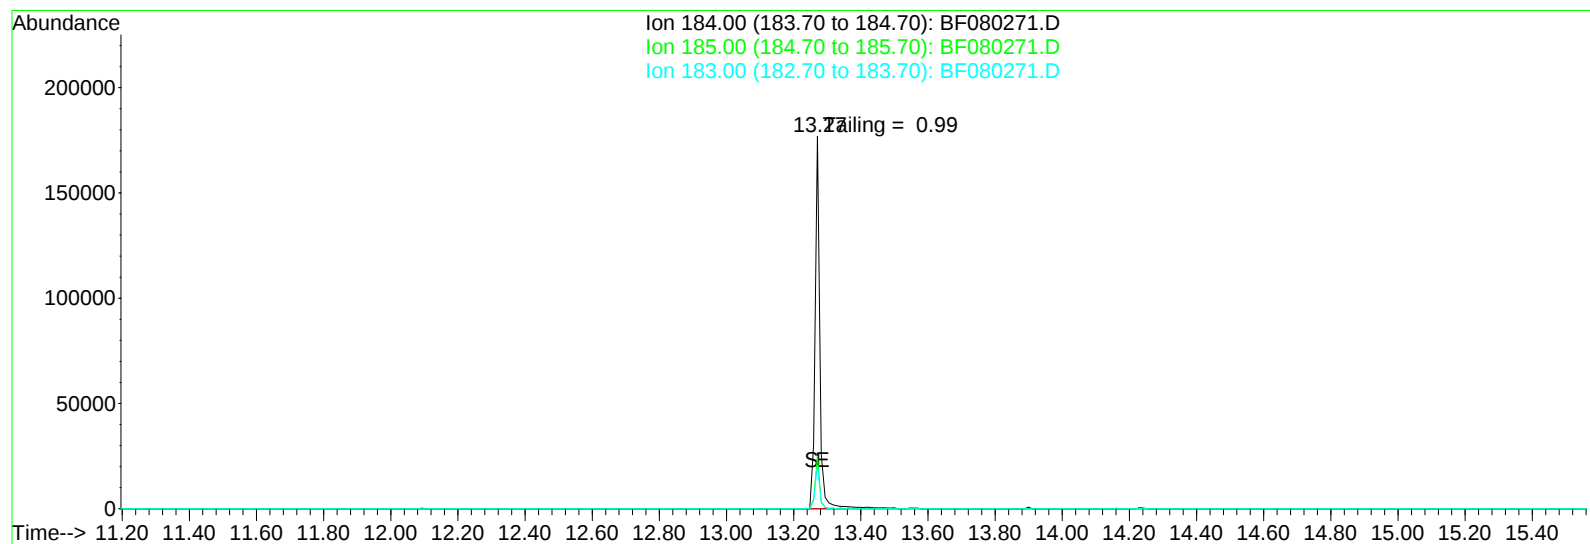

(76) Benzidine

19.292min (-19.292) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.40	0.00#
183.00	12.50	0.00#
0.00	0.00	0.00