
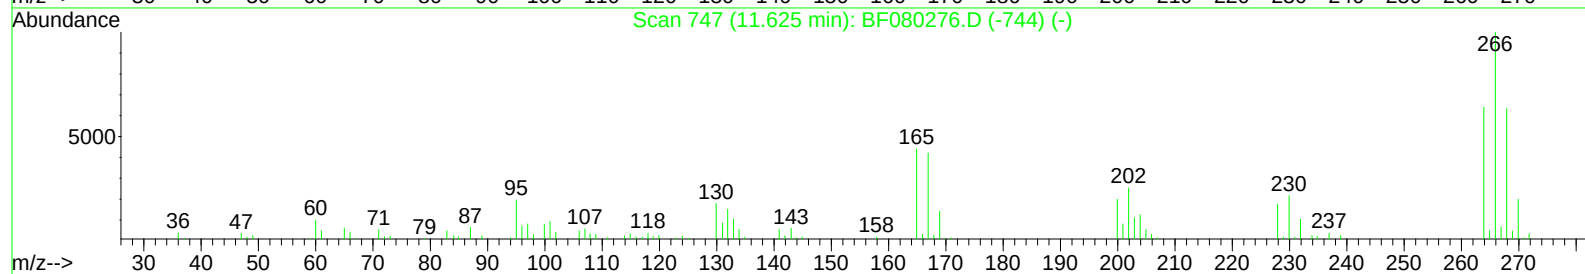
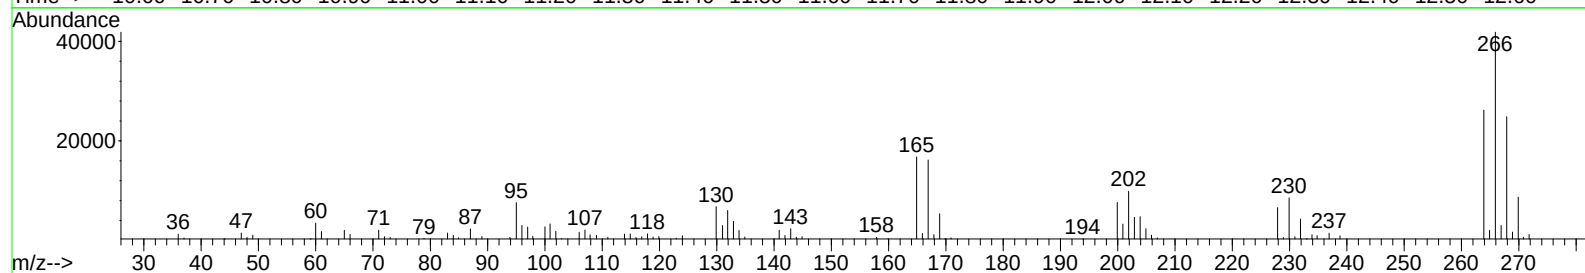


Data Path : Z:\HPCHEM1\BNA F\Data\BF070115\
Data File : BF080287.D
Acq On : 2 Jul 2015 00:03
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 07:56:42 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 03:50:52 2015
Response via : Initial Calibration

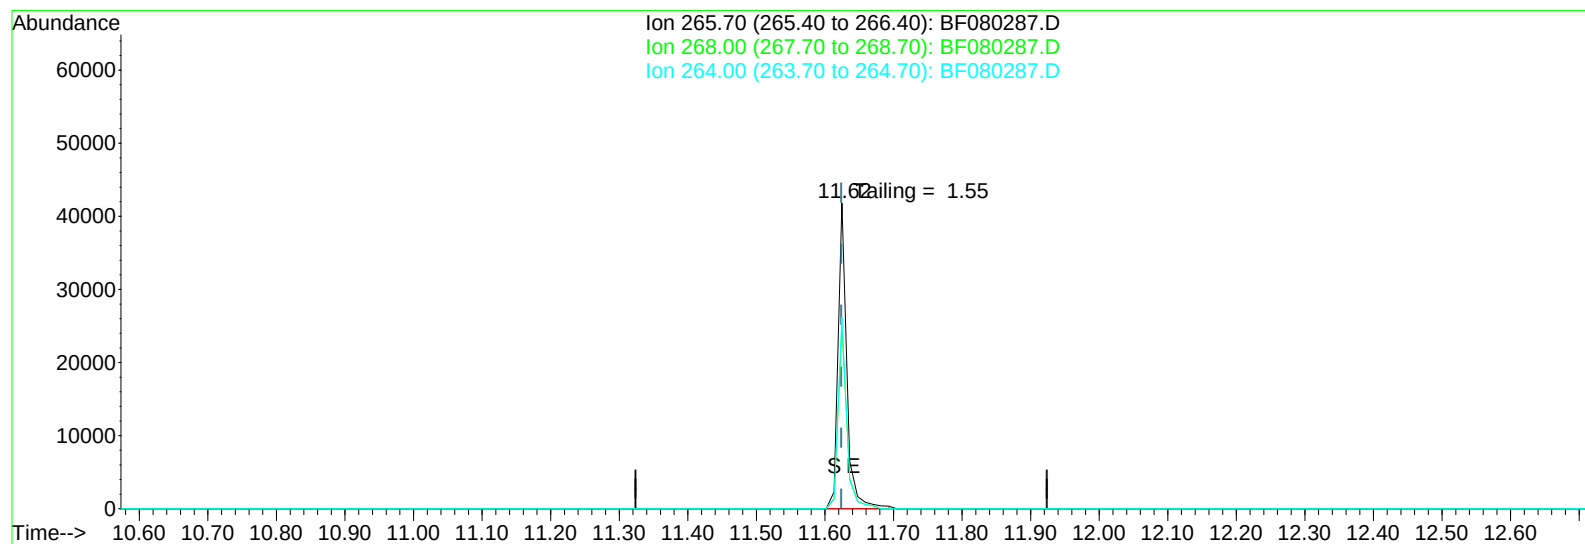

TIC: BF080287.D

(69) Pentachlorophenol (C)




11.625min (+0.001) 0.00ng

response 37343

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	59.47
264.00	64.10	62.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF070115\
Data File : BF080287.D
Acq On : 2 Jul 2015 00:03
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 07:56:42 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 03:50:52 2015
Response via : Initial Calibration

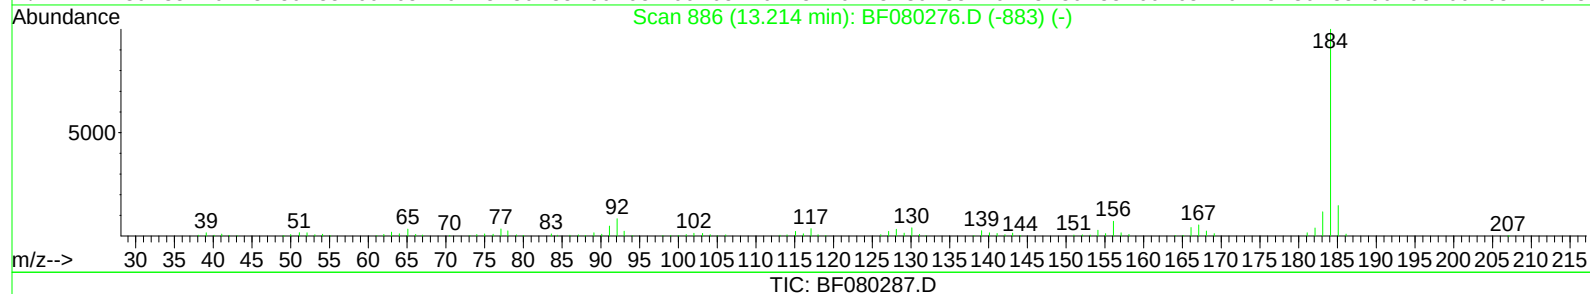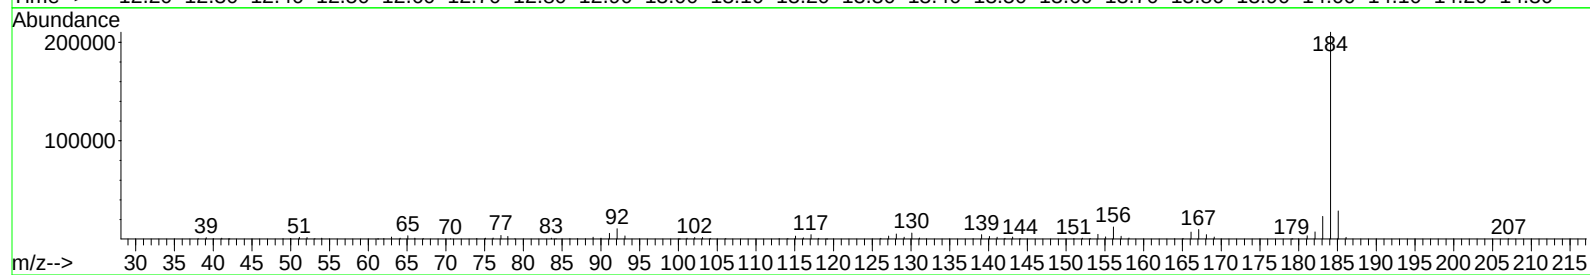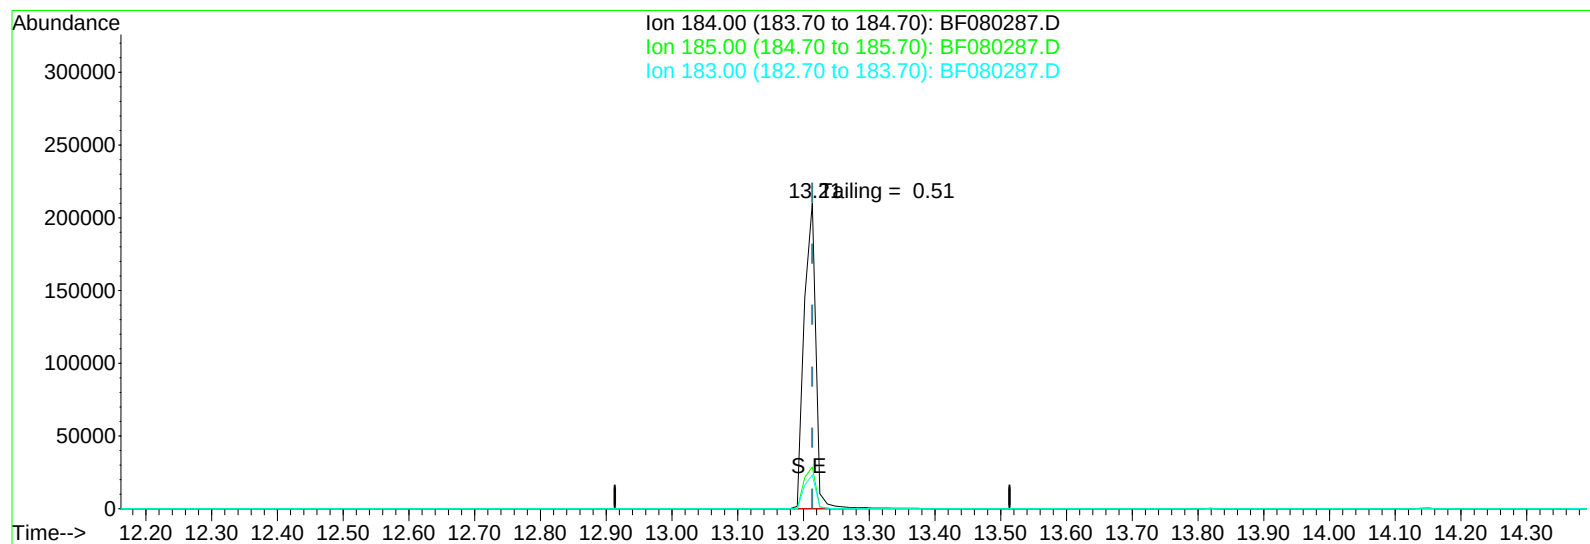

(76) Benzidine

13.213min (-0.000) 31143.91ng

response 259925

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.68
183.00	11.70	11.06
0.00	0.00	0.00