


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070115\
Data File : BF080271.D
Acq On : 1 Jul 2015 14:00
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 23 00:53:56 2015

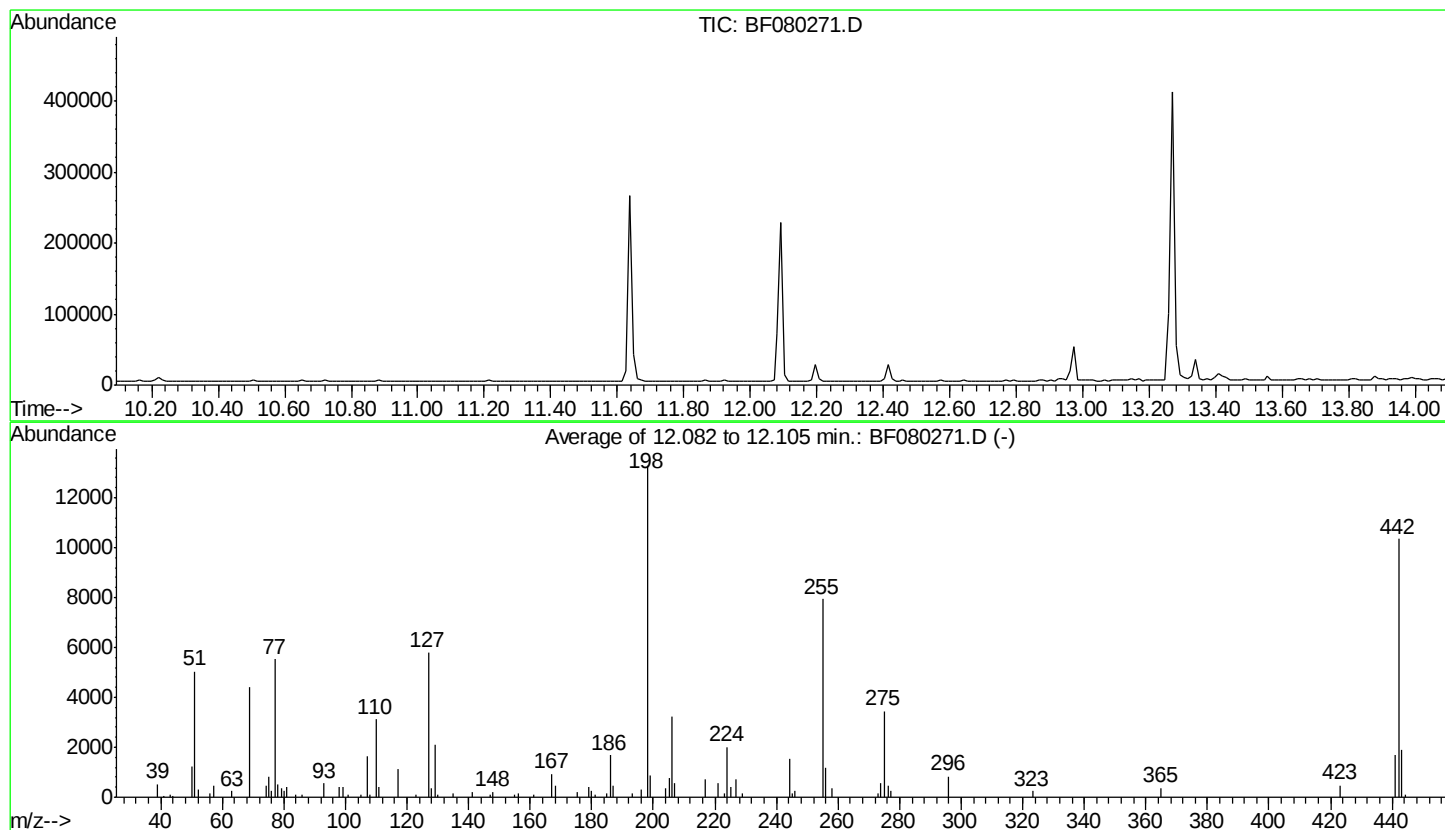

AutoFind: Scans 787, 788, 789; Background Corrected with Scan 784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	5027	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.3	4427	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	5779	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13279	PASS
199	198	5	9	6.5	867	PASS
275	198	10	60	26.0	3447	PASS
365	198	1	100	2.8	368	PASS
441	442	0.01	24	16.3	1691	PASS
442	198	50	100	77.9	10347	PASS
443	442	15	24	18.5	1913	PASS