


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070115\
 Data File : BF080287.D
 Acq On : 2 Jul 2015 00:03
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 23 00:53:56 2015

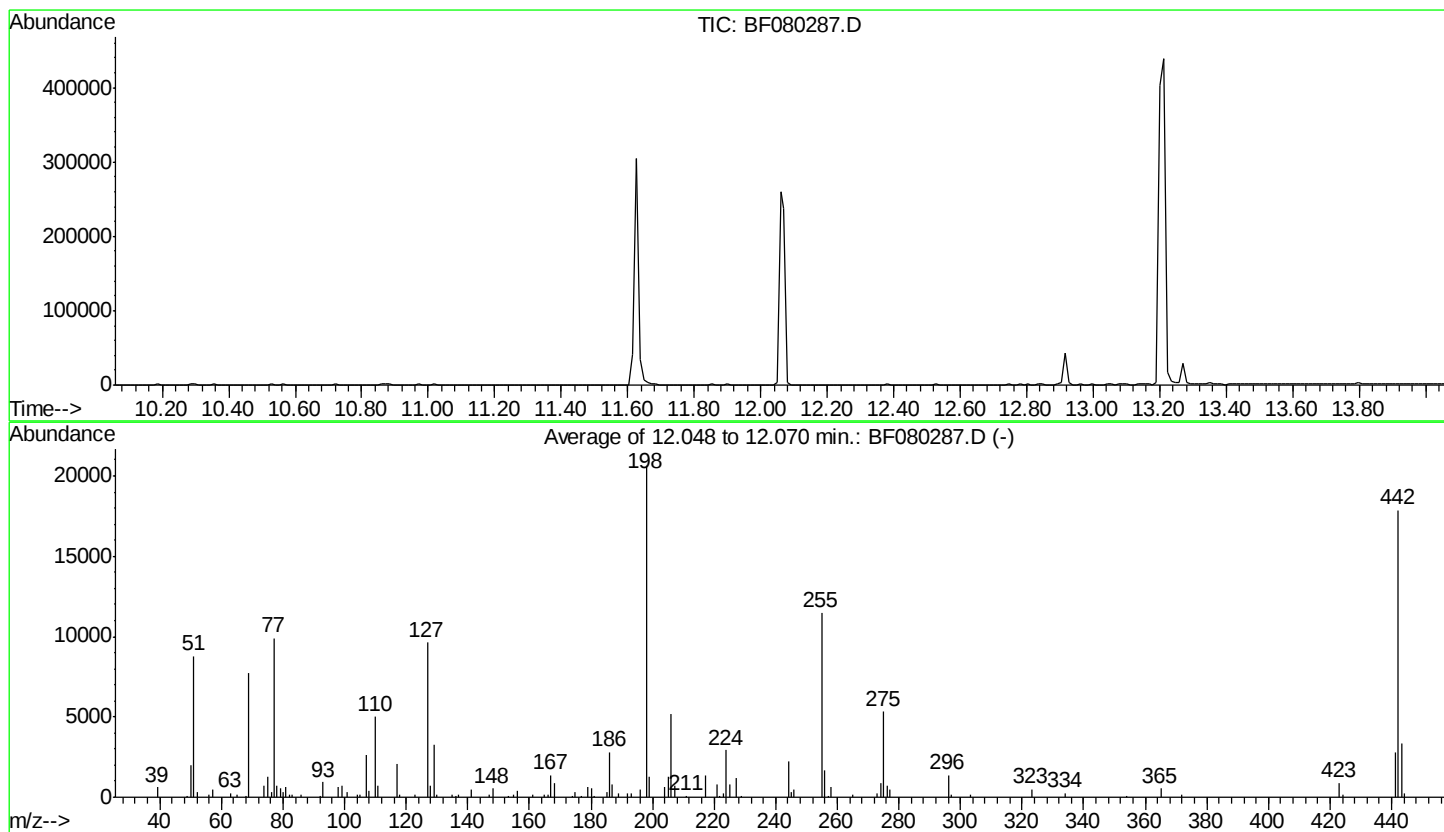

AutoFind: Scans 784, 785, 786; Background Corrected with Scan 782

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	8801	PASS
68	69	0.00	2	1.5	118	PASS
69	198	0.00	100	37.3	7708	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	9608	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20640	PASS
199	198	5	9	6.1	1253	PASS
275	198	10	60	25.8	5330	PASS
365	198	1	100	2.5	524	PASS
441	442	0.01	24	15.4	2758	PASS
442	198	50	100	86.5	17860	PASS
443	442	15	24	18.8	3362	PASS