
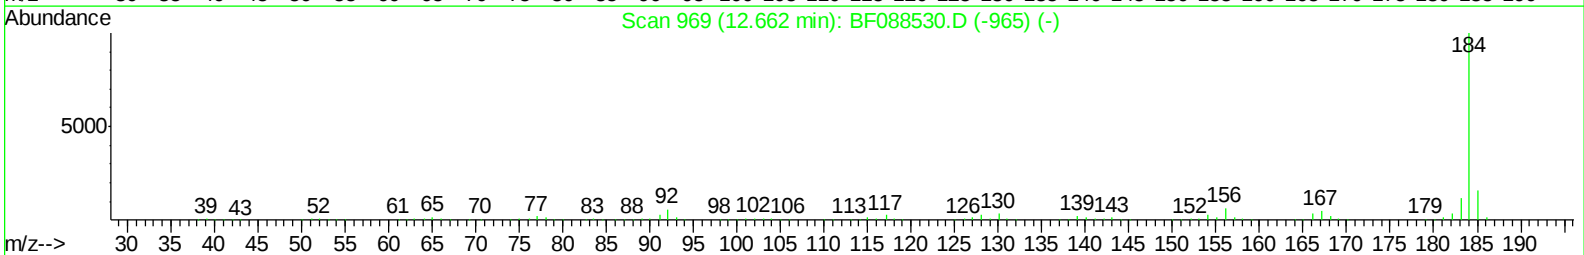
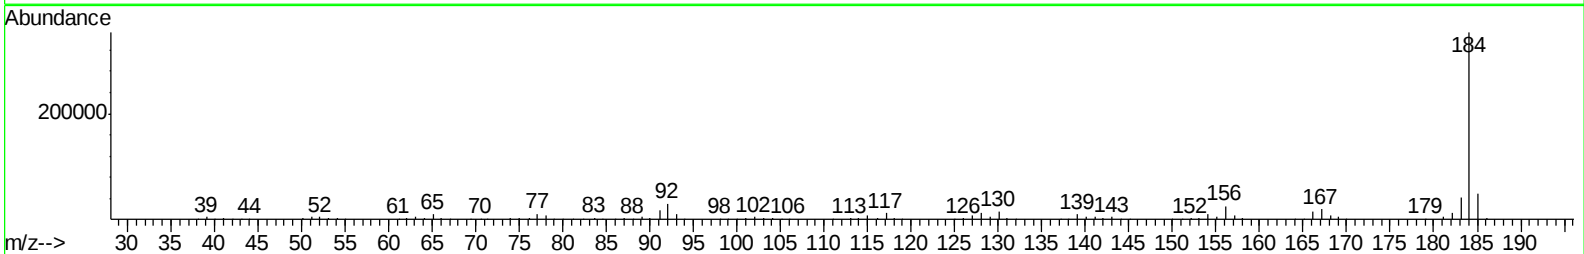


```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070116\  
Data File : BF088587.D  
Acq On    : 1 Jul 2016 21:41  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Jul 02 06:42:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 02:24:16 2016
Response via : Initial Calibration

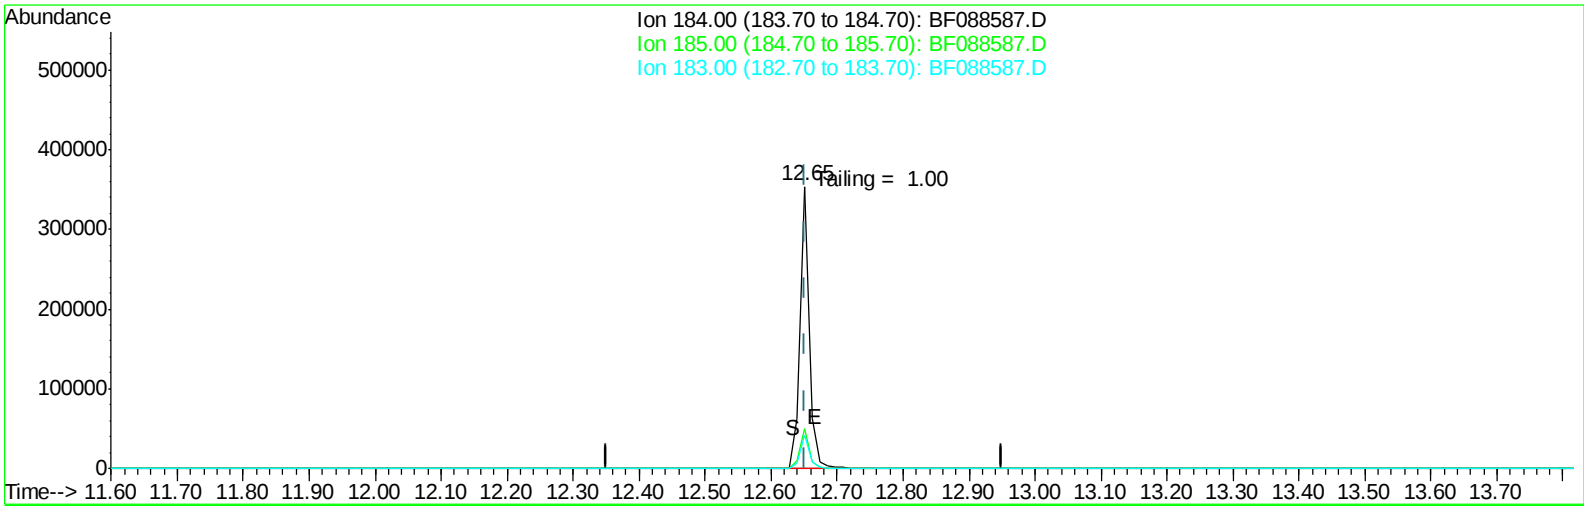

TIC: BF088587.D

(76) Benzidine




12.651min (+0.000) 0.00ng m

response 340276

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.10
183.00	11.60	11.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070116\
Data File : BF088587.D
Acq On : 1 Jul 2016 21:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 06:42:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 02:24:16 2016
Response via : Initial Calibration

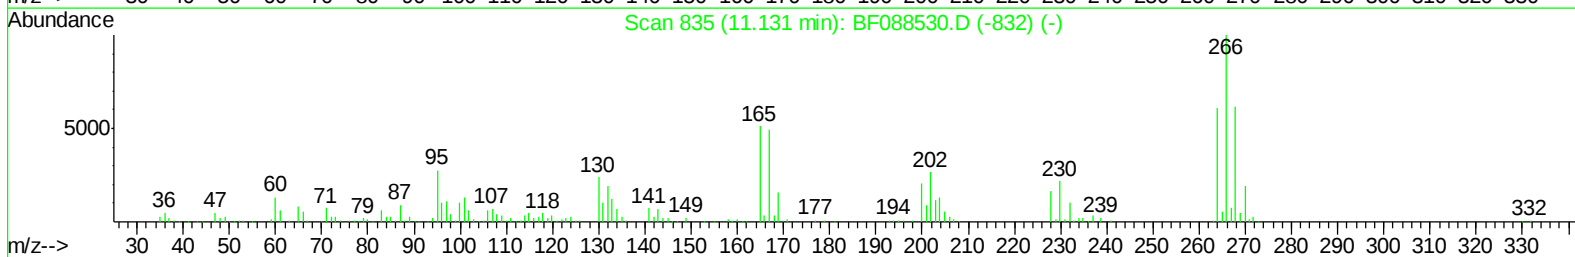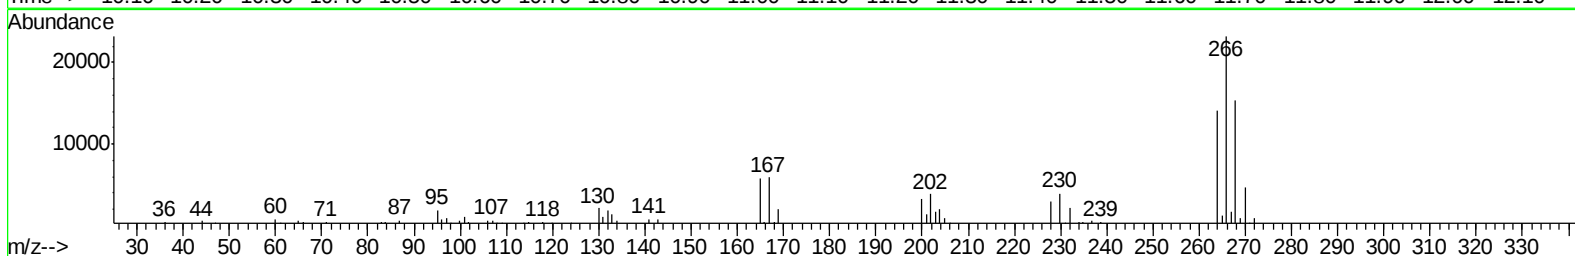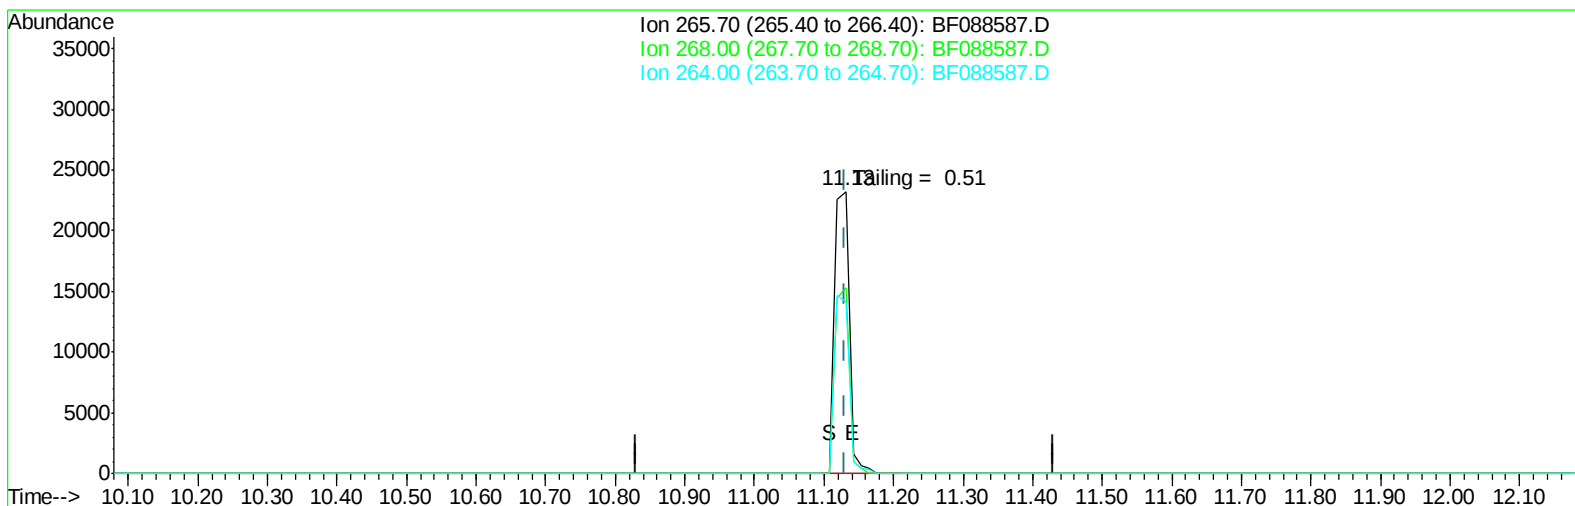

TIC: BF088587.D

(69) Pentachlorophenol (C)

11.131min (+0.000) 0.00ng

response 33239

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	66.02
264.00	62.00	61.01
0.00	0.00	0.00