

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070116\
 Data File : BF088565.D
 Acq On : 1 Jul 2016 10:13
 Operator : UM/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Manual Integrations
 APPROVED

sohil
 7/5/2016 7:30:44 PM

Quant Time: Jul 01 13:58:57 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 30 18:01:55 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	122720	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	484334	20.00	ng	-0.01
38) Acenaphthene-d10	9.85	164	232092	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	451670	20.00	ng	0.00
75) Chrysene-d12	13.95	240	339500	20.00	ng	0.00
86) Perylene-d12	15.35	264	307554	20.00	ng	0.00

System Monitoring Compounds

5) 2-Fluorophenol	5.39	112	576553	70.41	ng	-0.01
7) Phenol-d6	6.44	99	821579	77.65	ng	0.00
23) Nitrobenzene-d5	7.37	82	727635	78.73	ng	-0.01
41) 2,4,6-Tribromophenol	10.63	330	167702	77.81	ng	-0.01
44) 2-Fluorobiphenyl	9.18	172	1226845	83.50	ng	0.00
78) Terphenyl-d14	12.90	244	1019117	66.86	ng	-0.01

Target Compounds

						Qvalue
2) 1,4-Dioxane	2.38	88	150156	36.99	ng	# 32
3) Pyridine	3.07	79	439540	37.31	ng	94
4) n-Nitrosodimethylamine	3.03	42	164669	36.59	ng	89
6) Aniline	6.47	93	553846	35.92	ng	97
8) 2-Chlorophenol	6.59	128	351945	39.99	ng	93
9) Benzaldehyde	6.35	77	268030	37.40	ng	90
10) Phenol	6.46	94	486258	40.27	ng	78
11) bis(2-Chloroethyl)ether	6.55	93	365112	40.55	ng	89
12) 1,3-Dichlorobenzene	6.75	146	368664m	38.07	ng	
13) 1,4-Dichlorobenzene	6.82	146	347249	36.12	ng	94
14) 1,2-Dichlorobenzene	6.98	146	358796m	39.88	ng	
15) Benzyl Alcohol	6.95	79	277561	35.64	ng	94
16) 2,2'-oxybis(1-Chloropropan	7.10	45	468698	35.94	ng	92
17) 2-Methylphenol	7.06	107	274088	38.18	ng	98
18) Hexachloroethane	7.32	117	142869	38.42	ng	89
19) n-Nitroso-di-n-propylamine	7.23	70	272579	38.35	ng	88
20) 3+4-Methylphenols	7.22	107	325012	37.72	ng	# 74
22) Acetophenone	7.22	105	442792	37.67	ng	# 85
24) Nitrobenzene	7.39	77	400428	42.97	ng	# 85
25) Isophorone	7.63	82	655456	38.29	ng	95
26) 2-Nitrophenol	7.71	139	181085	47.39	ng	# 83
27) 2,4-Dimethylphenol	7.75	122	301330	37.86	ng	90
28) bis(2-Chloroethoxy)methane	7.85	93	455829	40.91	ng	# 96
29) 2,4-Dichlorophenol	7.95	162	283988	44.15	ng	97
30) 1,2,4-Trichlorobenzene	8.03	180	279161	39.55	ng	98
31) Naphthalene	8.11	128	914392	38.30	ng	100
32) Benzoic acid	7.86	122	158089	27.36	ng	92
33) 4-Chloroaniline	8.16	127	430200	40.49	ng	94
34) Hexachlorobutadiene	8.24	225	153599	40.64	ng	99
35) Caprolactam	8.54	113	88431	40.48	ng	99
36) 4-Chloro-3-methylphenol	8.65	107	326836	42.97	ng	97
37) 2-Methylnaphthalene	8.81	142	643461	41.85	ng	# 97
39) 1,2,4,5-Tetrachlorobenzene	8.97	216	286053	37.06	ng	# 1
40) Hexachlorocyclopentadiene	8.96	237	131120	34.61	ng	98

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070116\
 Data File : BF088565.D
 Acq On : 1 Jul 2016 10:13
 Operator : UM/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Manual Integrations
 APPROVED

sohil
 7/5/2016 7:30:44 PM

Quant Time: Jul 01 13:58:57 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 30 18:01:55 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) 2,4,6-Trichlorophenol	9.08	196	195360m	38.38	ng	
43) 2,4,5-Trichlorophenol	9.12	196	186172m	42.51	ng	
45) 1,1'-Biphenyl	9.27	154	718043	37.36	ng	98
46) 2-Chloronaphthalene	9.29	162	559754	37.10	ng	97
47) 2-Nitroaniline	9.38	65	206659	38.60	ng	91
48) Acenaphthylene	9.71	152	962571	40.10	ng	99
49) Dimethylphthalate	9.58	163	687313	41.57	ng	100
50) 2,6-Dinitrotoluene	9.63	165	165428	45.14	ng	# 79
51) Acenaphthene	9.88	154	592690	40.28	ng	99
52) 3-Nitroaniline	9.79	138	177034	38.00	ng	89
53) 2,4-Dinitrophenol	9.90	184	49611	30.66	ng	# 86
54) Dibenzofuran	10.06	168	760510	39.49	ng	100
55) 4-Nitrophenol	9.95	139	155138	43.82	ng	97
56) 2,4-Dinitrotoluene	10.03	165	221845	46.30	ng	# 80
57) Fluorene	10.39	166	540137	36.39	ng	98
58) 2,3,4,6-Tetrachlorophenol	10.17	232	144863	42.76	ng	# 55
59) Diethylphthalate	10.27	149	654911	39.47	ng	99
60) 4-Chlorophenyl-phenylether	10.39	204	266480	38.64	ng	100
61) 4-Nitroaniline	10.41	138	201904	45.04	ng	92
62) Azobenzene	10.55	77	781244	41.27	ng	97
64) 4,6-Dinitro-2-methylphenol	10.43	198	78352	32.43	ng	88
65) n-Nitrosodiphenylamine	10.50	169	524502	34.31	ng	100
66) 4-Bromophenyl-phenylether	10.88	248	176782	38.84	ng	93
67) Hexachlorobenzene	10.94	284	178715	35.47	ng	99
68) Atrazine	11.03	200	181309	38.06	ng	90
69) Pentachlorophenol	11.13	266	117892	39.54	ng	98
70) Phenanthrene	11.35	178	869794	35.23	ng	99
71) Anthracene	11.40	178	945195	38.50	ng	98
72) Carbazole	11.55	167	903631	39.11	ng	100
73) Di-n-butylphthalate	11.90	149	1062697	39.54	ng	99
74) Fluoranthene	12.53	202	924001	36.92	ng	96
76) Benzidine	12.65	184	533591	31.09	ng	99
77) Pyrene	12.75	202	933269	32.42	ng	100
79) Butylbenzylphthalate	13.38	149	433485	33.76	ng	# 79
80) Benzo(a)anthracene	13.94	228	783081	35.82	ng	100
81) 3,3'-Dichlorobenzidine	13.91	252	322303	39.21	ng	# 97
82) Chrysene	13.98	228	719366	33.26	ng	99
83) Bis(2-ethylhexyl)phthalate	13.94	149	511775	34.91	ng	# 98
84) Di-n-octyl phthalate	14.56	149	1031605	41.42	ng	# 100
85) Indeno(1,2,3-cd)pyrene	16.70	276	567185	34.09	ng	# 100
87) Benzo(b)fluoranthene	14.96	252	830032m	43.02	ng	
88) Benzo(k)fluoranthene	14.98	252	540973m	32.21	ng	
89) Benzo(a)pyrene	15.29	252	628400	38.47	ng	99
90) Dibenzo(a,h)anthracene	16.72	278	488375	35.80	ng	98
91) Benzo(g,h,i)perylene	17.11	276	490275	34.73	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070116\
 Data File : BF088565.D
 Acq On : 1 Jul 2016 10:13
 Operator : UM/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Manual Integrations
 APPROVED

sohil
 7/5/2016 7:30:44 PM

Quant Time: Jul 01 13:58:57 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 30 18:01:55 2016
 Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.81 min Scan# 457

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040

Tgt Ion: 152 Resp: 122720
Ion Ratio Lower Upper

152 100


150 157.1 123.8 185.6

115 60.7 39.6 59.4#




Manual Integrations
APPROVED

sohil

7/5/2016 7:30:44 PM



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E



#2

1,4-Dioxane

Concen: 36.99 ng

RT: 2.38 min Scan# 69

Delta R.T. -0.01 min

Lab File: BF088565.D


Acq: 1 Jul 2016 10:13

Tgt Ion: 88 Resp: 150156
Ion Ratio Lower Upper



88 100


58 70.6 0.0 0.0#

43 26.6 3.4 5.2#



Abundance Ion 88.00 (87.70 to 88.70): BF0
Ion 58.00 (57.70 to 58.70): BF0
Ion 43.00 (42.70 to 43.70): BF0









#3
 Pyridine
 Concen: 37.31 ng
 RT: 3.07 min Scan# 130
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTCCCC040

Tgt Ion	Ratio	Lower	Upper
79	100		
52	65.0	56.3	84.5
51	31.6	27.4	41.2




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM



#4
 n-Nitrosodimethylamine
 Concen: 36.59 ng
 RT: 3.03 min Scan# 126
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
42	100		
74	150.1	108.6	163.0
44	7.2	5.5	8.3





#5

2-Fluorophenol

Concen: 70.41 ng

RT: 5.39 min Scan# 333

Delta R.T. -0.01 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion:	112	Resp:	576553
Ion Ratio	Lower	Upper	
112	100		
64	63.7	42.2	63.2#
63	32.6	21.8	32.8

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



#6

Aniline

Concen: 35.92 ng




RT: 6.47 min Scan# 427


Delta R.T. -0.01 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion:	93	Resp:	553846
Ion Ratio	Lower	Upper	
93	100		
66	39.4	29.8	44.8
65	19.8	14.9	22.3





#7

Phenol-d6

Concen: 77.65 ng

RT: 6.44 min Scan# 425

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion:	99	Resp:	821579
Ion Ratio	Lower	Upper	
99	100		
42	14.9	12.2	18.2
71	31.5	23.4	35.0

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



#8

2-Chlorophenol

Concen: 39.99 ng




RT: 6.59 min Scan# 438


Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion:	128	Resp:	351945
Ion Ratio	Lower	Upper	
128	100		
130	32.9	12.0	52.0
64	43.1	30.8	70.8





#9

Benzaldehyde

Concen: 37.40 ng

RT: 6.35 min Scan# 417

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
77	100		
105	100.9	90.6	130.6
106	94.3	85.3	125.3

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



#10

Phenol

Concen: 40.27 ng




RT: 6.46 min Scan# 426


Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
94	100		
65	33.4	5.9	45.9
66	49.8	14.0	54.0









#11
bis(2-Chloroethyl)ether
Concen: 40.55 ng
RT: 6.55 min Scan# 434
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
93	100		
63	73.8	67.6	107.6
95	31.8	12.5	52.5




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#12
1,3-Dichlorobenzene
Concen: 38.07 ng m
RT: 6.75 min Scan# 452
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
146	100		
148	64.6	50.9	76.3
75	24.9	25.6	38.4#









#13
 1,4-Dichlorobenzene
 Concen: 36.12 ng
 RT: 6.82 min Scan# 458
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
146	100		
148	62.7	52.0	78.0
111	48.7	33.8	50.8




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM



#14
 1,2-Dichlorobenzene
 Concen: 39.88 ng m
 RT: 6.98 min Scan# 472
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
146	100		
148	63.8	52.3	78.5
111	44.6	28.7	43.1#





#15

Benzyl Alcohol

Concen: 35.64 ng

RT: 6.95 min Scan# 469

Delta R.T. -0.01 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion:	79	Resp:	277561
Ion Ratio	Lower	Upper	
79	100		
108	72.4	65.0	97.6
77	63.0	50.3	75.5

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



#16

2,2'-oxybis(1-Chloropropane)

Concen: 35.94 ng




RT: 7.10 min Scan# 482


Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13


Tgt Ion:	45	Resp:	468698
Ion Ratio	Lower	Upper	
45	100		
77	15.7	0.0	32.5
79	12.1	0.0	29.5





#17
2-Methylphenol
Concen: 38.18 ng
RT: 7.06 min Scan# 479
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040



Tgt Ion	Ratio	Resp	Lower	Upper
107	100	274088		
108	113.0	90.9	136.3	
77	49.0	36.6	55.0	
79	48.6	36.5	54.7	




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#18
Hexachloroethane
Concen: 38.42 ng
RT: 7.32 min Scan# 502
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
117	100	142869		
119	93.5	77.4	116.2	
201	81.8	80.4	120.6	









#19
n-Nitroso-di-n-propylamine
Concen: 38.35 ng
RT: 7.23 min Scan# 494
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
70	100		
42	50.2	49.6	74.4
101	9.4	7.1	10.7
130	21.0	15.4	23.2




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#20
3+4-Methylphenols
Concen: 37.72 ng
RT: 7.22 min Scan# 493
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
107	100		
108	90.7	67.8	107.8
77	129.3	59.3	99.3#
79	32.4	7.0	47.0









#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.09 min Scan# 569
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
136	100	484334		
137	11.3	9.1	13.7	
54	9.8	6.6	10.0	
68	8.2	5.1	7.7#	




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#22
Acetophenone
Concen: 37.67 ng
RT: 7.22 min Scan# 493
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
105	100	442792		
71	4.5	5.3	7.9#	
51	35.8	18.2	27.4#	
120	19.9	18.0	27.0	









#23
 Nitrobenzene-d5
 Concen: 78.73 ng
 RT: 7.37 min Scan# 506
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
82	100		
128	40.8	35.9	53.9
54	50.0	40.9	61.3




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM



#24
 Nitrobenzene
 Concen: 42.97 ng
 RT: 7.39 min Scan# 508
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
77	100		
123	42.9	45.0	67.4#
65	13.2	10.2	15.2





#25

Isophorone

Concen: 38.29 ng

RT: 7.63 min Scan# 529

Delta R.T. -0.01 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
82	100	655456		
95	6.7	5.4	8.2	
138	15.0	14.6	21.8	

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



#26

2-Nitrophenol

Concen: 47.39 ng




RT: 7.71 min Scan# 536


Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
139	100	181085		
109	27.1	23.0	34.4	
65	39.7	45.8	68.8	









#27
2,4-Dimethylphenol
Concen: 37.86 ng
RT: 7.75 min Scan# 539
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
122	100	301330		
107	118.2	82.4	123.6	
121	58.8	46.3	69.5	




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#28
bis(2-Chloroethoxy)methane
Concen: 40.91 ng
RT: 7.85 min Scan# 548
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
93	100	455829		
95	32.2	26.5	39.7	
123	10.6	11.6	17.4	






#29
 2,4-Dichlorophenol
 Concen: 44.15 ng
 RT: 7.95 min Scan# 557
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040




Tgt Ion	Ratio	Resp Lower	Resp Upper
162	100		
164	64.0	43.8	83.8
98	36.8	21.3	61.3

Manual Integrations
 APPROVED

sohil
 7/5/2016 7:30:44 PM




Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 98.00 (97.70 to 98.70): BF0






#30
 1,2,4-Trichlorobenzene
 Concen: 39.55 ng
 RT: 8.03 min Scan# 564
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp Lower	Resp Upper
180	100		
182	93.5	76.0	114.0
145	34.9	26.5	39.7



Abundance Ion 180.00 (179.70 to 180.70): E
 Ion 182.00 (181.70 to 182.70): E
 Ion 145.00 (144.70 to 145.70): E






#31
Naphthalene
Concen: 38.30 ng
RT: 8.11 min Scan# 571
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040




Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.7	9.4	14.2
127	13.5	10.9	16.3

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM






Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E




#32
Benzoic acid
Concen: 27.36 ng
RT: 7.86 min Scan# 549
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
122	100		
105	129.2	101.6	141.6
77	99.3	70.6	110.6

Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF0





#33

4-Chloroaniline

Concen: 40.49 ng

RT: 8.16 min Scan# 575

Delta R.T. -0.01 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F


ClientSampleId :

SSTDCCC040




Tgt Ion	Ratio	Resp	Lower	Upper
127	100	430200		
129	31.9	26.3	39.5	
65	36.4	24.7	37.1	
92	22.1	15.4	23.0	

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 65.00 (64.70 to 65.70): BF0
Ion 92.00 (91.70 to 92.70): BF0



#34

Hexachlorobutadiene

Concen: 40.64 ng


RT: 8.24 min Scan# 582

Delta R.T. -0.01 min



Lab File: BF088565.D


Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
225	100	153599		
223	63.3	50.9	76.3	
227	63.4	51.9	77.9	



Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E






#35
 Caprolactam
 Concen: 40.48 ng
 RT: 8.54 min Scan# 608
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTCCCC040

Tgt Ion	Ratio	Lower	Upper
113	100		
55	177.6	158.6	198.6
56	132.1	110.6	150.6

Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM





Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BF0

Ion 56.00 (55.70 to 56.70): BF0




Time-->



#36
 4-Chloro-3-methylphenol
 Concen: 42.97 ng
 RT: 8.65 min Scan# 618
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13


Tgt Ion	Ratio	Lower	Upper
107	100		
144	27.1	20.8	31.2
142	81.9	63.4	95.2




Abundance Ion 107.00 (106.70 to 107.70): E


Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E



Time-->






#37
2-Methylnaphthalene
Concen: 41.85 ng
RT: 8.81 min Scan# 632
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040




Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.6	71.0	106.6
115	33.8	22.6	33.8#

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM




Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E
Ion 115.00 (114.70 to 115.70): E






#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.85 min Scan# 723
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.7	85.4	128.2
160	48.7	39.5	59.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E






#39
1,2,4,5-Tetrachlorobenzene
Concen: 37.06 ng
RT: 8.97 min Scan# 646
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040




Tgt Ion	Ratio	Resp Lower	Resp Upper
216	100		
214	79.0	2.9	4.3#
179	22.6	0.0	0.0#
108	22.2	0.5	0.7#

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM




Abundance Ion 216.00 (215.70 to 216.70): E
Ion 214.00 (213.70 to 214.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 108.00 (107.70 to 108.70): E






#40
Hexachlorocyclopentadiene
Concen: 34.61 ng
RT: 8.96 min Scan# 645
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp Lower	Resp Upper
237	100		
235	65.0	43.4	83.4
272	11.5	0.0	32.3



Abundance Ion 236.80 (236.50 to 237.50): E
Ion 234.90 (234.60 to 235.60): E
Ion 271.75 (271.45 to 272.45): E









#41
 2,4,6-Tribromophenol
 Concen: 77.81 ng
 RT: 10.63 min Scan# 791
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Resp Lower	Resp Upper
330	100		
332	95.6	0.0	0.0#
141	40.1	0.0	0.0#




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM



#42
 2,4,6-Trichlorophenol
 Concen: 38.38 ng m
 RT: 9.08 min Scan# 656
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13


Tgt Ion	Ratio	Resp Lower	Resp Upper
196	100		
198	94.8	78.0	117.0
200	30.1	25.4	38.2





#43
 2,4,5-Trichlorophenol
 Concen: 42.51 ng m
 RT: 9.12 min Scan# 659
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040



Tgt Ion	Ratio	Resp	Lower	Upper
196	100	186172		
198	94.3	77.5	116.3	
97	65.3	32.0	48.0	#
132	32.7	20.9	31.3	#




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM



#44
 2-Fluorobiphenyl
 Concen: 83.50 ng
 RT: 9.18 min Scan# 664
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	1226845		
171	36.2	28.6	43.0	
170	24.0	19.2	28.8	






#45
 1,1'-Biphenyl
 Concen: 37.36 ng
 RT: 9.27 min Scan# 672
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040




Tgt Ion	Ratio	Lower	Upper
154	100		
153	40.6	20.6	60.6
76	18.4	0.0	35.1

Manual Integrations
 APPROVED

sohil
 7/5/2016 7:30:44 PM




Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BF0






#46
 2-Chloronaphthalene
 Concen: 37.10 ng
 RT: 9.29 min Scan# 674
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
162	100		
127	47.4	35.2	52.8
164	32.8	26.6	39.8



Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 127.00 (126.70 to 127.70): E
 Ion 164.00 (163.70 to 164.70): E









#47
2-Nitroaniline
Concen: 38.60 ng
RT: 9.38 min Scan# 682
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
65	100		
92	66.3	54.6	82.0
138	82.4	77.0	115.4




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#48
Acenaphthylene
Concen: 40.10 ng
RT: 9.71 min Scan# 711
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.0	16.2	24.4
153	12.8	11.0	16.6





#49

Dimethylphthalate

Concen: 41.57 ng

RT: 9.58 min Scan# 699

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F


ClientSampleId :

SSTDCCC040

Tgt Ion:	163	Resp:	687313
Ion Ratio	Lower	Upper	
163	100		
194	3.4	2.8	4.2
164	10.2	8.3	12.5

Manual Integrations
APPROVED




sohil
7/5/2016 7:30:44 PM



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



#50

2,6-Dinitrotoluene

Concen: 45.14 ng


RT: 9.63 min Scan# 704

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13



Tgt Ion:	165	Resp:	165428
Ion Ratio	Lower	Upper	
165	100		
63	47.3	28.1	42.1#
89	53.1	32.2	48.2#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0





#51

Acenaphthene

Concen: 40.28 ng

RT: 9.88 min Scan# 726

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F


ClientSampleId :

SSTDCCC040




Tgt Ion:	154	Resp:	592690
Ion Ratio	Lower	Upper	
154	100		
153	113.7	89.5	134.3
152	54.0	42.7	64.1

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E



#52

3-Nitroaniline

Concen: 38.00 ng


RT: 9.79 min Scan# 718

Delta R.T. -0.01 min



Lab File: BF088565.D


Acq: 1 Jul 2016 10:13

Tgt Ion:	138	Resp:	177034
Ion Ratio	Lower	Upper	
138	100		
108	11.1	8.5	12.7
92	132.6	95.7	143.5



Abundance Ion 138.00 (137.70 to 138.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 92.00 (91.70 to 92.70): BF0









#53
2,4-Dinitrophenol
Concen: 30.66 ng
RT: 9.90 min Scan# 727
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
184	100	49611		
63	89.9	57.6	86.4#	
154	71.5	53.5	80.3	




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#54
Dibenzofuran
Concen: 39.49 ng
RT: 10.06 min Scan# 741
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
168	100	760510		
139	33.3	26.4	39.6	
169	13.0	10.4	15.6	









#55
4-Nitrophenol
Concen: 43.82 ng
RT: 9.95 min Scan# 732
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion:139 Resp: 155138
Ion Ratio Lower Upper
139 100
109 71.2 48.9 88.9
65 101.4 84.9 124.9




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#56
2,4-Dinitrotoluene
Concen: 46.30 ng
RT: 10.03 min Scan# 739
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion:165 Resp: 221845
Ion Ratio Lower Upper
165 100
63 37.0 22.0 33.0#
89 66.5 41.1 61.7#
182 2.5 2.0 3.0





#57

Fluorene

Concen: 36.39 ng

RT: 10.39 min Scan# 770

Delta R.T. -0.01 min

Lab File: BF088565.D


Acq: 1 Jul 2016 10:13

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040



Tgt Ion:166 Resp: 540137

Ion Ratio Lower Upper




166 100

165 99.1 77.8 116.8

167 14.2 11.2 16.8

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



#58

2,3,4,6-Tetrachlorophenol

Concen: 42.76 ng

RT: 10.17 min Scan# 751

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion:232 Resp: 144863




Ion Ratio Lower Upper


232 100

131 49.0 0.9 1.3#

130 2.6 1.5 2.3#

166 32.5 0.5 0.7#









#59
Diethylphthalate
Concen: 39.47 ng
RT: 10.27 min Scan# 760
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	654911		
177	21.6	16.9	25.3	
150	12.6	10.1	15.1	




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#60
4-Chlorophenyl-phenylether
Concen: 38.64 ng
RT: 10.39 min Scan# 770
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
204	100	266480		
206	33.3	26.3	39.5	
141	68.6	55.0	82.6	





#61

4-Nitroaniline

Concen: 45.04 ng

RT: 10.41 min Scan# 772

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F


ClientSampleId :

SSTDCCC040




Tgt Ion:	138	Resp:	201904
Ion Ratio	Lower	Upper	
138	100		
92	52.9	27.3	67.3
108	73.3	46.7	86.7

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



Abundance Ion 138.00 (137.70 to 138.70): E
Ion 92.00 (91.70 to 92.70): BF0
Ion 108.00 (107.70 to 108.70): E



#62

Azobenzene

Concen: 41.27 ng

RT: 10.55 min Scan# 784




Delta R.T. -0.00 min


Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion:	77	Resp:	781244
Ion Ratio	Lower	Upper	
77	100		
182	23.7	4.4	44.4
105	23.0	3.8	43.8
51	25.9	9.3	49.3

Abundance Ion 77.00 (76.70 to 77.70): BF0
Ion 182.00 (181.70 to 182.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 51.00 (50.70 to 51.70): BF0






#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.32 min Scan# 852
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040




Tgt Ion	Ratio	Resp	Lower	Upper
188	100	451670		
94	9.8	9.0	13.6	
80	10.5	10.0	15.0	

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM

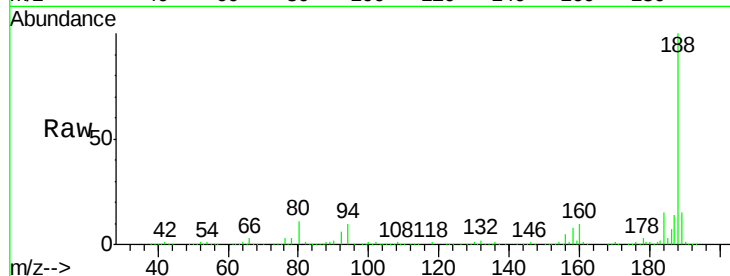


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


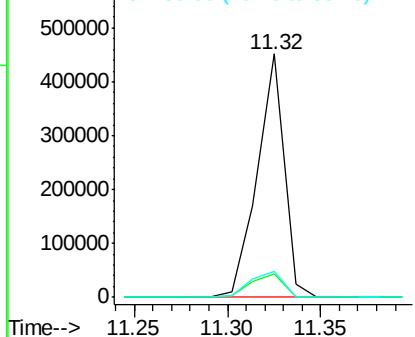



#64
4,6-Dinitro-2-methylphenol
Concen: 32.43 ng
RT: 10.43 min Scan# 774
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
198	100	78352		
51	67.9	39.6	79.6	
105	66.3	36.6	76.6	



Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF0
Ion 105.00 (104.70 to 105.70): E

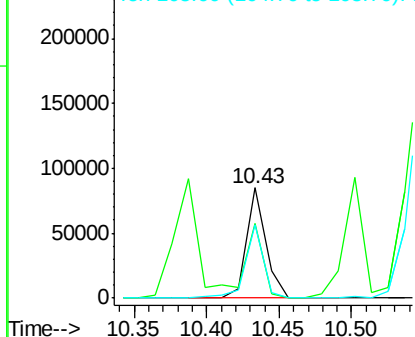







#65
 n-Nitrosodiphenylamine
 Concen: 34.31 ng
 RT: 10.50 min Scan# 780
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
169	100	524502		
168	66.6	53.4	80.0	
167	36.6	29.4	44.0	




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM

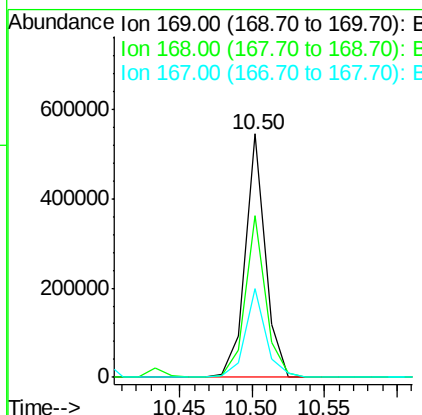

#66
 4-Bromophenyl-phenylether
 Concen: 38.84 ng
 RT: 10.88 min Scan# 813
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
248	100	176782		
250	98.6	77.1	115.7	
141	51.9	50.6	76.0	









#67
Hexachlorobenzene
Concen: 35.47 ng
RT: 10.94 min Scan# 818
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp Lower	Resp Upper
284	100		
142	44.9	35.8	53.8
249	33.3	25.8	38.6




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM

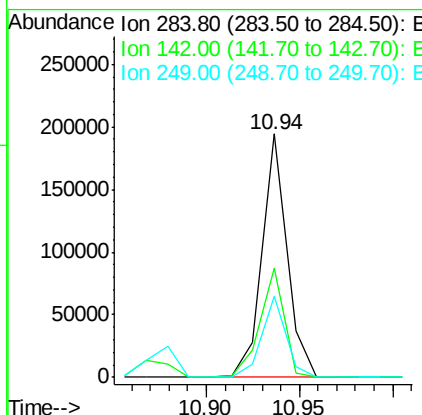

#68
Atrazine
Concen: 38.06 ng
RT: 11.03 min Scan# 826
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp Lower	Resp Upper
200	100		
173	30.8	4.0	44.0
215	43.6	29.3	69.3





#69

Pentachlorophenol

Concen: 39.54 ng

RT: 11.13 min Scan# 835

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion:	266	Resp:	117892
Ion Ratio		Lower	Upper
266	100		
268	63.6	52.8	79.2
264	61.3	49.6	74.4

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM

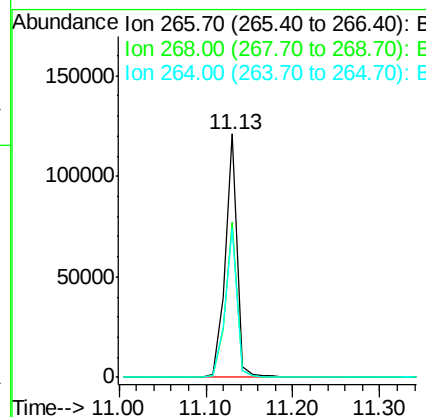

#70

Phenanthrene

Concen: 35.23 ng




RT: 11.35 min Scan# 854


Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion:	178	Resp:	869794
Ion Ratio		Lower	Upper
178	100		
176	20.0	15.8	23.6
179	15.9	13.0	19.4

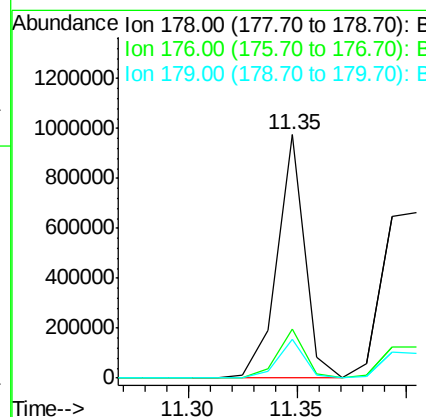







#71
 Anthracene
 Concen: 38.50 ng
 RT: 11.40 min Scan# 859
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.6	23.4
179	15.2	12.8	19.2




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM

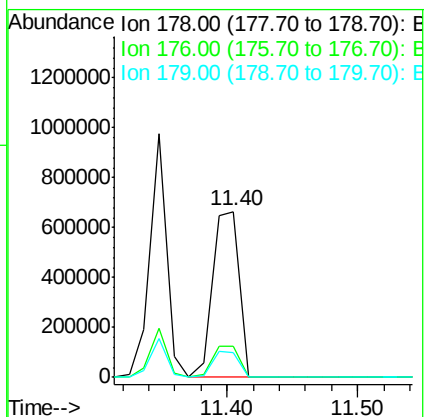

#72
 Carbazole
 Concen: 39.11 ng
 RT: 11.55 min Scan# 872
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
167	100		
166	22.2	17.8	26.6
139	13.7	11.2	16.8

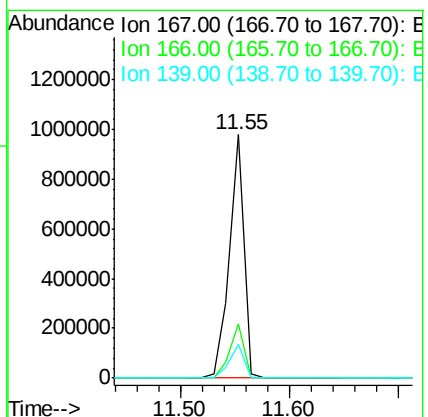

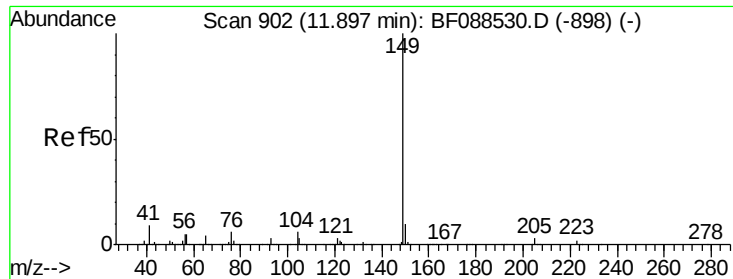

#73

Di-n-butylphthalate

Concen: 39.54 ng

RT: 11.90 min Scan# 902

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion:	149	Resp:	1062697
Ion Ratio	Lower	Upper	
149	100		
150	9.2	7.8	11.6
104	4.8	4.0	6.0

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM

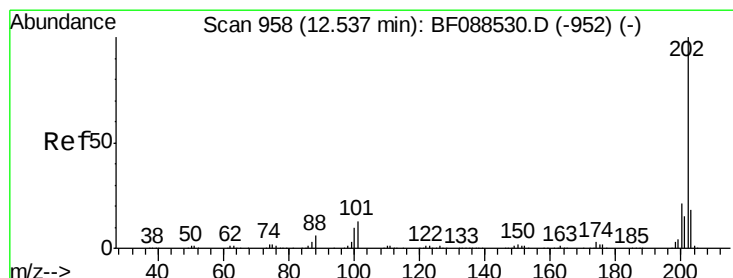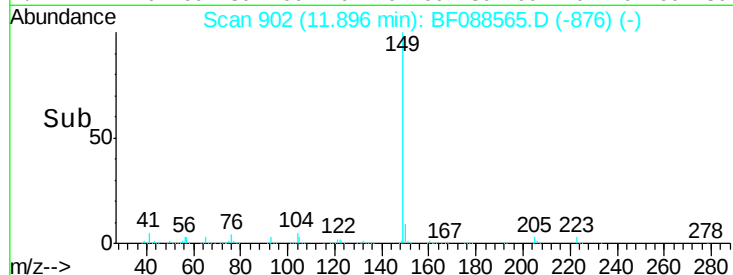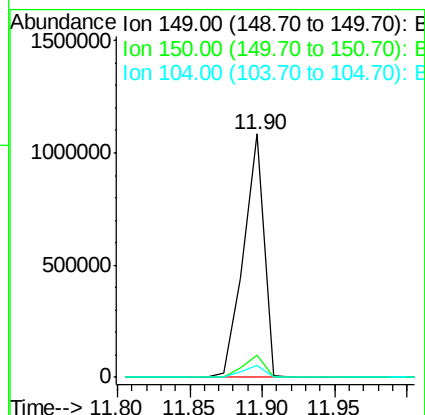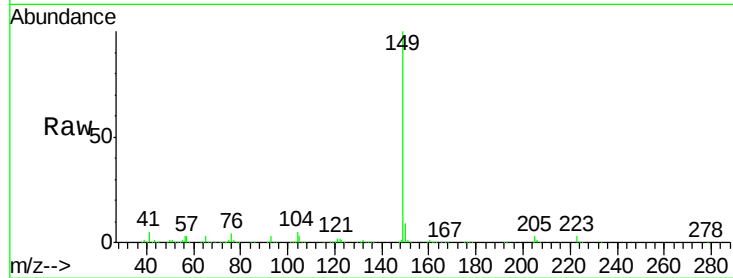

#74

Fluoranthene

Concen: 36.92 ng




RT: 12.53 min Scan# 957


Delta R.T. -0.01 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion:	202	Resp:	924001
Ion Ratio	Lower	Upper	
202	100		
101	17.0	0.0	33.1
203	18.0	0.0	38.1

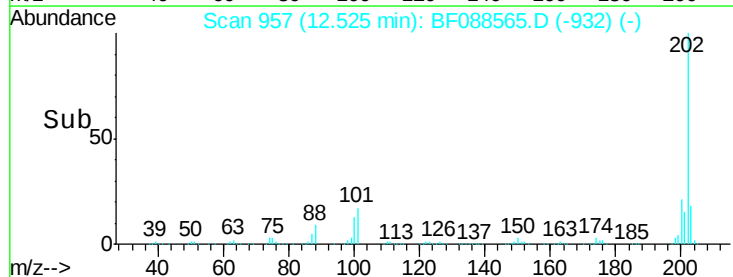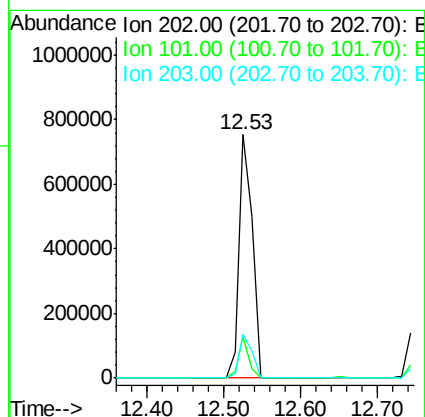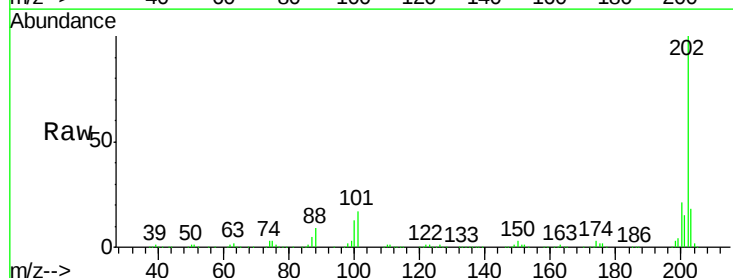

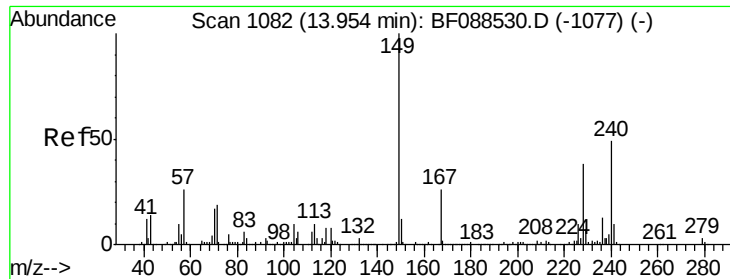

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.95 min Scan# 1082

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040

Tgt Ion: 240 Resp: 339500
Ion Ratio Lower Upper

240 100


120 12.1 6.8 10.2#

236 26.1 20.2 30.2




Manual Integrations
APPROVED

sohil

7/5/2016 7:30:44 PM

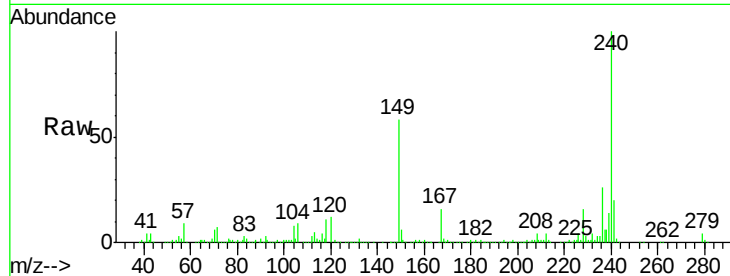

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

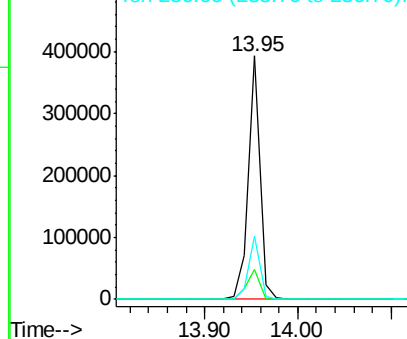

#76

Benzidine

Concen: 31.09 ng

RT: 12.65 min Scan# 968

Delta R.T. -0.01 min

Lab File: BF088565.D


Acq: 1 Jul 2016 10:13

Tgt Ion: 184 Resp: 533591
Ion Ratio Lower Upper



184 100


185 15.8 12.5 18.7

183 12.0 9.3 13.9



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 185.00 (184.70 to 185.70): E
Ion 183.00 (182.70 to 183.70): E

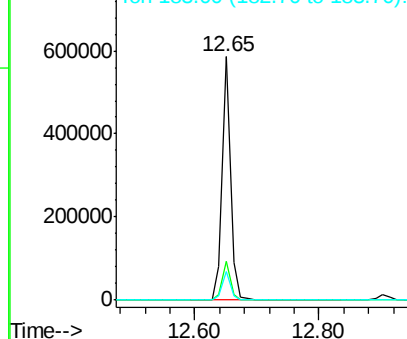




#77
 Pyrene
 Concen: 32.42 ng
 RT: 12.75 min Scan# 977
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040




Tgt Ion	Ratio	Resp	Lower	Upper
202	100	933269		
200	21.8		17.4	26.2
203	18.1		14.5	21.7

Manual Integrations
 APPROVED

sohil
 7/5/2016 7:30:44 PM




Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 200.00 (199.70 to 200.70): E
 Ion 203.00 (202.70 to 203.70): E


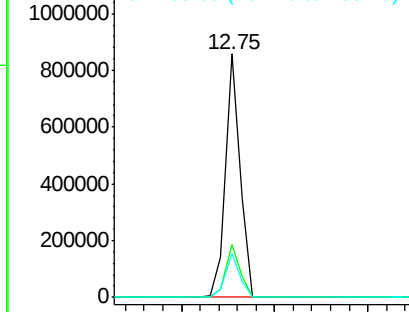



#78
 Terphenyl-d14
 Concen: 66.86 ng
 RT: 12.90 min Scan# 990
 Delta R.T. -0.01 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
244	100	1019117		
212	8.1		6.0	9.0
122	16.5		11.2	16.8



Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

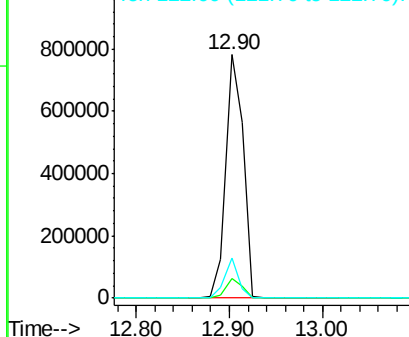







#79
Butylbenzylphthalate
Concen: 33.76 ng
RT: 13.38 min Scan# 1032
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	433485		
91	80.1	48.0	72.0#	
206	17.5	16.0	24.0	




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#80
Benzo(a)anthracene
Concen: 35.82 ng
RT: 13.94 min Scan# 1081
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	783081		
226	27.7	22.3	33.5	
229	19.8	16.0	24.0	









#81
 3,3'-Dichlorobenzidine
 Concen: 39.21 ng
 RT: 13.91 min Scan# 1078
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	322303		
254	64.2	52.6	78.8	
126	13.5	6.2	9.2	




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM

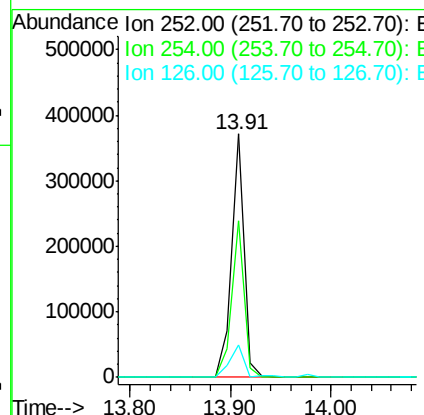

#82
 Chrysene
 Concen: 33.26 ng
 RT: 13.98 min Scan# 1084
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	719366		
226	31.5	25.4	38.2	
229	20.1	16.3	24.5	

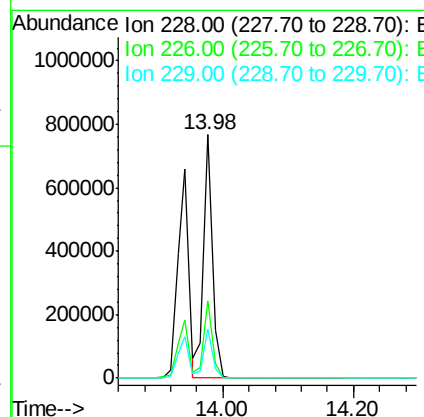



#83

Bis(2-ethylhexyl)phthalate

Concen: 34.91 ng

RT: 13.94 min Scan# 1081

Delta R.T. -0.01 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040

Tgt Ion:149 Resp: 511775
Ion Ratio Lower Upper

149 100


167 24.3 20.5 30.7

279 1.9 2.0 3.0#




Manual Integrations
APPROVED

sohil

7/5/2016 7:30:44 PM



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

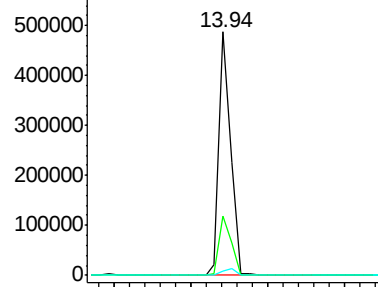

#84

Di-n-octyl phthalate

Concen: 41.42 ng

RT: 14.56 min Scan# 1135

Delta R.T. -0.00 min

Lab File: BF088565.D


Acq: 1 Jul 2016 10:13

Tgt Ion:149 Resp: 1031605
Ion Ratio Lower Upper



149 100


167 1.5 0.0 0.0#

43 9.9 0.0 0.0#



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 43.00 (42.70 to 43.70): BF0

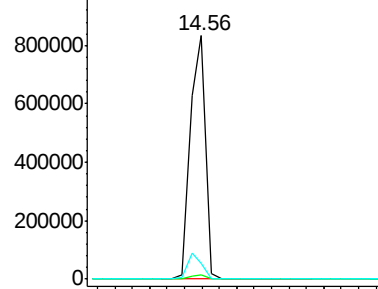

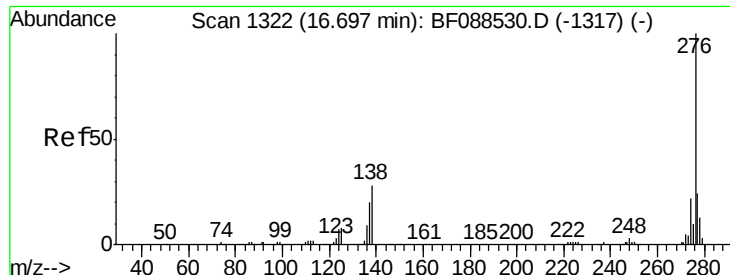





#85
 Indeno(1,2,3-cd)pyrene
 Concen: 34.09 ng
 RT: 16.70 min Scan# 1322
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	31.2	0.0	0.0#
277	25.3	0.0	0.0#




Manual Integrations
 APPROVED


sohil
 7/5/2016 7:30:44 PM



#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.35 min Scan# 1204
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Resp Lower	Resp Upper
264	100		
260	23.7	19.2	28.8
265	21.4	16.9	25.3





#87

Benzo(b)fluoranthene

Concen: 43.02 ng m

RT: 14.96 min Scan# 1170

Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Instrument :

BNA_F





ClientSampleId :

SSTDCCC040

Tgt Ion:	252	Resp:	830032
Ion Ratio	Lower	Upper	
252	100		
253	21.9	17.4	26.2
125	8.9	7.1	10.7

Manual Integrations
APPROVED

sohil
7/5/2016 7:30:44 PM



#88

Benzo(k)fluoranthene

Concen: 32.21 ng m




RT: 14.98 min Scan# 1172


Delta R.T. -0.00 min

Lab File: BF088565.D

Acq: 1 Jul 2016 10:13

Tgt Ion:	252	Resp:	540973
Ion Ratio	Lower	Upper	
252	100		
253	22.8	18.0	27.0
125	13.9	11.2	16.8









#89
Benzo(a)pyrene
Concen: 38.47 ng
RT: 15.29 min Scan# 1199
Delta R.T. -0.01 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.9	26.9
125	14.8	12.5	18.7




Manual Integrations
APPROVED


sohil
7/5/2016 7:30:44 PM



#90
Dibenzo(a,h)anthracene
Concen: 35.80 ng
RT: 16.72 min Scan# 1324
Delta R.T. -0.00 min
Lab File: BF088565.D
Acq: 1 Jul 2016 10:13

Tgt Ion	Ratio	Lower	Upper
278	100		
139	17.5	15.7	23.5
279	24.4	19.4	29.2





#91
 Benzo(g,h,i)perylene
 Concen: 34.73 ng
 RT: 17.11 min Scan# 1358
 Delta R.T. -0.00 min
 Lab File: BF088565.D
 Acq: 1 Jul 2016 10:13

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tgt Ion:	276	Resp:	490275
Ion Ratio		Lower	Upper
276	100		
277	23.2	18.9	28.3
138	23.5	21.4	32.2

Manual Integrations
 APPROVED

sohil
 7/5/2016 7:30:44 PM

