

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070116\
 Data File : BF088575.D
 Acq On : 1 Jul 2016 15:20
 Operator : UM/SJ
 Sample : H3808-15 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.872	22	25	116	rVB	3581664	10643154	100.00%	43.101%
2	5.393	328	333	340	rVB	595188	614692	5.78%	2.489%
3	6.433	417	424	429	rVB	453822	615448	5.78%	2.492%
4	6.570	432	436	439	rVV	711318	641282	6.03%	2.597%
5	6.810	452	457	460	rBV	849083	837425	7.87%	3.391%
6	6.959	466	470	473	rVB	491077	461089	4.33%	1.867%
7	7.359	502	505	508	rBV	277275	346914	3.26%	1.405%
8	8.090	563	569	577	rVB	1225681	1113970	10.47%	4.511%
9	9.165	656	663	666	rVB	815798	687648	6.46%	2.785%
10	9.839	719	722	730	rBV2	1062171	1161377	10.91%	4.703%
11	10.616	786	790	797	rBV2	263298	352313	3.31%	1.427%
12	11.325	848	852	856	rBV2	786607	1547197	14.54%	6.266%
13	12.525	953	957	960	rBV	935955	801997	7.54%	3.248%
14	12.754	973	977	980	rBV	752086	822394	7.73%	3.330%
15	12.902	984	990	993	rBV	642811	645531	6.07%	2.614%
16	13.942	1077	1081	1087	rBV	1125018	1836103	17.25%	7.435%
17	14.948	1167	1169	1174	rVB	312712	595144	5.59%	2.410%
18	15.348	1201	1204	1215	rVB	652922	970108	9.11%	3.929%


Sum of corrected areas: 24693786

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070116\
Data File : BF088575.D
Acq On : 1 Jul 2016 15:20
Operator : UM/SJ
Sample : H3808-15 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-08-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: rteint.p

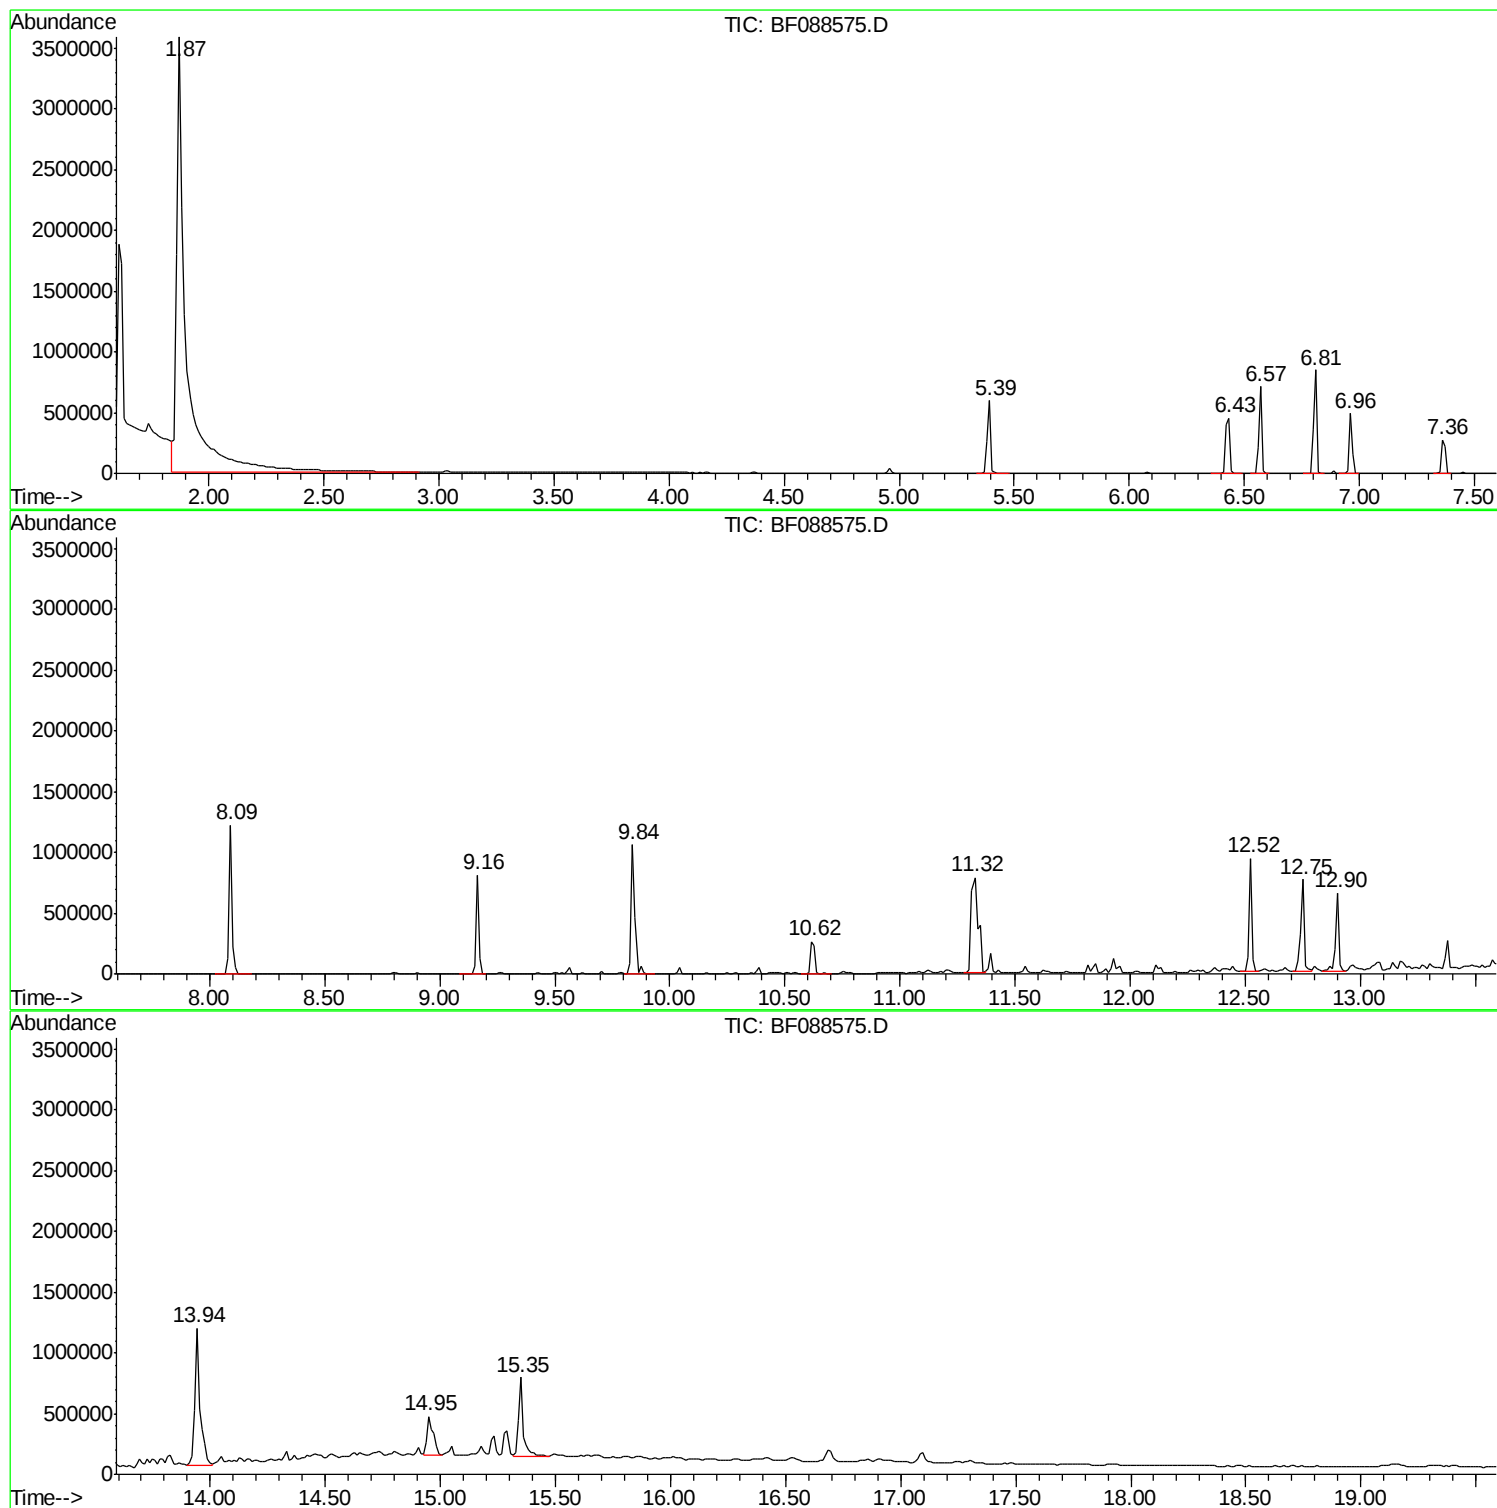

DbaaaPbaah::ZZ\NRPBEMM1BBAFNDATA\BB0000166\
 DbaaaFfile::BB0088335DD
 Aeqq00n :: 11JUW120066 155200
 Oppaaa00r::UMMSJ
 Saaapbae::HB80081555X
 Mmsc ::
 AASSVaal::122 SaaapbaeMMWifpbaer:11

Instrument :
 BNA_F
 ClientSampleId :
 SB-08-COMP

QqaabtMebbdd::ZZ\NRPBEMM1BBAFMEH00S82Z0BB000066MM
 QqaabtTfile::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICCLibbaay::CC\DaababbaeN0\$T11LL
 TICCIbeggaaionPaaabbaess:rteabtp

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
