

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070117\
 Data File : BF096402.D
 Acq On : 2 Jul 2017 2:08
 Operator : SJ/MA
 Sample : I3908-10 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-58-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	476	480	487	rBV	47116	53734	4.48%	0.546%
2	5.334	549	552	556	rBV	381778	337154	28.12%	3.424%
3	6.357	723	726	731	rVB	403470	316452	26.40%	3.213%
4	6.498	746	750	753	rBV	399786	326361	27.22%	3.314%
5	6.734	786	790	793	rBV	1218547	962577	80.29%	9.774%
6	6.887	813	816	820	rVB	293316	235076	19.61%	2.387%
7	7.287	880	884	887	rBV	240048	186647	15.57%	1.895%
8	8.016	1003	1008	1011	rBV	1459746	1198845	100.00%	12.173%
9	8.728	1126	1129	1132	rVB	20498	13891	1.16%	0.141%
10	9.086	1187	1190	1194	rVB	338325	273677	22.83%	2.779%
11	9.481	1255	1257	1259	rBV	36560	26274	2.19%	0.267%
12	9.663	1285	1288	1294	rVB5	10719	14798	1.23%	0.150%
13	9.769	1300	1306	1309	rBV	981172	921243	76.84%	9.354%
14	9.969	1337	1340	1344	rVB	16653	13986	1.17%	0.142%
15	10.545	1435	1438	1444	rVB	152584	122849	10.25%	1.247%
16	10.680	1458	1461	1468	rVB2	14561	19020	1.59%	0.193%
17	11.133	1535	1538	1541	rVB3	10670	14505	1.21%	0.147%
18	11.245	1553	1557	1559	rBV	1082407	882888	73.64%	8.965%
19	11.269	1559	1561	1564	rVV	256487	193349	16.13%	1.963%
20	11.316	1567	1569	1572	rVB	47823	38444	3.21%	0.390%
21	11.469	1591	1595	1600	rBV2	27820	26468	2.21%	0.269%
22	11.745	1639	1642	1644	rBV	43036	32558	2.72%	0.331%
23	11.775	1644	1647	1650	rVV	63973	56571	4.72%	0.574%
24	11.822	1650	1655	1657	rVV	16969	18418	1.54%	0.187%
25	11.857	1657	1661	1663	rVV	54279	60573	5.05%	0.615%
26	11.880	1663	1665	1669	rVB	29146	25140	2.10%	0.255%
27	12.039	1687	1692	1694	rBV	26621	27672	2.31%	0.281%
28	12.192	1715	1718	1721	rBV4	13013	14992	1.25%	0.152%
29	12.292	1732	1735	1739	rBV	30097	40227	3.36%	0.408%
30	12.327	1739	1741	1743	rVV3	18860	17884	1.49%	0.182%
31	12.374	1747	1749	1756	rVB5	20087	22055	1.84%	0.224%
32	12.451	1758	1762	1766	rBV	362535	306178	25.54%	3.109%
33	12.498	1768	1770	1773	rBV4	12139	15423	1.29%	0.157%
34	12.586	1780	1785	1789	rBV7	13100	27545	2.30%	0.280%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070117\
Data File : BF096402.D
Acq On : 2 Jul 2017 2:08
Operator : SJ/MA
Sample : I3908-10 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-58-1.5-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.680	1795	1801	1803	rBV	307971	310011	25.86%	3.148%
36	12.827	1823	1826	1832	rVB	248118	234867	19.59%	2.385%
37	12.898	1836	1838	1841	rVB2	15406	15162	1.26%	0.154%
38	13.004	1854	1856	1859	rVB	55256	53034	4.42%	0.539%
39	13.074	1865	1868	1872	rVB3	23924	21107	1.76%	0.214%
40	13.110	1872	1874	1876	rBV	34733	29091	2.43%	0.295%
41	13.204	1887	1890	1892	rBV	27432	25340	2.11%	0.257%
42	13.233	1892	1895	1898	rVV2	30068	24569	2.05%	0.249%
43	13.310	1905	1908	1913	rBV	35623	39255	3.27%	0.399%
44	13.510	1939	1942	1944	rBV	21775	22204	1.85%	0.225%
45	13.621	1957	1961	1964	rBV2	38422	60596	5.05%	0.615%
46	13.651	1964	1966	1968	rVV	27753	23826	1.99%	0.242%
47	13.874	1999	2004	2006	rBV2	959993	1009668	84.22%	10.252%
48	13.898	2006	2008	2015	rVB	174940	146904	12.25%	1.492%
49	14.086	2038	2040	2042	rBV2	23667	19959	1.66%	0.203%
50	14.880	2171	2175	2182	rVB	113790	222273	18.54%	2.257%
51	15.163	2221	2223	2228	rVB	47216	52664	4.39%	0.535%
52	15.221	2230	2233	2239	rVB	86600	113260	9.45%	1.150%
53	15.286	2239	2244	2251	rBV	426846	580881	48.45%	5.898%


Sum of corrected areas: 9848145

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070117\
Data File : BF096402.D
Acq On : 2 Jul 2017 2:08
Operator : SJ/MA
Sample : I3908-10 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-58-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

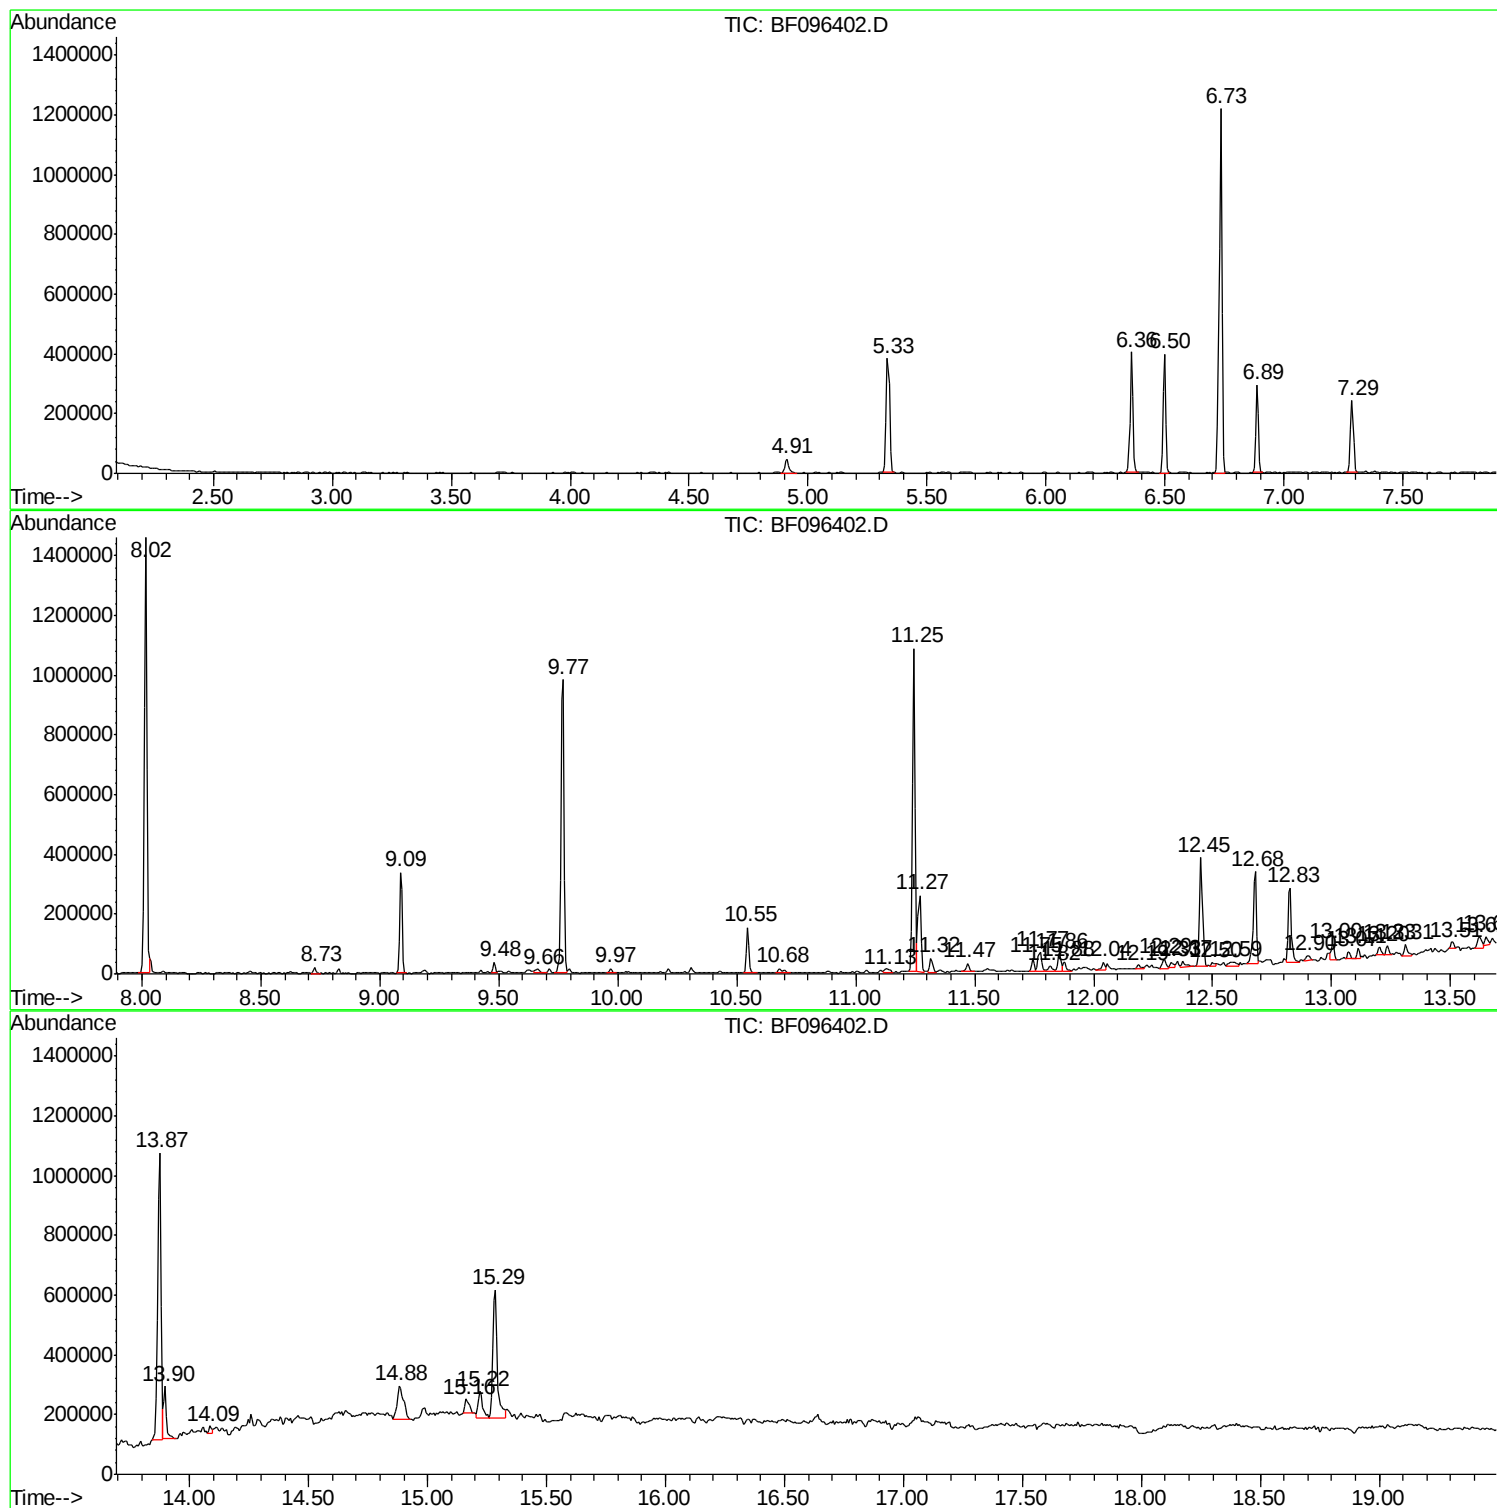

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070117\
Data File : BF096402.D
Acq On : 2 Jul 2017 2:08
Operator : SJ/MA
Sample : I3908-10 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-58-1.5-3







Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	6.78 ng	326361	1,4-Dichlorobenzene-d4	6.73

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4			5-Aminoindole	132	C8H8N2	005192-03-0	12
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

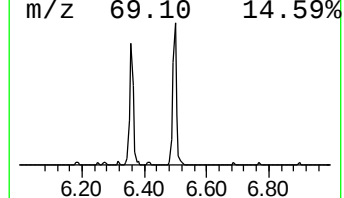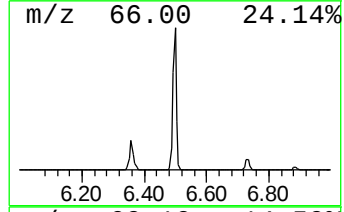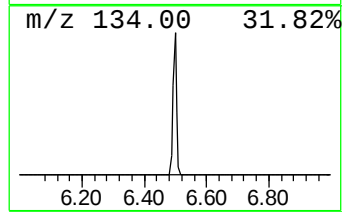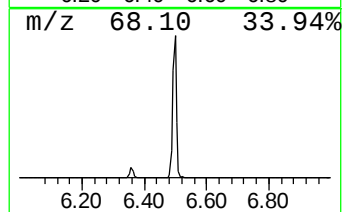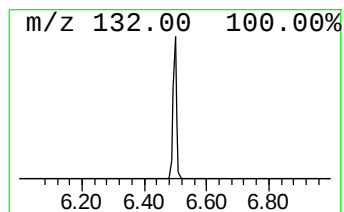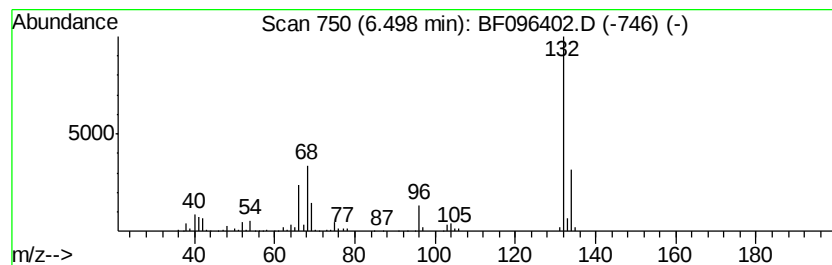

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070117\
Data File : BF096402.D
Acq On : 2 Jul 2017 2:08
Operator : SJ/MA
Sample : I3908-10 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-58-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	6.8	ng	326361	1	6.73	962577	20.0