


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070117\
Data File : BF096369.D
Acq On : 1 Jul 2017 10:40
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 03 01:43:12 2017

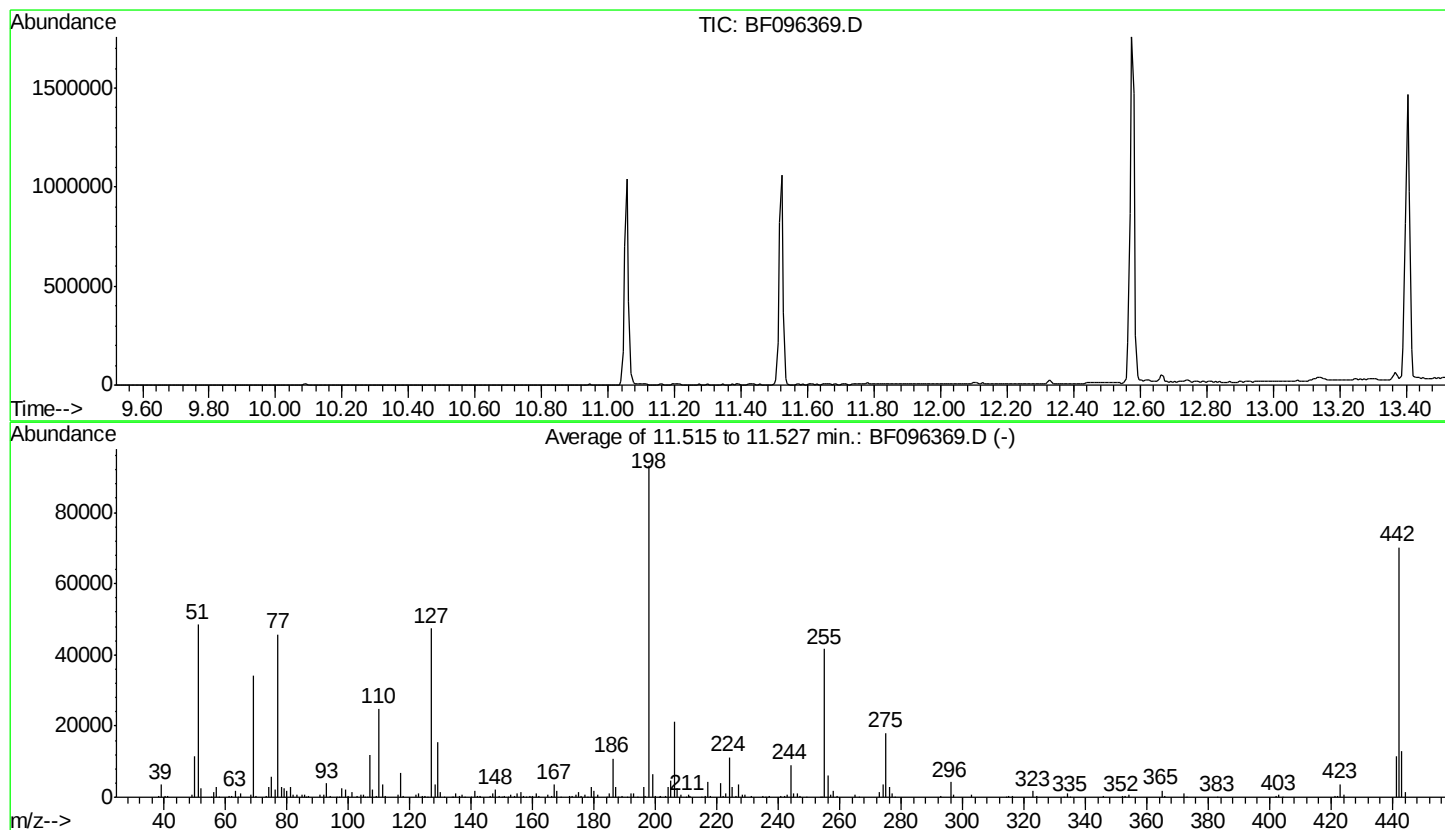

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	48473	PASS
68	69	0.00	2	1.9	658	PASS
69	198	0.00	100	36.8	34266	PASS
70	69	0.00	2	0.8	268	PASS
127	198	10	80	50.8	47320	PASS
197	198	0.00	2	0.4	402	PASS
198	198	100	100	100.0	93176	PASS
199	198	5	9	6.9	6437	PASS
275	198	10	60	19.5	18148	PASS
365	198	1	100	2.0	1910	PASS
441	442	0.01	24	16.6	11640	PASS
442	198	50	100	75.3	70178	PASS
443	442	15	24	18.6	13069	PASS