


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070117\
 Data File : BF096378.D
 Acq On : 1 Jul 2017 14:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 01:43:12 2017

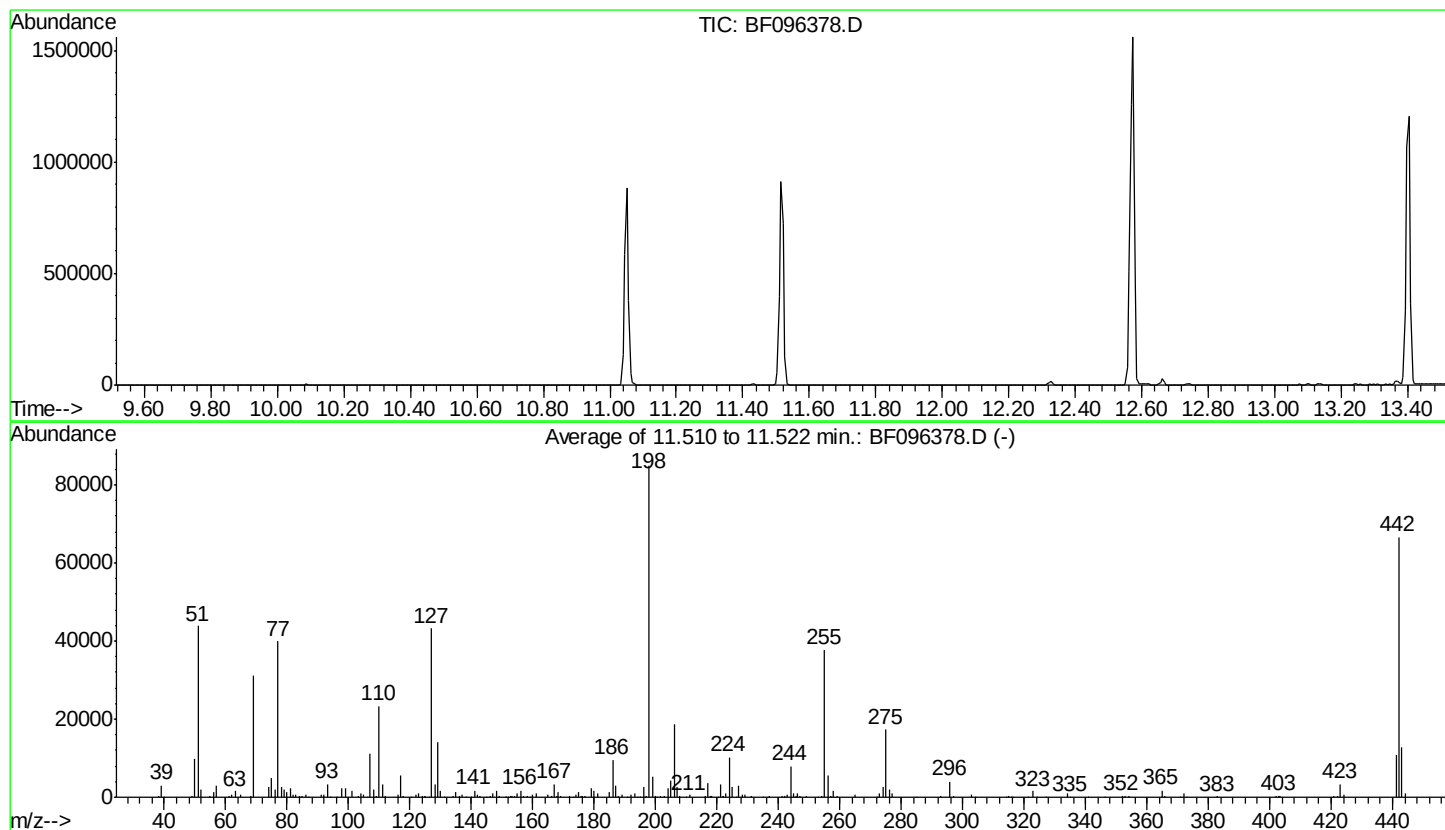

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	43920	PASS
68	69	0.00	2	1.6	500	PASS
69	198	0.00	100	36.7	31210	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	43256	PASS
197	198	0.00	2	0.5	416	PASS
198	198	100	100	100.0	84960	PASS
199	198	5	9	6.2	5238	PASS
275	198	10	60	20.4	17301	PASS
365	198	1	100	2.1	1773	PASS
441	442	0.01	24	16.1	10709	PASS
442	198	50	100	78.5	66704	PASS
443	442	15	24	19.1	12727	PASS