
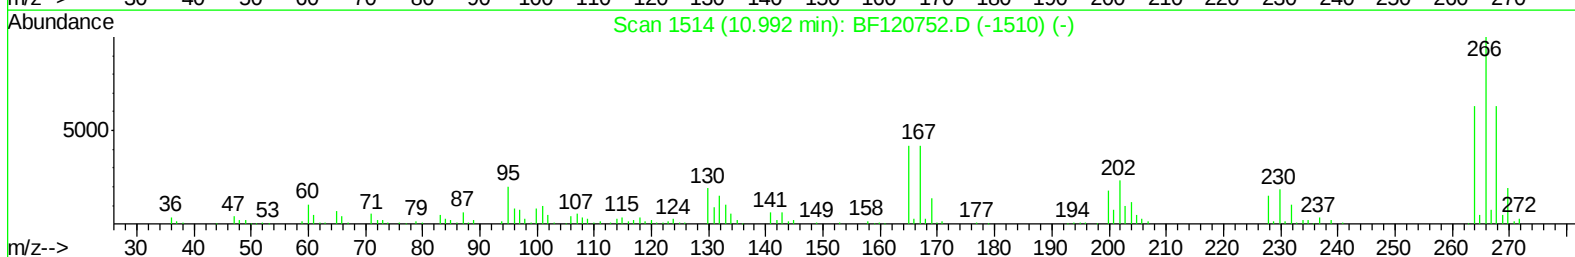
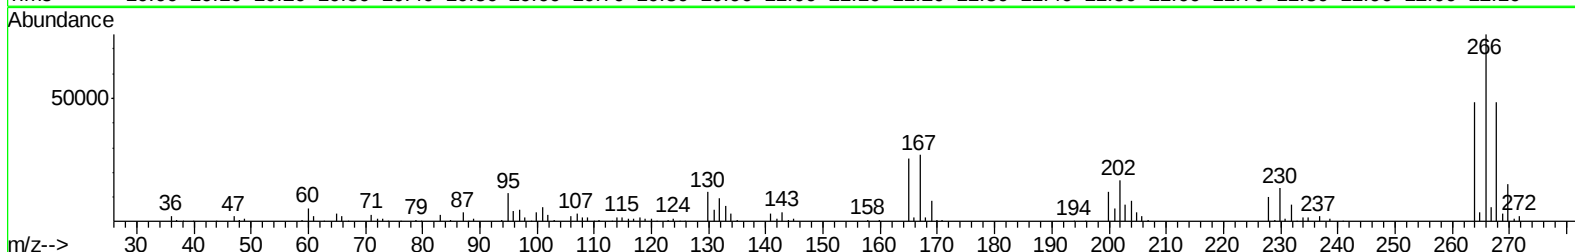


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070120\
 Data File : BF120748.D
 Acq On : 1 Jul 2020 9:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 06:07:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 01 18:02:25 2020
 Response via : Initial Calibration

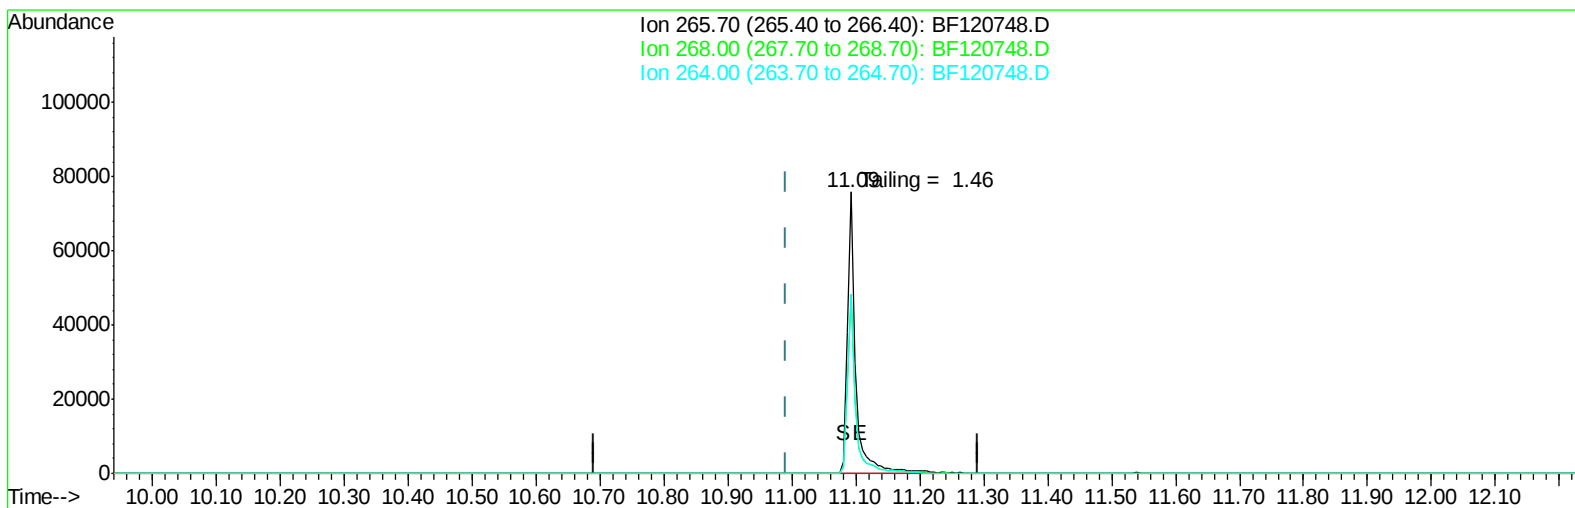

TIC: BF120748.D

(70) Pentachlorophenol (C)




11.092min (+0.100) 0.00ng

response 67222

Ion	Exp%	Act%
265.70	100	100
268.00	62.80	63.55
264.00	63.10	63.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070120\
 Data File : BF120748.D
 Acq On : 1 Jul 2020 9:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 06:07:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 01 18:02:25 2020
 Response via : Initial Calibration

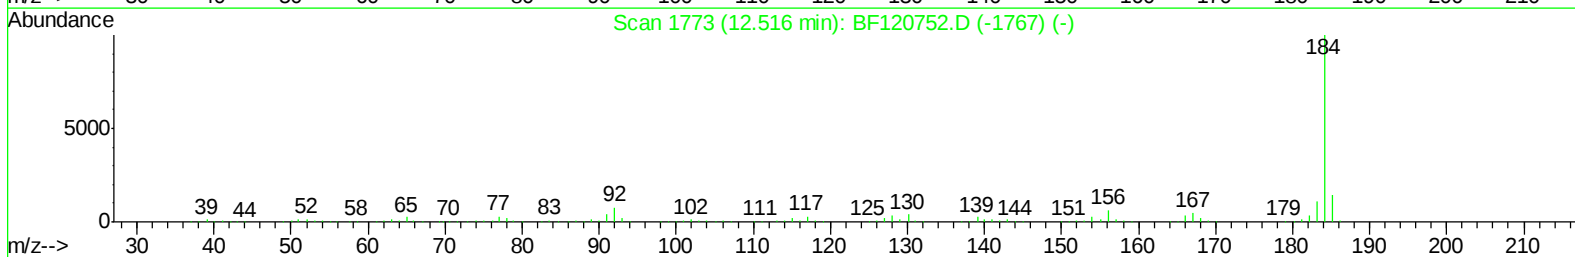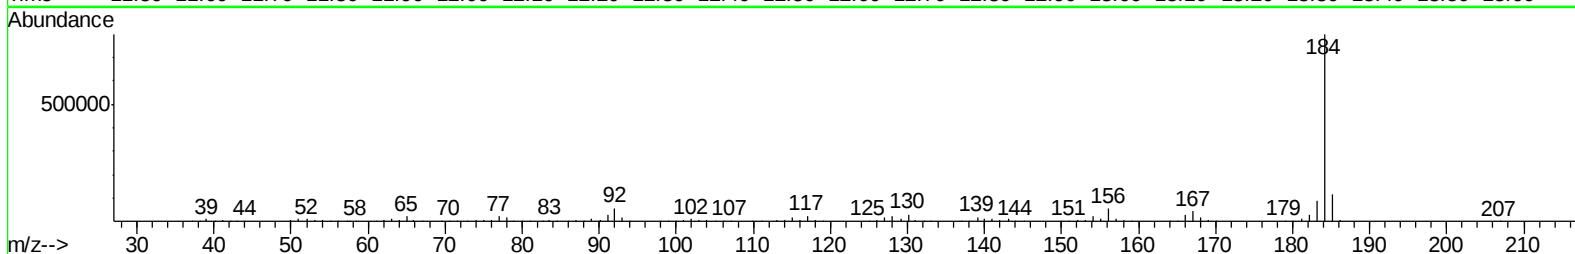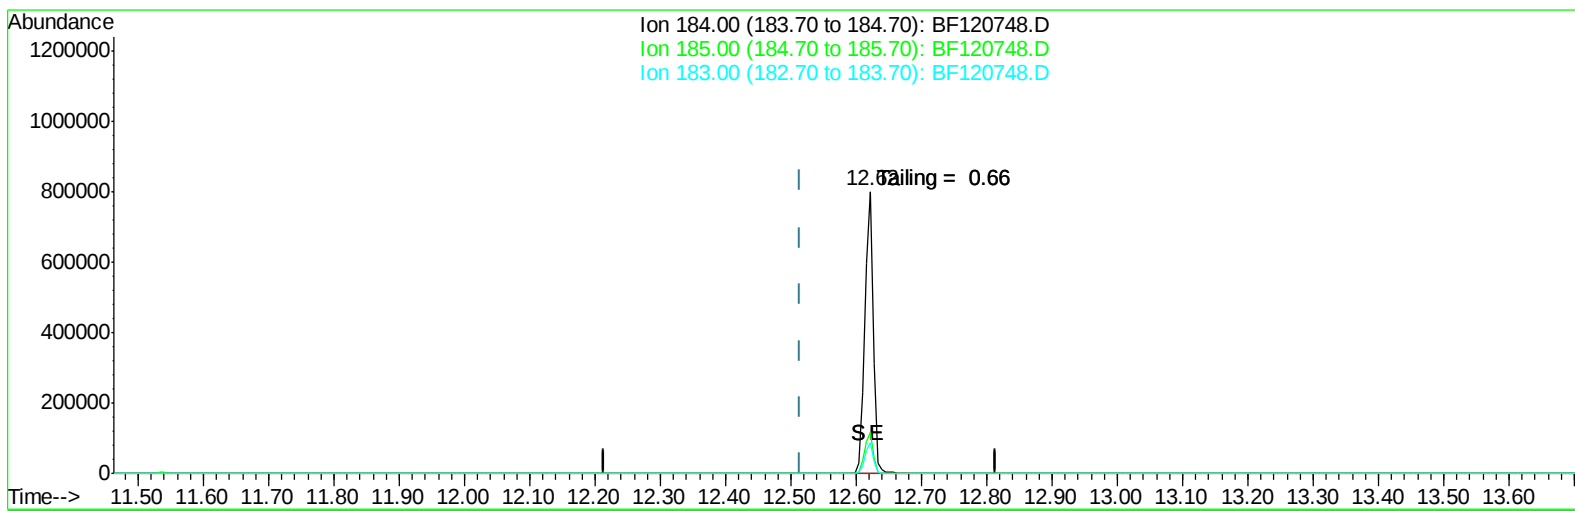

TIC: BF120748.D

(77) Benzidine

12.622min (+0.107) 0.00ng

response 713980

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.40
183.00	10.90	11.06
0.00	0.00	0.00