


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070120\
 Data File : BF120748.D
 Acq On : 1 Jul 2020 9:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 01 18:02:25 2020

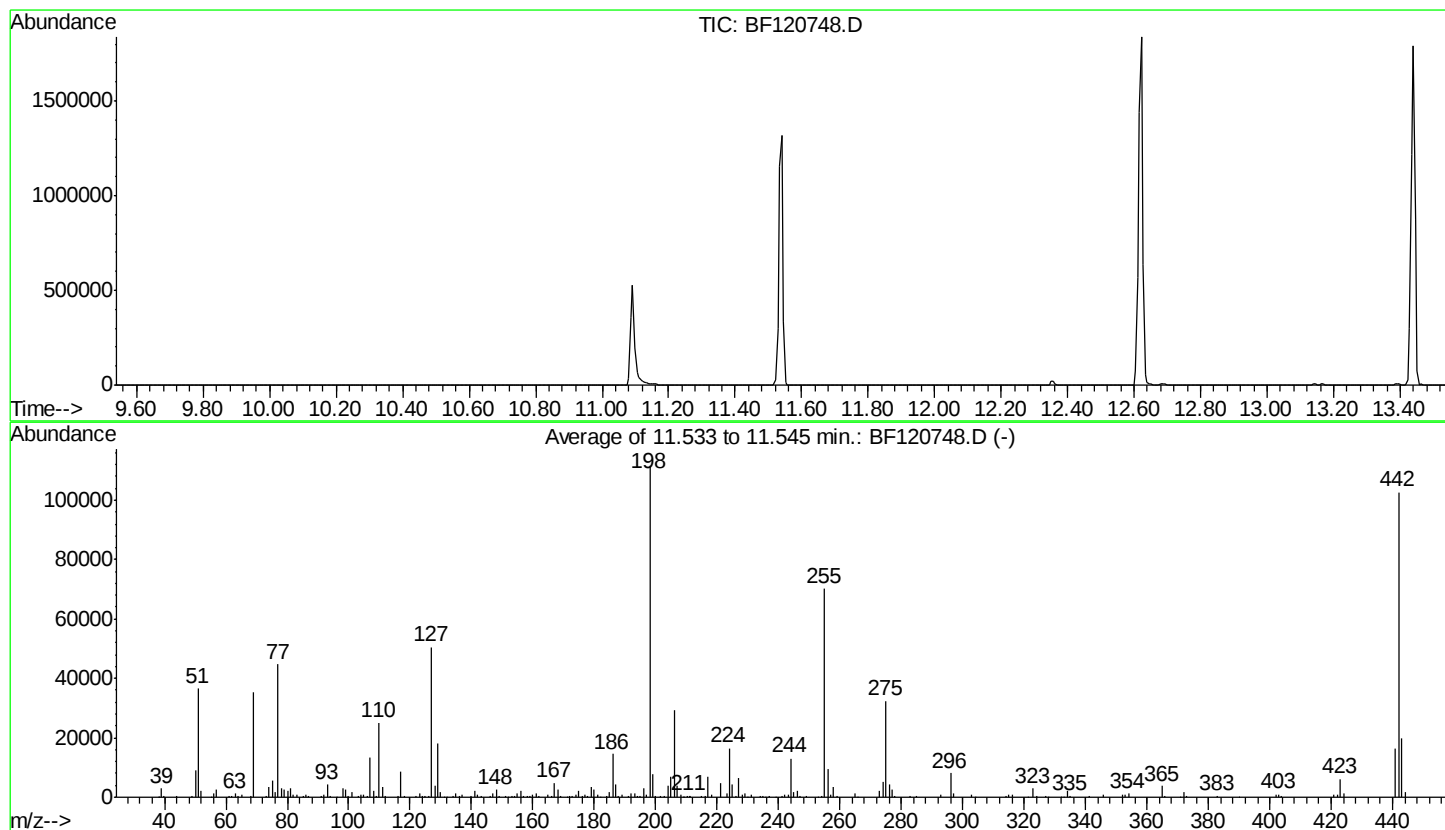

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	36464	PASS
68	69	0.00	2	1.5	514	PASS
69	198	0.00	100	31.7	35392	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	50592	PASS
197	198	0.00	2	0.7	745	PASS
198	198	100	100	100.0	111613	PASS
199	198	5	9	6.9	7650	PASS
275	198	10	60	29.1	32432	PASS
365	198	1	100	3.4	3789	PASS
441	198	0.01	100	14.8	16482	PASS
442	198	50	100	91.9	102602	PASS
443	442	15	24	19.2	19704	PASS