
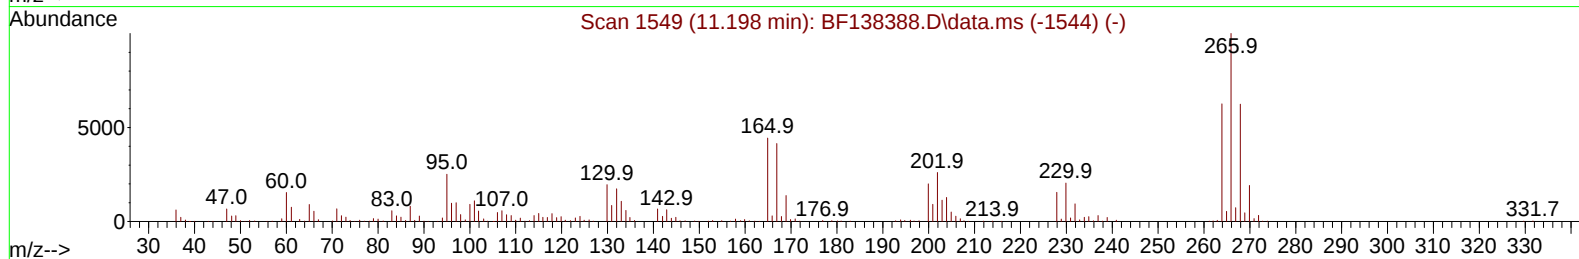
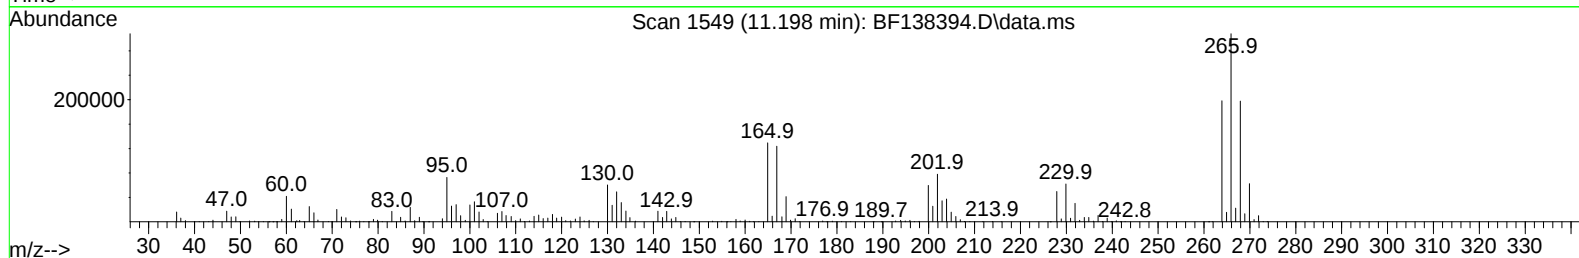


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138394.D
Acq On : 01 Jul 2024 10:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 12:11:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

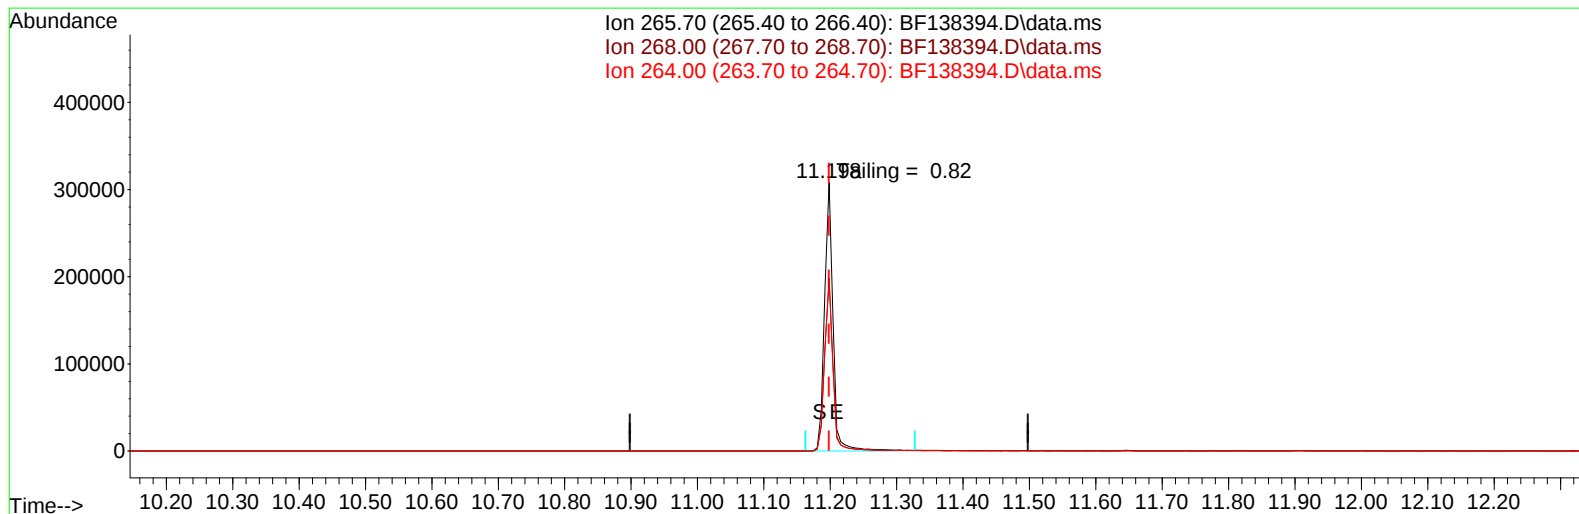

TIC: BF138394.D\data.ms




(70) Pentachlorophenol (C)

11.198min (+ 0.000) 738560.39 ng

response 275341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.21
264.00	62.50	64.38
0.00	0.00	0.00

Quant Time: Jul 01 12:11:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

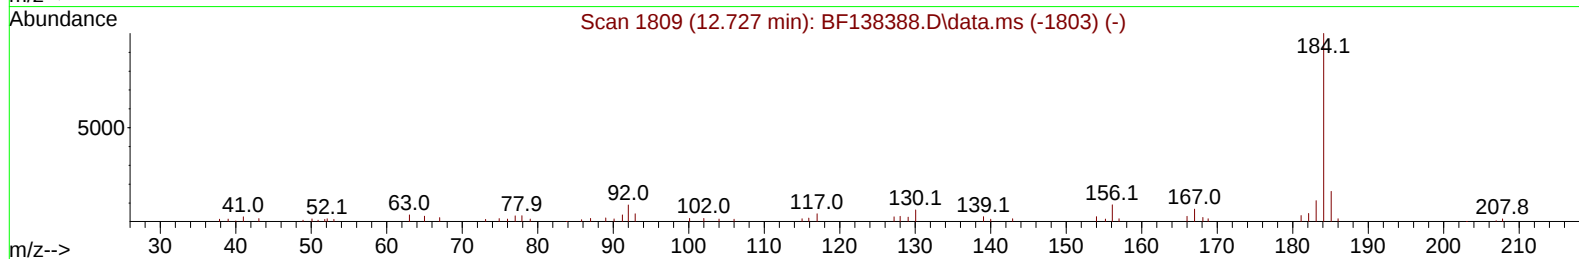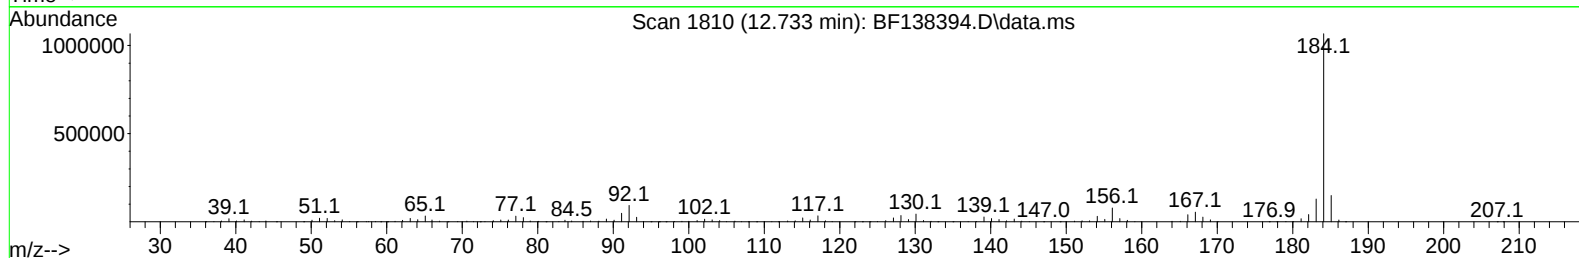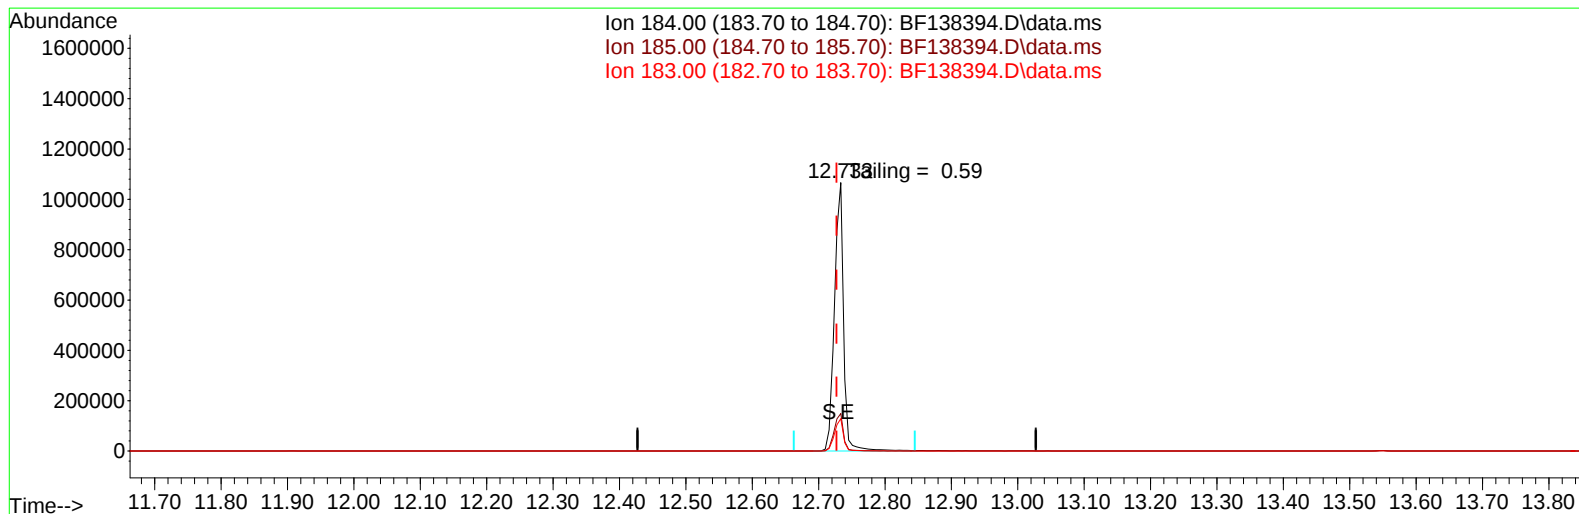

TIC: BF138394.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 36231.18 ng

```
response      1016333
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	13.98
183.00	11.30	12.06
0.00	0.00	0.00