

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
 Data File : BF138416.D
 Acq On : 01 Jul 2024 21:34
 Operator : CG\JU
 Sample : P2977-21RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OSTL-D3RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	5	11	18	rVB	1914843	2341379	76.91%	6.747%
2	3.381	216	220	231	rBV	88030	198118	6.51%	0.571%
3	5.057	501	505	507	rBV	34716	34667	1.14%	0.100%
4	5.092	507	511	517	rVB	216031	248161	8.15%	0.715%
5	5.498	576	580	589	rBV	3232934	3044356	100.00%	8.773%
6	5.816	630	634	640	rVB	67432	72464	2.38%	0.209%
7	6.510	747	752	755	rBV	3408908	2940571	96.59%	8.474%
8	6.698	781	784	789	rBV	268694	205989	6.77%	0.594%
9	6.875	810	814	817	rBV	1466199	1134970	37.28%	3.271%
10	6.934	820	824	829	rBV	47871	39858	1.31%	0.115%
11	7.434	905	909	912	rBV	2168092	1851676	60.82%	5.336%
12	7.686	948	952	958	rVB	164180	120684	3.96%	0.348%
13	8.157	1028	1032	1035	rBV	1466401	1278370	41.99%	3.684%
14	8.369	1063	1068	1074	rBV	60884	47640	1.56%	0.137%
15	8.463	1080	1084	1092	rBV	313928	262220	8.61%	0.756%
16	9.228	1210	1214	1217	rBV	3458540	2595255	85.25%	7.479%
17	9.710	1293	1296	1301	rBV	32373	36659	1.20%	0.106%
18	9.904	1323	1329	1333	rBV	1240221	1067487	35.06%	3.076%
19	10.004	1341	1346	1349	rBV	873728	1009390	33.16%	2.909%
20	10.657	1454	1457	1459	rBV	63923	59020	1.94%	0.170%
21	10.692	1459	1463	1473	rVB	1473889	1250186	41.07%	3.603%
22	10.822	1480	1485	1488	rBV	184957	167015	5.49%	0.481%
23	10.874	1491	1494	1496	rVV	400521	332874	10.93%	0.959%
24	10.910	1496	1500	1503	rVV2	321093	435851	14.32%	1.256%
25	10.939	1503	1505	1507	rVV	346546	277632	9.12%	0.800%
26	10.963	1507	1509	1512	rVV	197784	169360	5.56%	0.488%
27	11.010	1512	1517	1518	rVV2	110454	163746	5.38%	0.472%
28	11.022	1518	1519	1521	rVV	121553	73246	2.41%	0.211%
29	11.051	1521	1524	1528	rVV3	298860	370933	12.18%	1.069%
30	11.086	1528	1530	1533	rVV	295608	292448	9.61%	0.843%
31	11.133	1536	1538	1542	rVB2	164528	134105	4.41%	0.386%
32	11.274	1559	1562	1565	rBV	51930	52344	1.72%	0.151%
33	11.339	1568	1573	1576	rVB3	58907	85146	2.80%	0.245%
34	11.392	1578	1582	1584	rVV	1125540	939044	30.85%	2.706%
35	11.416	1584	1586	1588	rVB	168796	126694	4.16%	0.365%
36	11.780	1642	1648	1651	rBV	40926	38402	1.26%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
 Data File : BF138416.D
 Acq On : 01 Jul 2024 21:34
 Operator : CG\JU
 Sample : P2977-21RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OSTL-D3RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.845	1655	1659	1662	rBV2	54732	62297	2.05%	0.180%
38	11.886	1662	1666	1668	rBV3	43024	68876	2.26%	0.198%
39	11.916	1668	1671	1678	rVV2	530613	485306	15.94%	1.398%
40	12.004	1682	1686	1688	rBV2	56339	55297	1.82%	0.159%
41	12.086	1695	1700	1709	rBV4	47401	86940	2.86%	0.251%
42	12.439	1756	1760	1763	rBV2	35016	40038	1.32%	0.115%
43	12.486	1763	1768	1772	rBV6	32676	59582	1.96%	0.172%
44	12.521	1772	1774	1779	rBV4	35271	44219	1.45%	0.127%
45	12.580	1781	1784	1785	rBV	146123	118807	3.90%	0.342%
46	12.604	1785	1788	1791	rVB	513902	423965	13.93%	1.222%
47	12.698	1801	1804	1812	rBV2	125811	154260	5.07%	0.445%
48	12.827	1821	1826	1829	rBV	443248	491288	16.14%	1.416%
49	12.974	1847	1851	1854	rBV	2793855	2359258	77.50%	6.799%
50	13.045	1860	1863	1868	rBV4	33031	47788	1.57%	0.138%
51	13.133	1875	1878	1880	rBV4	29572	38585	1.27%	0.111%
52	13.157	1880	1882	1884	rVB	67601	53347	1.75%	0.154%
53	13.221	1891	1893	1896	rVB	44899	35939	1.18%	0.104%
54	13.263	1897	1900	1903	rVB2	54428	50801	1.67%	0.146%
55	13.386	1918	1921	1924	rBV	40096	48305	1.59%	0.139%
56	13.545	1945	1948	1950	rBV	45208	38759	1.27%	0.112%
57	13.663	1966	1968	1972	rVB	62028	58261	1.91%	0.168%
58	13.827	1994	1996	2000	rBV3	40811	54621	1.79%	0.157%
59	13.868	2000	2003	2011	rVB	350468	384546	12.63%	1.108%
60	14.027	2022	2030	2032	rBV3	1079567	1451529	47.68%	4.183%
61	14.051	2032	2034	2040	rVB	249554	227470	7.47%	0.655%
62	14.186	2055	2057	2061	rVB2	56542	50825	1.67%	0.146%
63	14.410	2093	2095	2099	rVB2	62713	62005	2.04%	0.179%
64	14.492	2106	2109	2114	rBV3	162676	229426	7.54%	0.661%
65	14.798	2159	2161	2166	rBV2	54272	64472	2.12%	0.186%
66	14.874	2172	2174	2178	rVB	94459	86518	2.84%	0.249%
67	14.945	2183	2186	2195	rVB	603687	627379	20.61%	1.808%
68	15.062	2203	2206	2210	rBV	160805	248548	8.16%	0.716%
69	15.139	2216	2219	2221	rBV	206809	246998	8.11%	0.712%
70	15.168	2221	2224	2237	rVB2	695031	1053978	34.62%	3.037%
71	15.433	2265	2269	2274	rVB	117465	153739	5.05%	0.443%
72	15.492	2275	2279	2283	rBV	487291	634058	20.83%	1.827%
73	15.727	2315	2319	2324	rVB	236033	296145	9.73%	0.853%
74	15.962	2354	2359	2364	rBV	225152	321011	10.54%	0.925%
75	16.015	2365	2368	2377	rVB4	102691	188936	6.21%	0.544%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138416.D
Acq On : 01 Jul 2024 21:34
Operator : CG\JU
Sample : P2977-21RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OSTL-D3RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 34702082

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138416.D
Acq On : 01 Jul 2024 21:34
Operator : CG\JU
Sample : P2977-21RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OSTL-D3RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

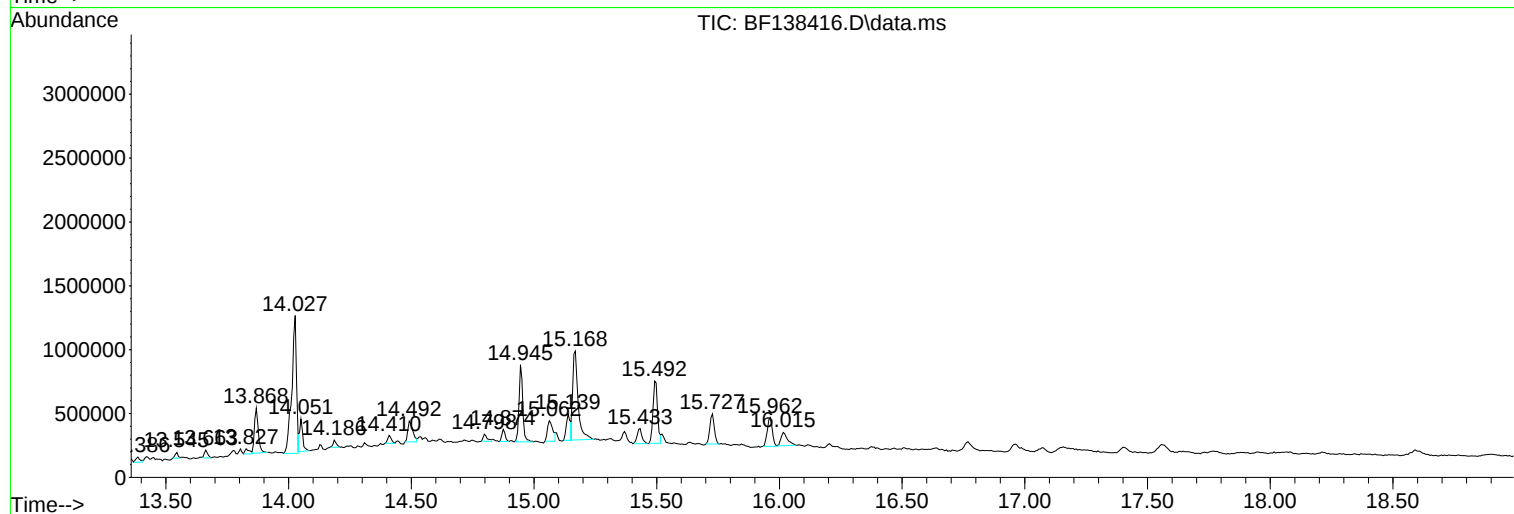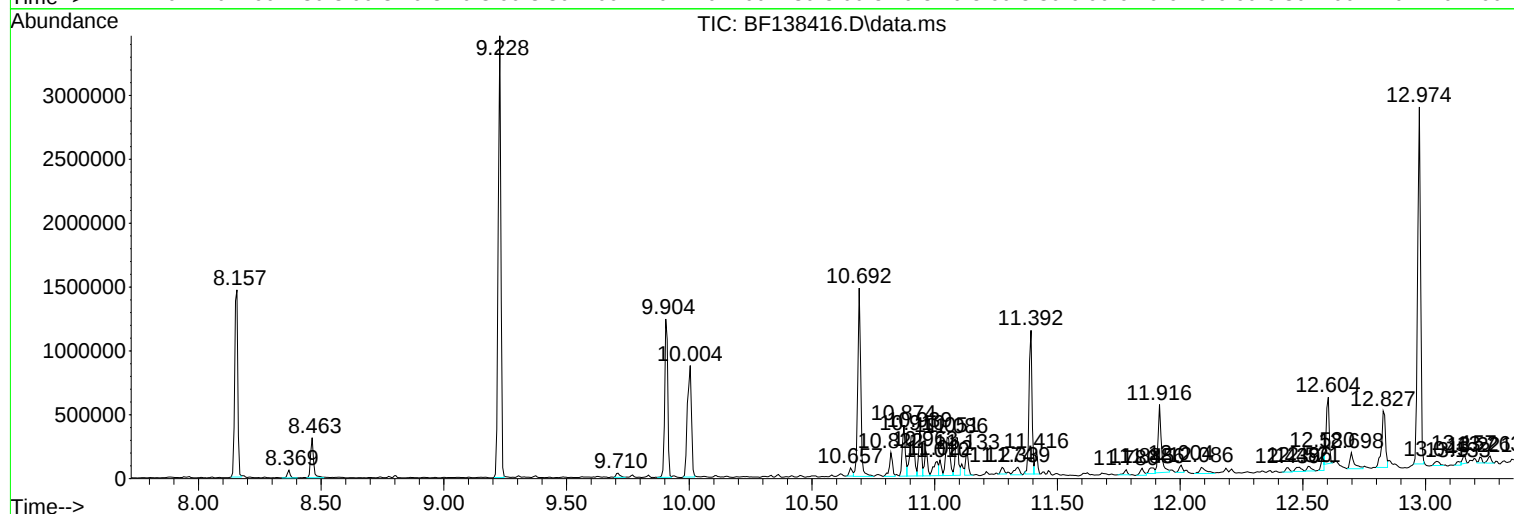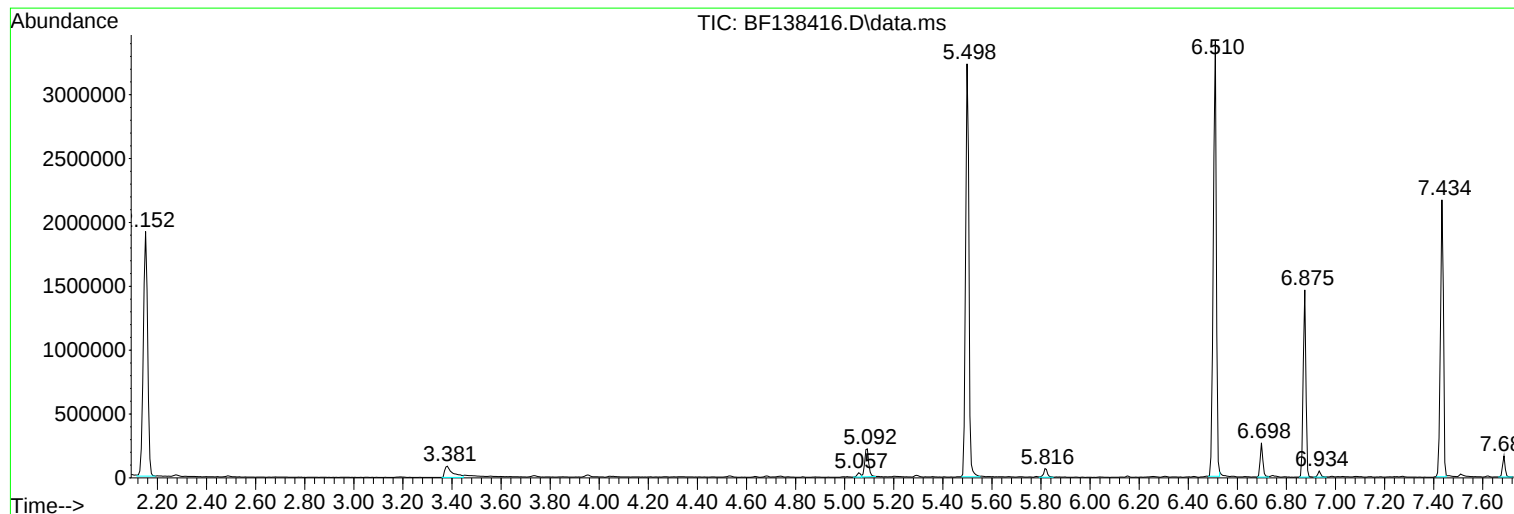

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138416.D
Acq On : 01 Jul 2024 21:34
Operator : CG\JU
Sample : P2977-21RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OSTL-D3RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138416.D
Acq On : 01 Jul 2024 21:34
Operator : CG\JU
Sample : P2977-21RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OSTL-D3RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------