


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138394.D
Acq On : 01 Jul 2024 10:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 29 02:44:30 2024

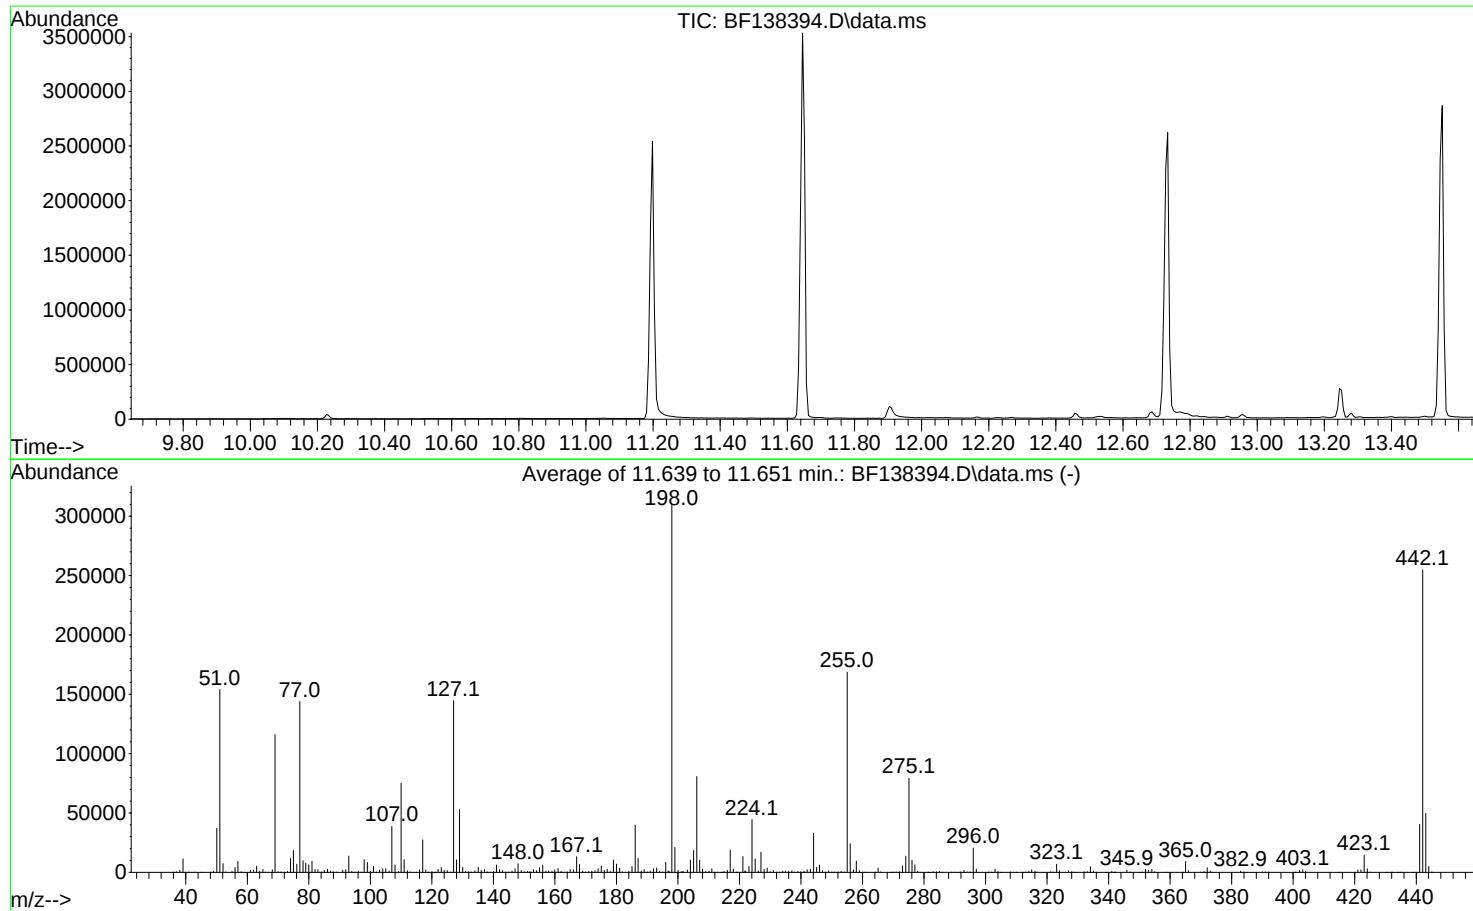




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	49.7	153949	PASS
68	69	0.00	2	1.9	2186	PASS
69	198	0.00	100	37.4	116001	PASS
70	69	0.00	2	0.5	621	PASS
127	198	10	80	46.7	144600	PASS
197	198	0.00	2	0.4	1156	PASS
198	198	100	100	100.0	309909	PASS
199	198	5	9	6.8	21024	PASS
275	198	10	60	25.6	79283	PASS
365	198	1	100	2.9	9079	PASS
441	198	0.01	100	13.1	40458	PASS
442	442	50	100	100.0	254763	PASS
443	442	15	24	19.5	49739	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138394.D
Acq On : 01 Jul 2024 10:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 01 12:11:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

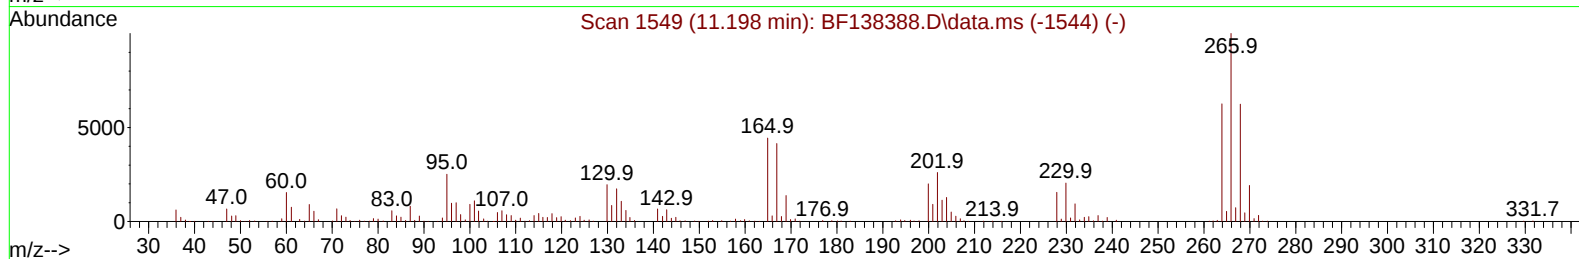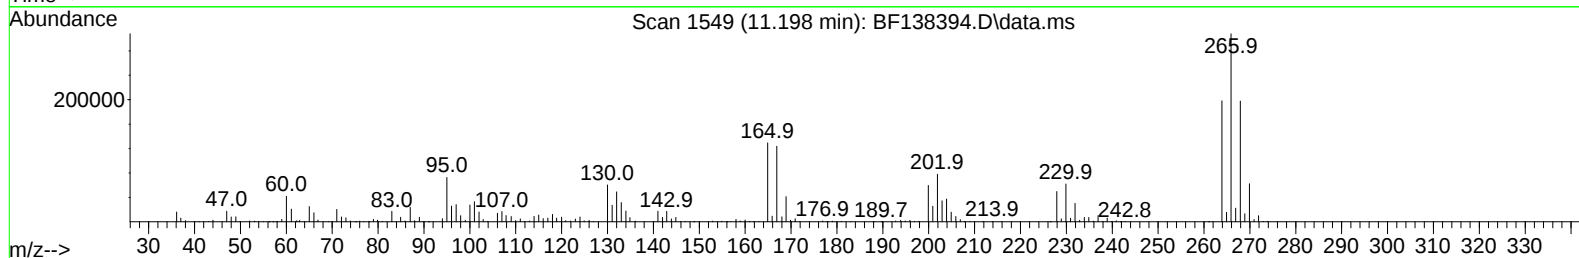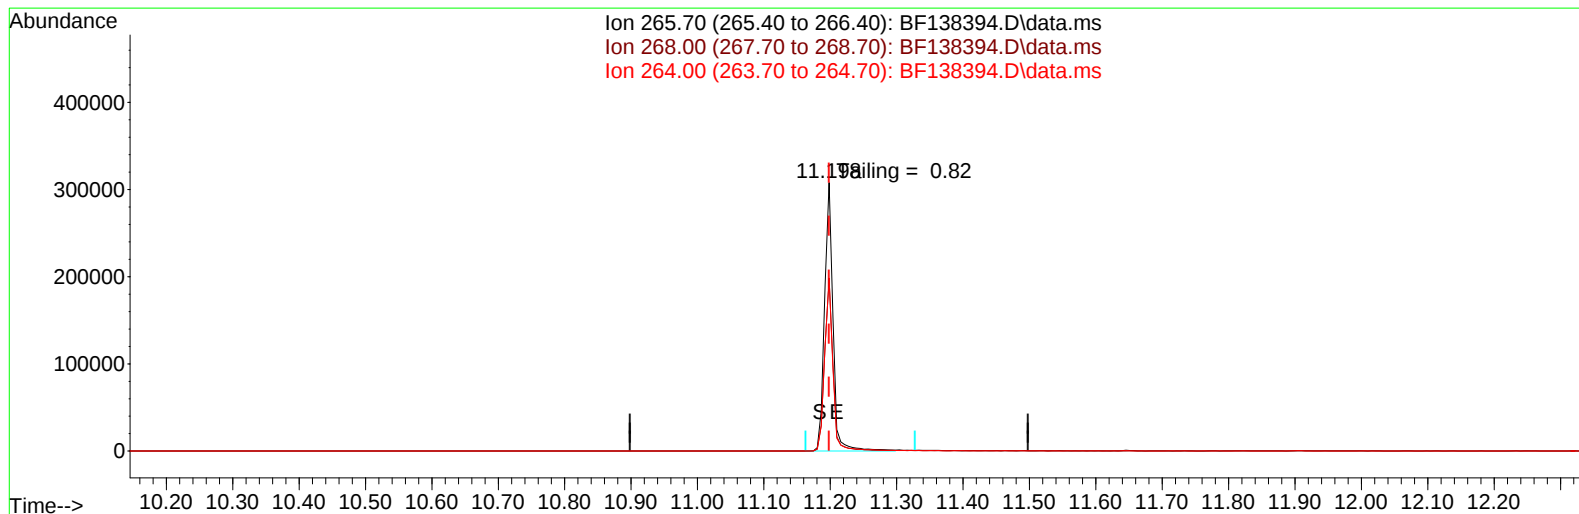

TIC: BF138394.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 738560.39 ng




response 275341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.21
264.00	62.50	64.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070124\
Data File : BF138394.D
Acq On : 01 Jul 2024 10:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 01 12:11:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

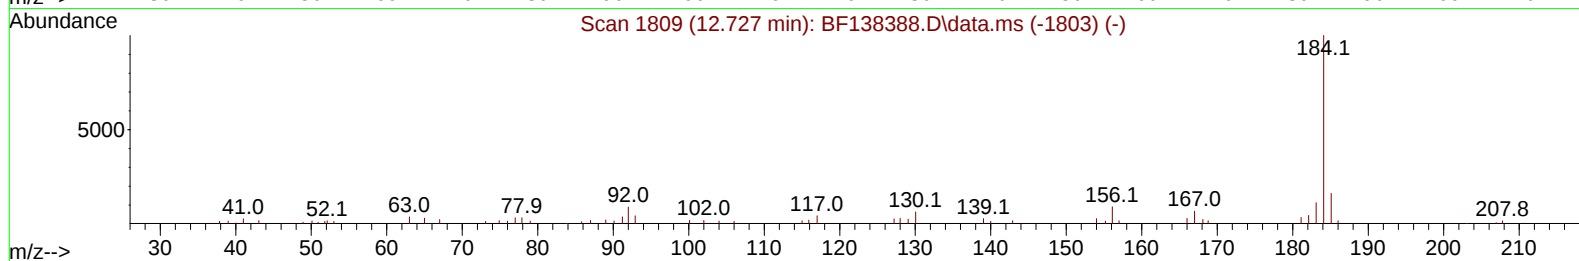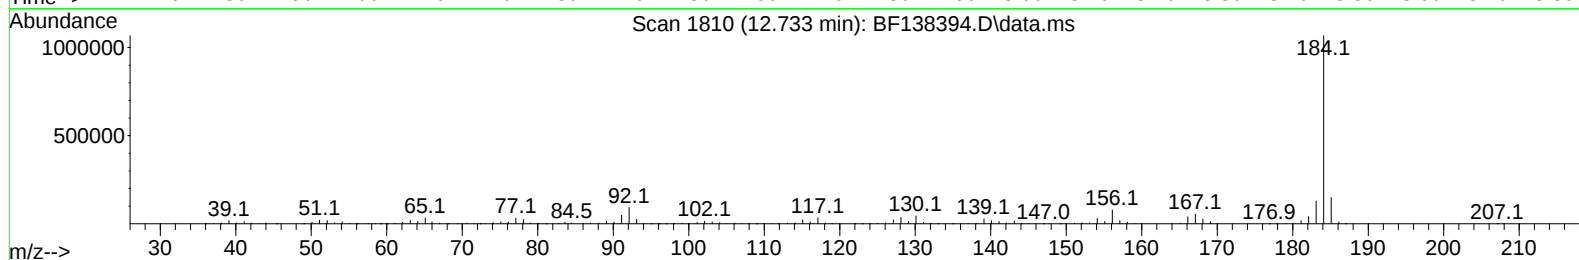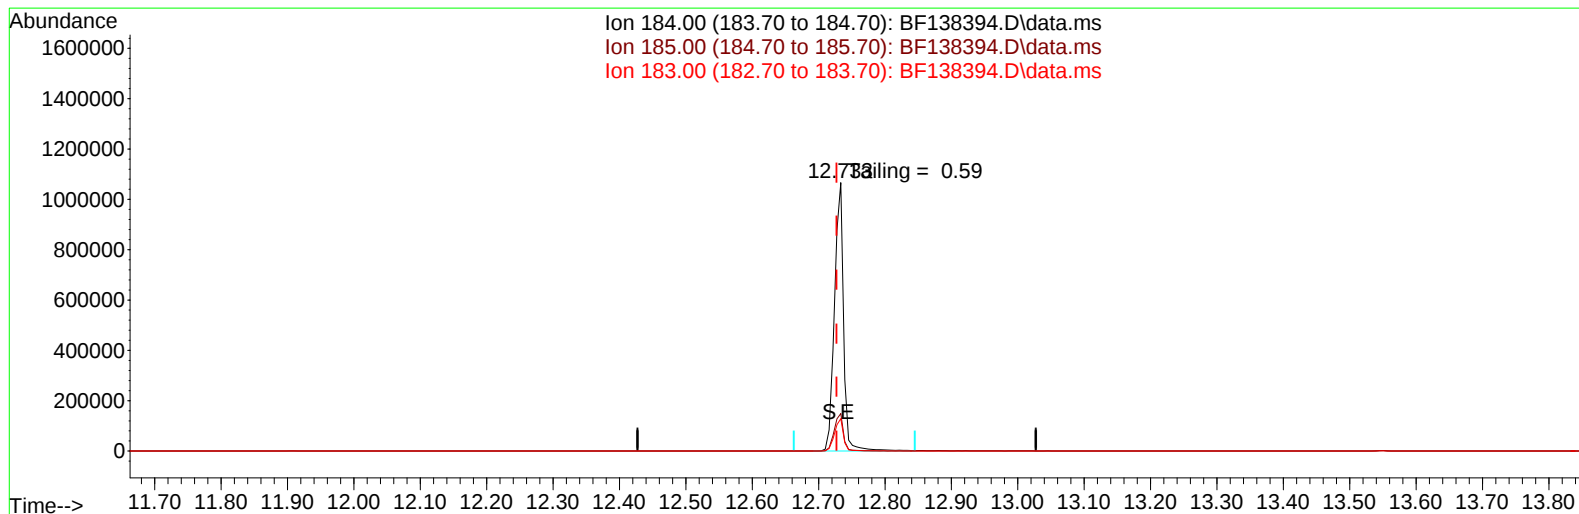

TIC: BF138394.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 36231.18 ng

response 1016333

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	13.98
183.00	11.30	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2024	BNA_F	<u>BF138394.D</u>
Compound Name	Response	Retention Time
DDT	477432	13.551
DDD	51835	13.251
DDE	1689	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53524	530956	10.08

Instrument :
BNA_F
ClientSampleId :
DFTPP