

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142950.D
Acq On : 01 Jul 2025 15:21
Operator : RC/JU
Sample : PB168657BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168657BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	488	494	505	rBV	90915	150599	7.47%	1.342%
2	5.498	556	562	584	rBV	1171652	1549363	76.83%	13.805%
3	6.504	727	733	738	rBV	1084657	1497948	74.28%	13.347%
4	6.869	791	795	804	rBV	273753	344499	17.08%	3.070%
5	7.433	885	891	896	rBV	737622	994258	49.30%	8.859%
6	8.157	1008	1014	1022	rBV	344177	446683	22.15%	3.980%
7	9.233	1190	1197	1202	rBV	1558105	2016733	100.00%	17.969%
8	9.910	1307	1312	1324	rBV	387238	499600	24.77%	4.451%
9	10.704	1442	1447	1467	rBV	832793	1064854	52.80%	9.488%
10	11.404	1560	1566	1573	rBV	369883	465783	23.10%	4.150%
11	12.992	1830	1836	1841	rBV	1184479	1545877	76.65%	13.774%
12	14.045	2010	2015	2023	rBV	230633	297423	14.75%	2.650%
13	15.539	2262	2269	2278	rBV	226779	349595	17.33%	3.115%




Sum of corrected areas: 11223215

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142950.D
Acq On : 01 Jul 2025 15:21
Operator : RC/JU
Sample : PB168657BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168657BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

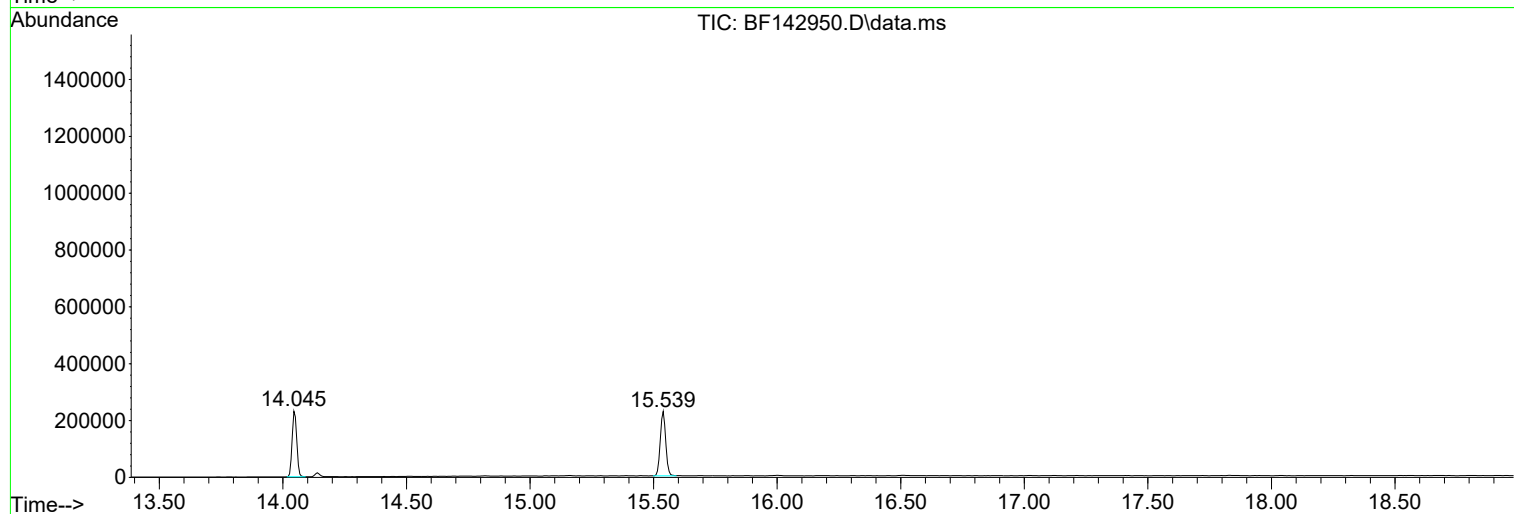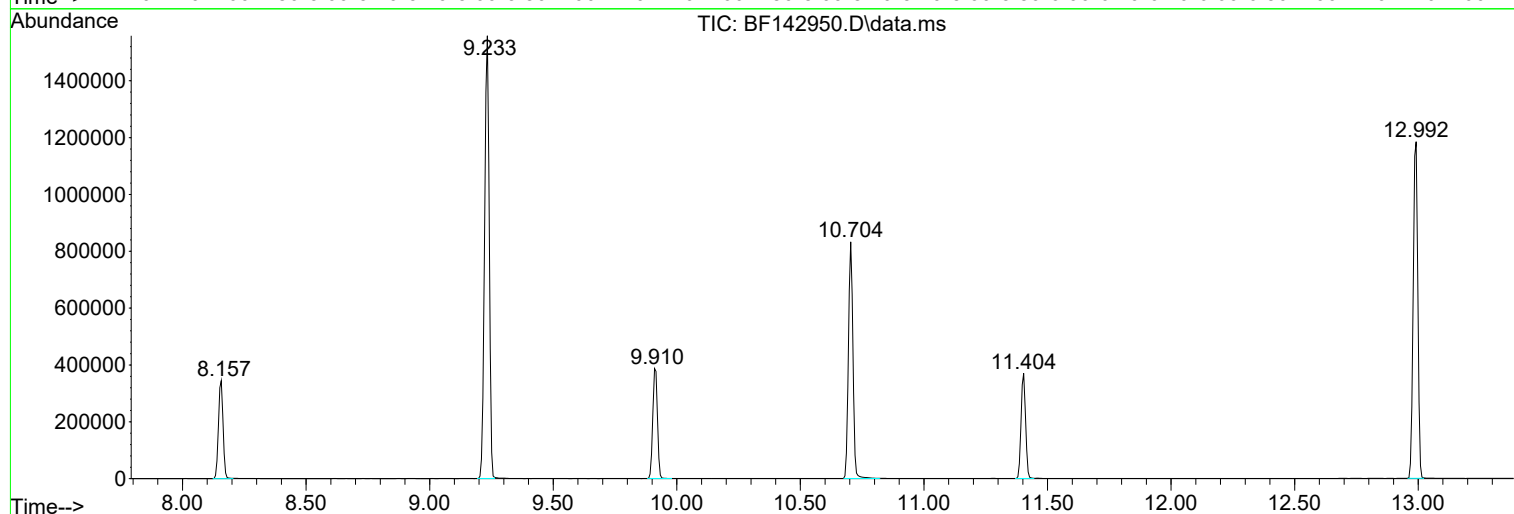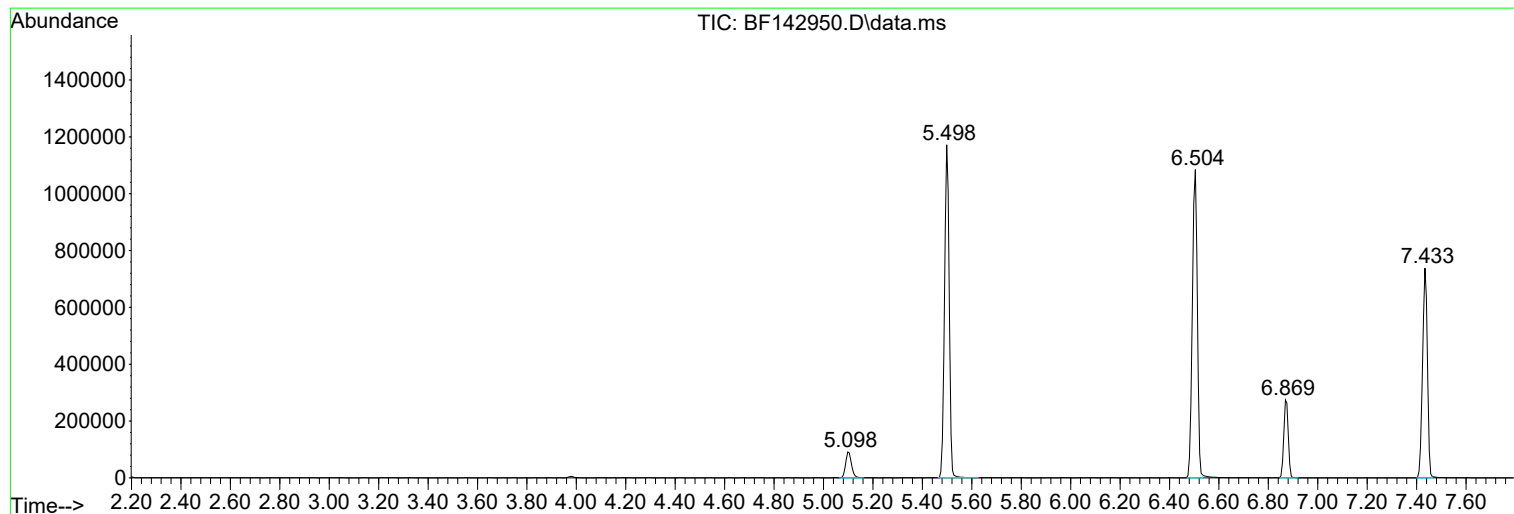

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142950.D
Acq On : 01 Jul 2025 15:21
Operator : RC/JU
Sample : PB168657BL
Misc :
ALS Vial : 11 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB168657BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.098	8.74 ng	150599	1,4-Dichlorobenzene-d4	6.869	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12

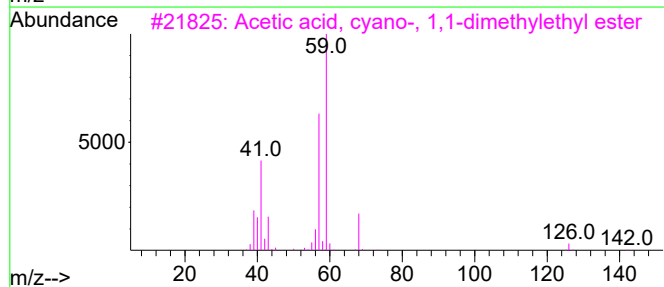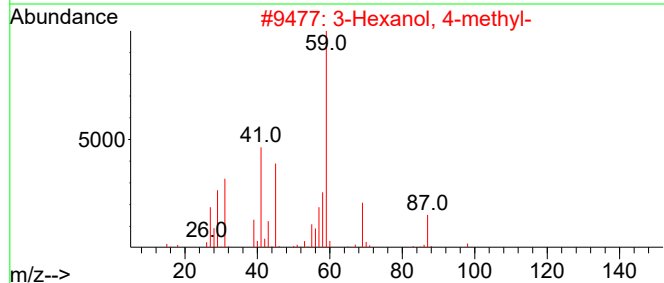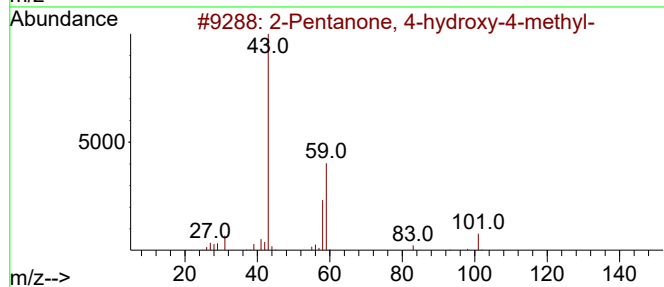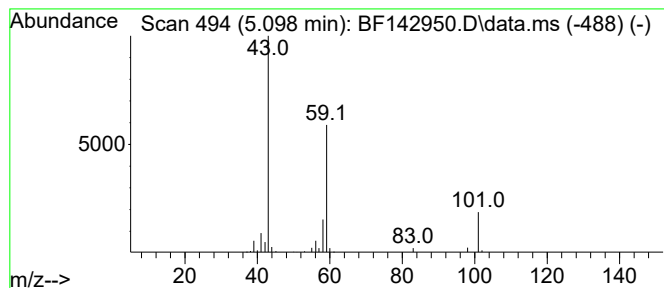

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142950.D
Acq On : 01 Jul 2025 15:21
Operator : RC/JU
Sample : PB168657BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168657BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.098	8.7	ng	150599	1	6.869	344499	20.0