

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
 Data File : BF142961.D
 Acq On : 01 Jul 2025 21:04
 Operator : RC/JU
 Sample : Q2458-02 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	483	490	497	rBB2	7129	10707	3.03%	0.425%
2	5.493	556	561	573	rBV	79242	114240	32.35%	4.533%
3	6.504	728	733	749	rBV	74901	106344	30.11%	4.220%
4	6.875	791	796	804	rVB	173422	211768	59.96%	8.403%
5	7.434	886	891	901	rBV	49334	63968	18.11%	2.538%
6	8.157	1009	1014	1037	rBV	207397	253478	71.77%	10.058%
7	9.233	1192	1197	1211	rVB	116049	144995	41.06%	5.754%
8	9.916	1308	1313	1318	rBV	247460	299300	84.75%	11.877%
9	10.627	1430	1434	1439	rVB	12029	14339	4.06%	0.569%
10	10.704	1442	1447	1453	rBV	76199	92699	26.25%	3.678%
11	11.404	1561	1566	1573	rBV	287833	353162	100.00%	14.014%
12	11.927	1649	1655	1664	rBV4	7407	15062	4.26%	0.598%
13	12.022	1667	1671	1677	rVB4	1844	3829	1.08%	0.152%
14	12.621	1768	1773	1777	rBV	14672	17842	5.05%	0.708%
15	12.716	1785	1789	1794	rBV3	2351	4026	1.14%	0.160%
16	12.851	1806	1812	1817	rBV	18097	26763	7.58%	1.062%
17	12.986	1830	1835	1840	rBV	168885	208344	58.99%	8.267%
18	13.168	1862	1866	1871	rBV3	4399	7870	2.23%	0.312%
19	13.280	1882	1885	1888	rBV4	4111	5207	1.47%	0.207%
20	14.051	2011	2016	2027	rBV	237450	342061	96.86%	13.573%
21	15.545	2265	2270	2278	rVB	140727	224071	63.45%	8.891%




Sum of corrected areas: 2520075

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142961.D
Acq On : 01 Jul 2025 21:04
Operator : RC/JU
Sample : Q2458-02 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

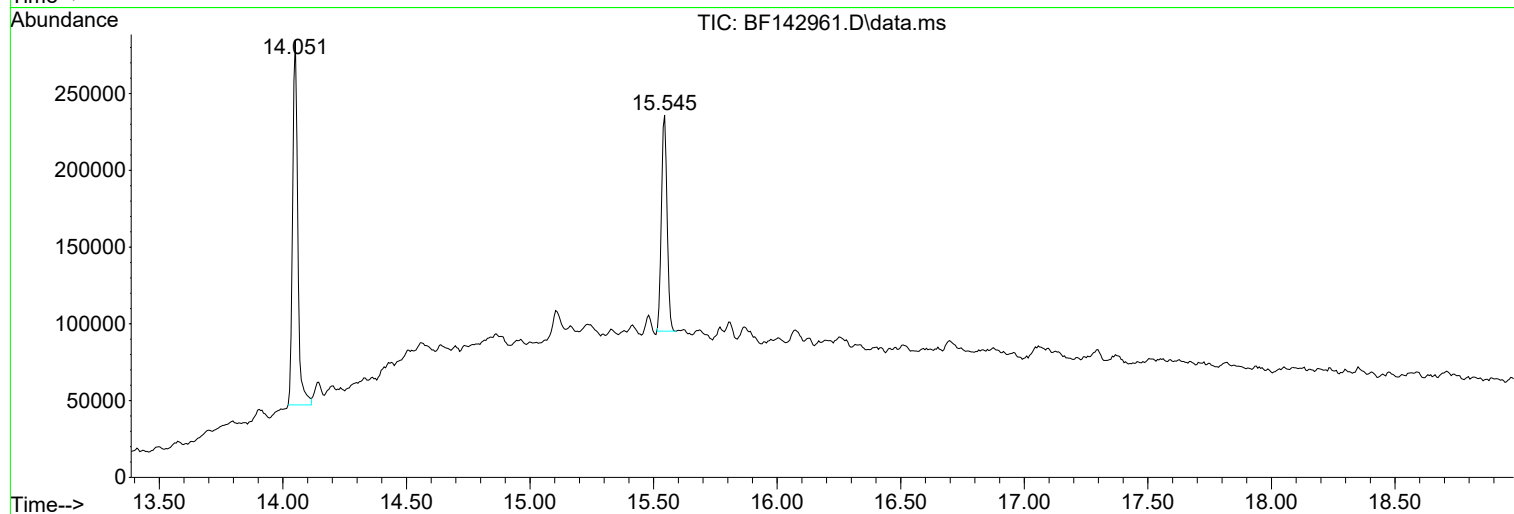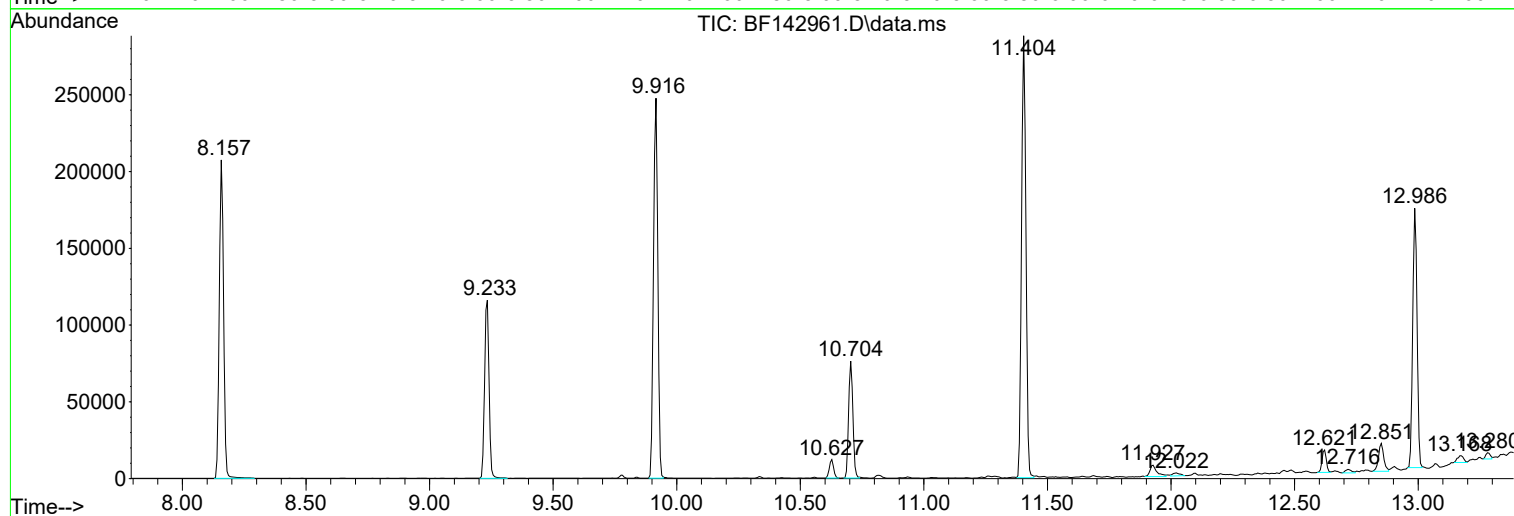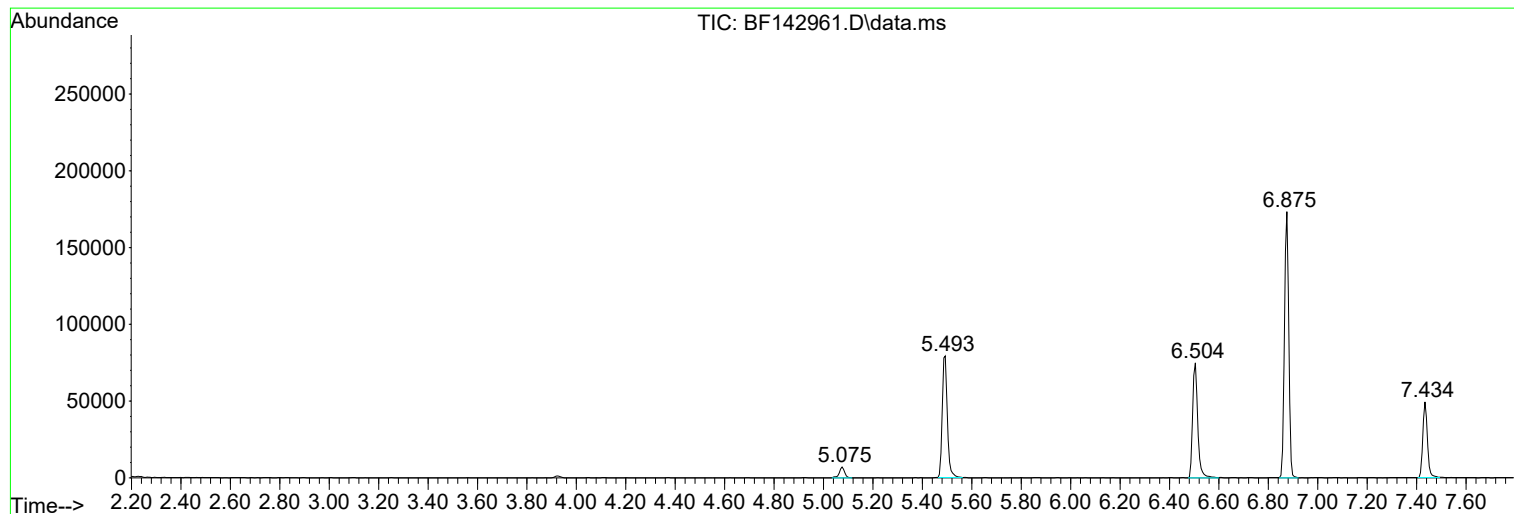

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142961.D
Acq On : 01 Jul 2025 21:04
Operator : RC/JU
Sample : Q2458-02 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142961.D
Acq On : 01 Jul 2025 21:04
Operator : RC/JU
Sample : Q2458-02 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------