
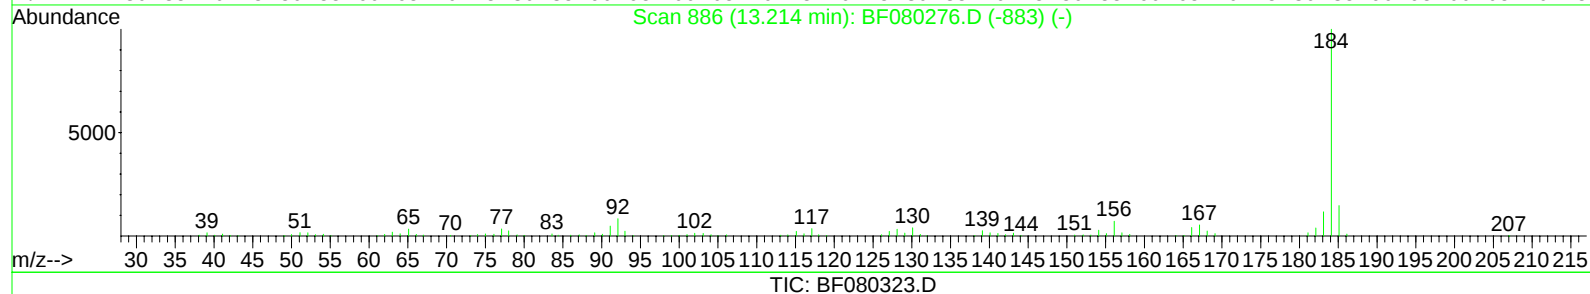
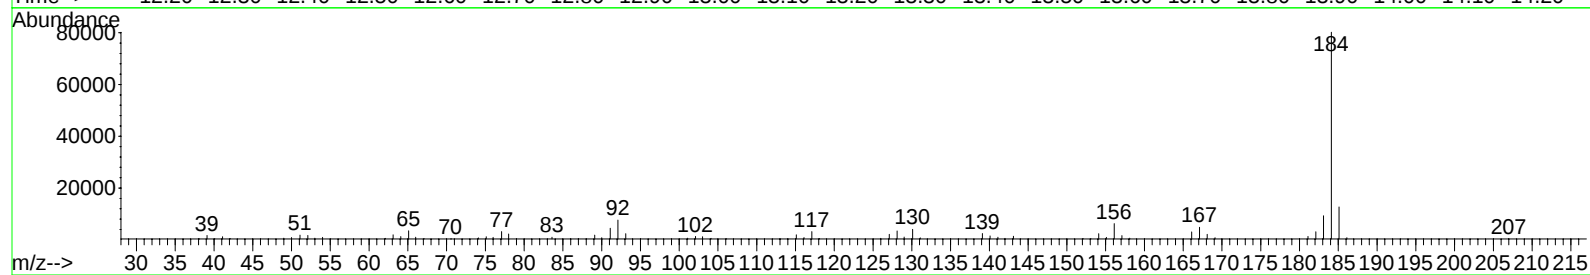


Data Path : Z:\HPCHEM1\BNA F\Data\BF070215\
Data File : BF080323.D
Acq On : 3 Jul 2015 3:43
Operator : TP/IZ
Sample : DF TPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 08:48:52 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 13:33:16 2015
Response via : Initial Calibration

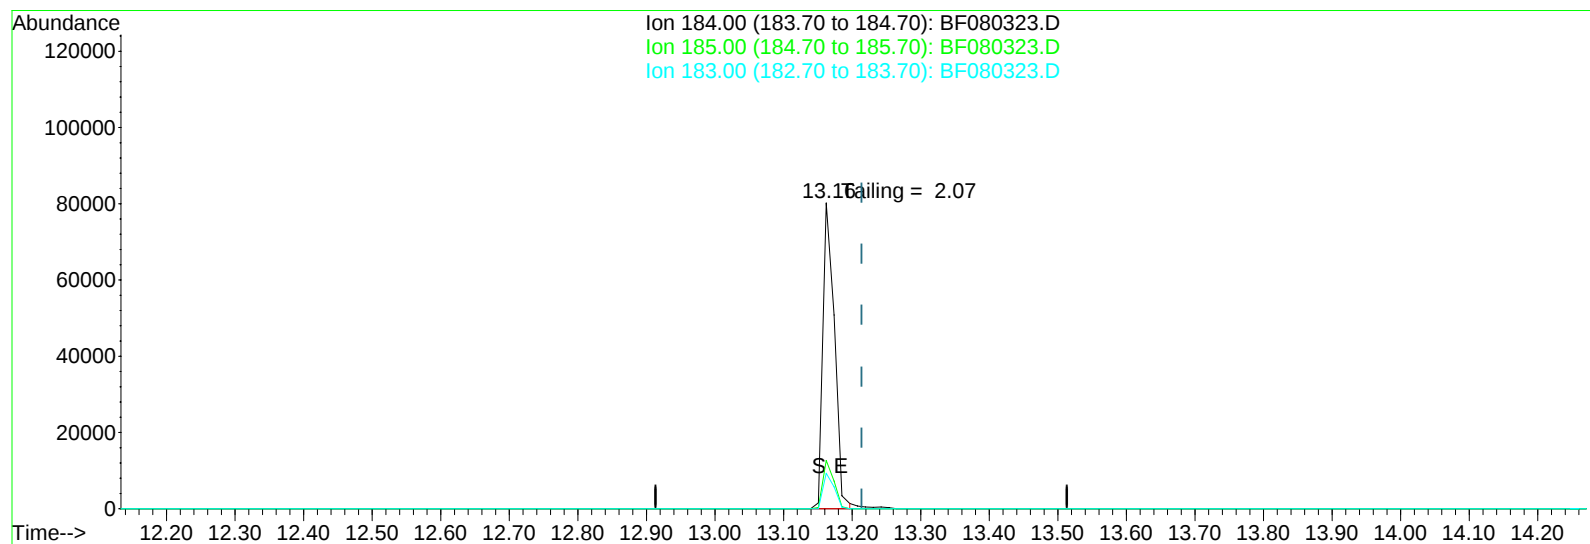

(76) Benzidine

13.162min (-0.051) 0.00ng

response 95815




Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.82
183.00	11.70	11.61
0.00	0.00	0.00

```

Data Path   : Z:\HPCHEM1\BNA F\Data\BF070215\
Data File   : BF080323.D
Acq On      : 3 Jul 2015    3:43
Operator    : TP/IZ
Sample      : DFTPP
Misc        :
ALS Vial    : 1      Sample Multiplier: 1

```

Quant Time: Jul 03 08:48:52 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 13:33:16 2015
Response via : Initial Calibration

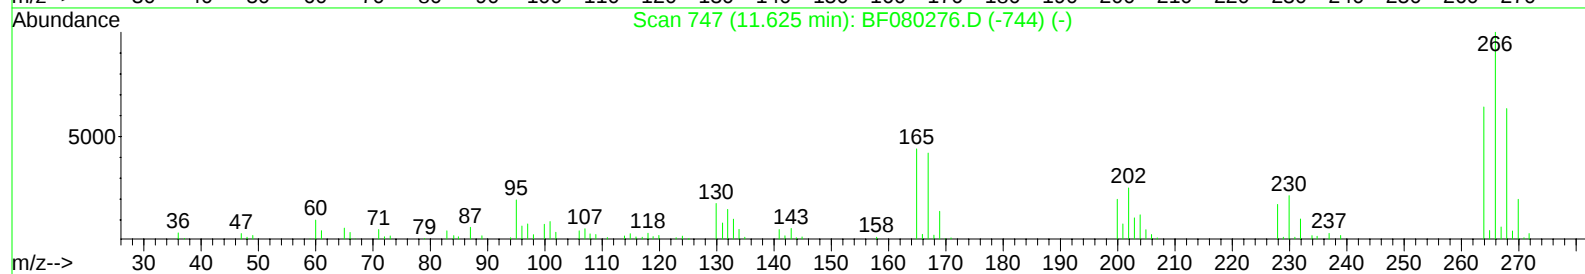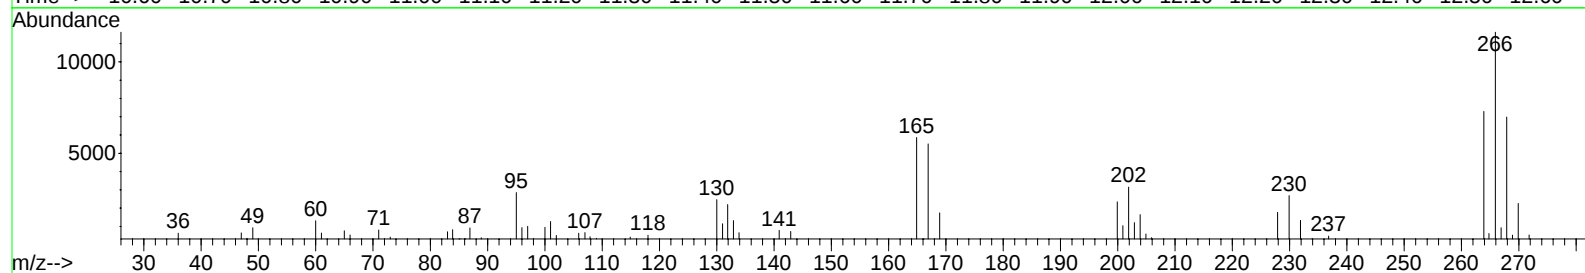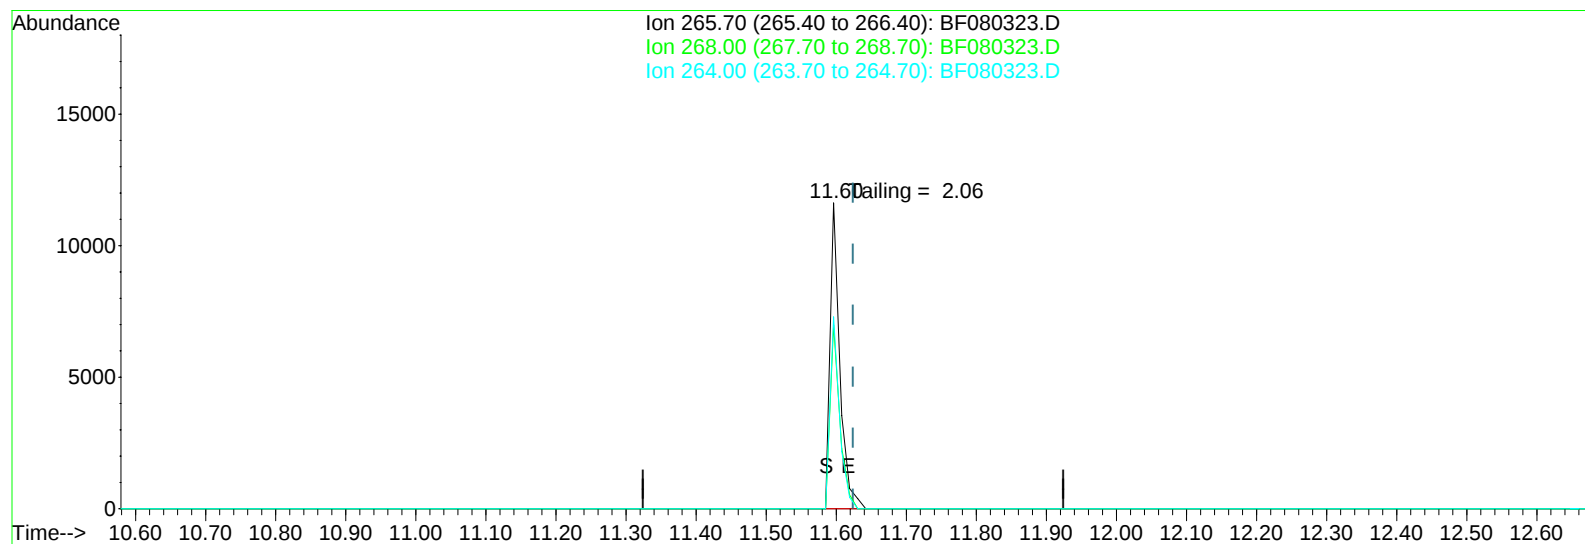

TIC: BF080323.D

(69) Pentachlorophenol (C)

11.596min (-0.028) 0.00ng m

response 11185

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	60.12
264.00	64.10	62.76
0.00	0.00	0.00