


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070215\
 Data File : BF080308.D
 Acq On : 2 Jul 2015 14:23
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 06 11:42:01 2015

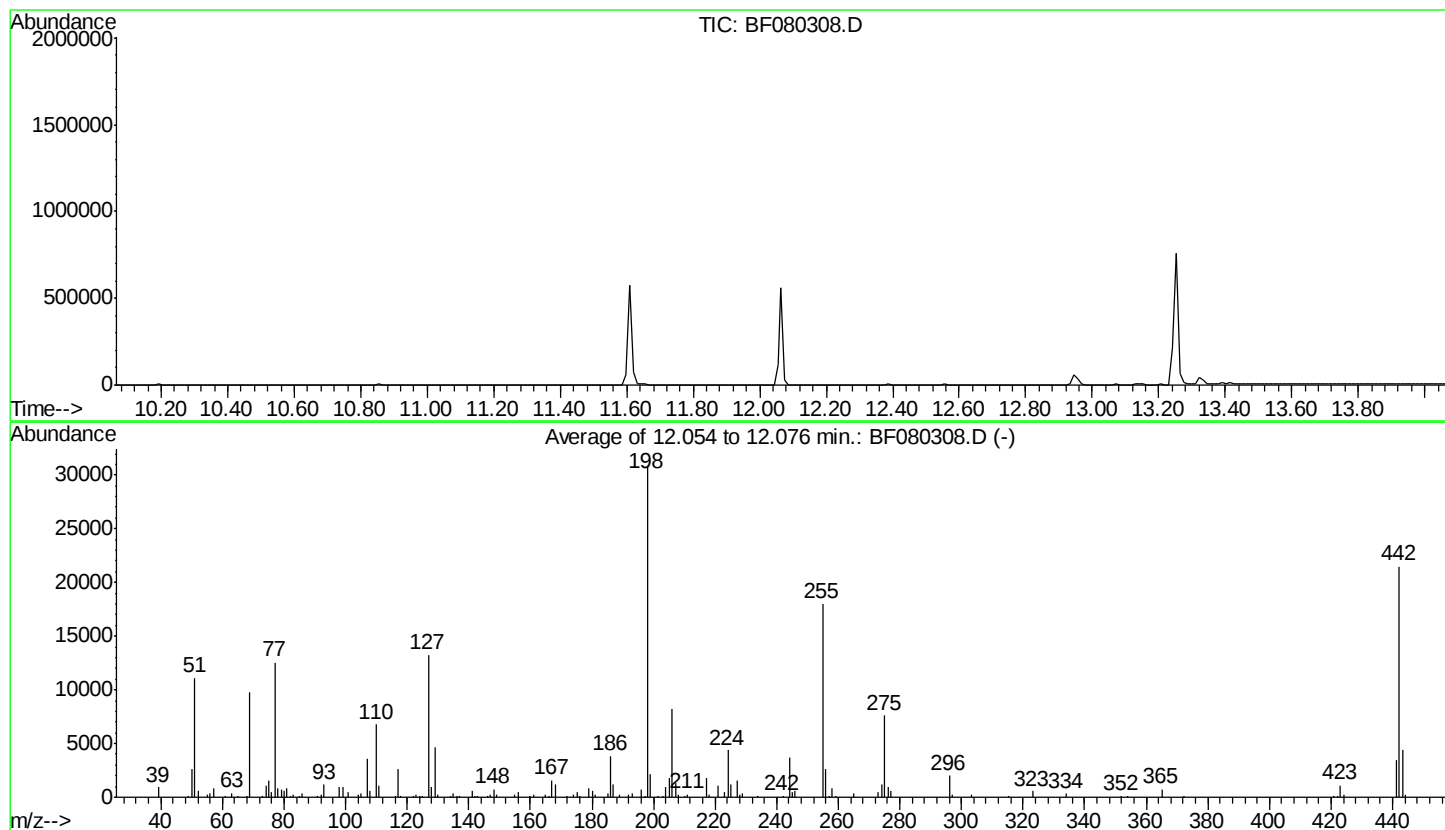

AutoFind: Scans 872, 873, 874; Background Corrected with Scan 869

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	11103	PASS
68	69	0.00	2	1.4	137	PASS
69	198	0.00	100	31.8	9817	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.9	13254	PASS
197	198	0.00	2	0.4	114	PASS
198	198	100	100	100.0	30873	PASS
199	198	5	9	6.9	2132	PASS
275	198	10	60	24.6	7591	PASS
365	198	1	100	2.4	730	PASS
441	442	0.01	24	16.4	3513	PASS
442	198	50	100	69.6	21476	PASS
443	442	15	24	20.3	4354	PASS