


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070215\
 Data File : BF080323.D
 Acq On : 3 Jul 2015 3:43
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 06 11:42:01 2015

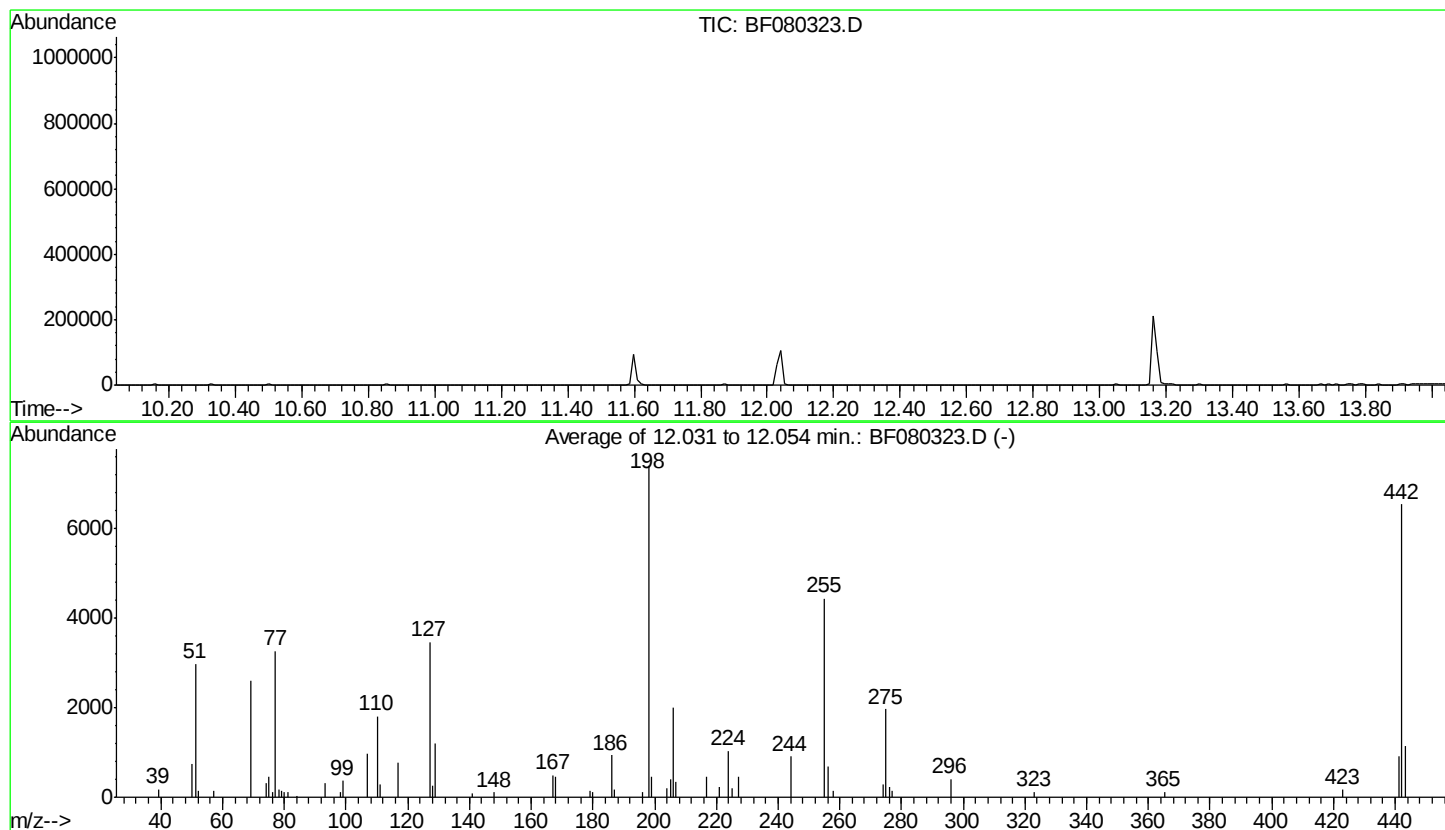

AutoFind: Scans 870, 871, 872; Background Corrected with Scan 867

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	2980	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.1	2591	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	3454	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7392	PASS
199	198	5	9	6.3	466	PASS
275	198	10	60	26.5	1961	PASS
365	198	1	100	1.6	116	PASS
441	442	0.01	24	13.9	908	PASS
442	198	50	100	88.2	6523	PASS
443	442	15	24	17.7	1156	PASS