

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070216\
 Data File : BF088613.D
 Acq On : 2 Jul 2016 13:16
 Operator : UM/SJ
 Sample : H3871-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 K8-B2(0-11)C

Quant Time: Jul 03 03:01:55 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 30 18:01:55 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	102066	20.00	ng	-0.02
21) Naphthalene-d8	8.08	136	435532	20.00	ng	-0.02
38) Acenaphthene-d10	9.83	164	190347	20.00	ng	-0.02
63) Phenanthrene-d10	11.30	188	306262	20.00	ng	-0.02
75) Chrysene-d12	13.93	240	206312	20.00	ng	-0.02
86) Perylene-d12	15.33	264	213612	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	737009	108.22	ng	-0.01
7) Phenol-d6	6.43	99	987477	112.22	ng	-0.01
23) Nitrobenzene-d5	7.36	82	642787	77.34	ng	-0.02
41) 2,4,6-Tribromophenol	10.62	330	180995	102.40	ng	-0.02
44) 2-Fluorobiphenyl	9.15	172	829024	68.80	ng	-0.02
78) Terphenyl-d14	12.89	244	585940	63.26	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.36	70	86829	14.69	ng	# 70
49) Dimethylphthalate	9.55	163	132701	9.79	ng	98
56) 2,4-Dinitrotoluene	9.83	165	24236	6.17	ng	# 38
66) 4-Bromophenyl-phenylether	10.62	248	12237	3.96	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070216\
Data File : BF088613.D
Acq On : 2 Jul 2016 13:16
Operator : UM/SJ
Sample : H3871-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
K8-B2(0-11)C

Quant Time: Jul 03 03:01:55 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 30 18:01:55 2016
Response via : Initial Calibration

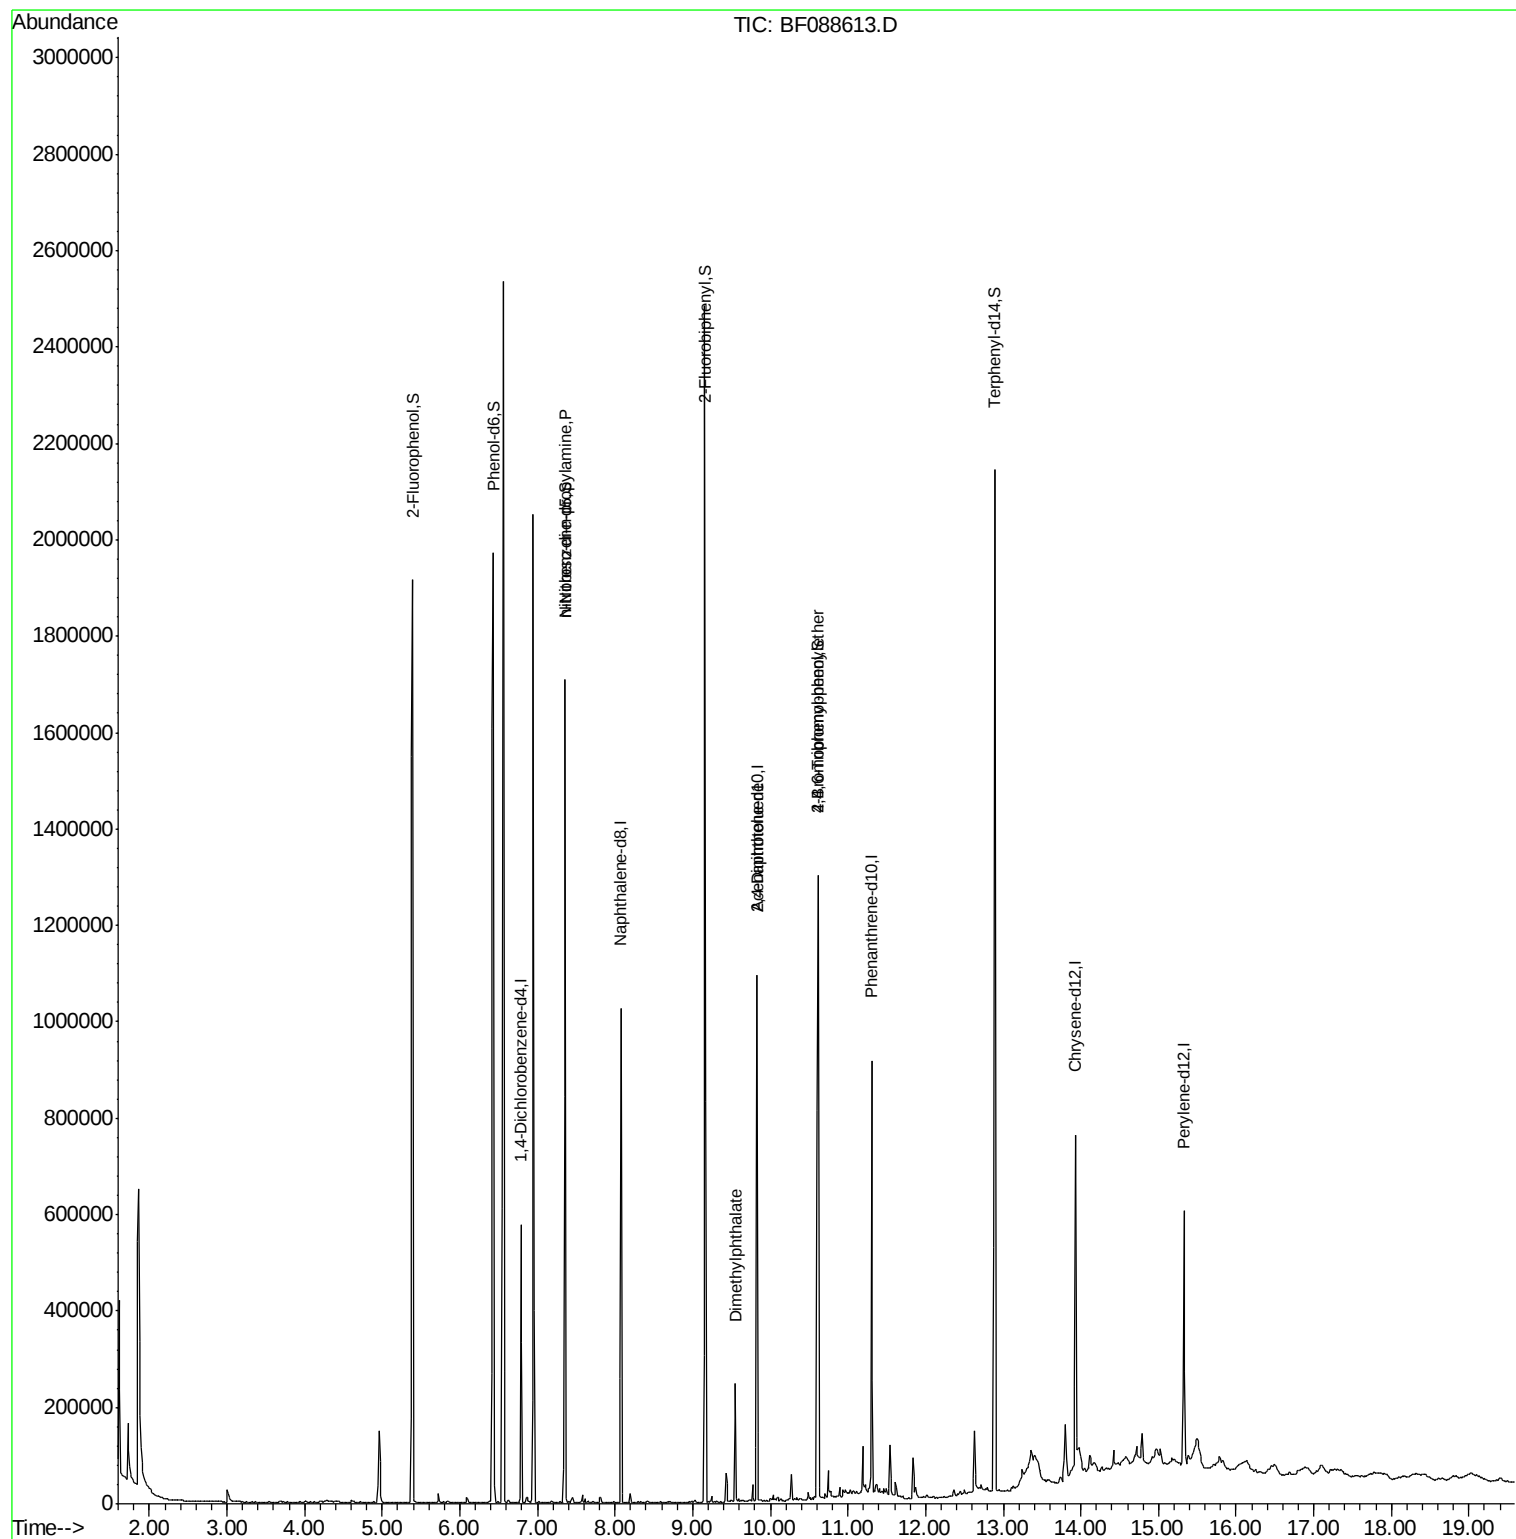

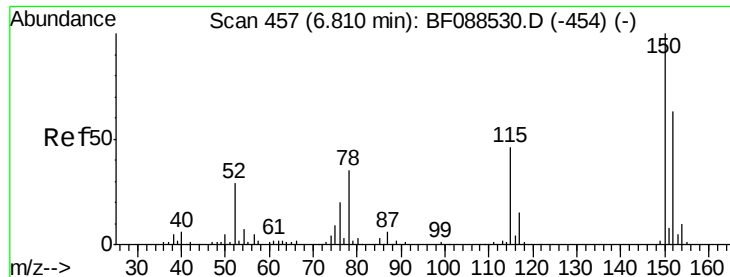

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.79 min Scan# 455

Delta R.T. -0.02 min

Lab File: BF088613.D

Acq: 2 Jul 2016 13:16

Instrument :

BNA_F

ClientSampleId :

K8-B2(0-11)C


Tgt Ion:152 Resp: 102066

Ion Ratio Lower Upper

152 100

150 163.3 123.8 185.6




115 73.7 39.6 59.4#

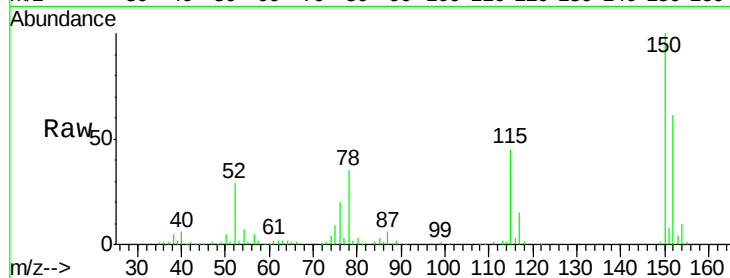

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

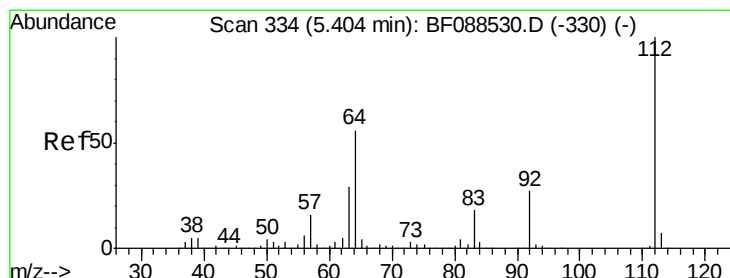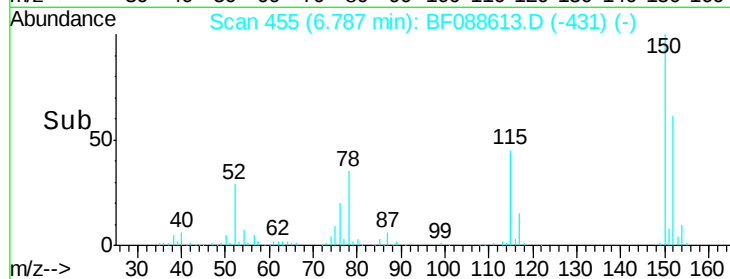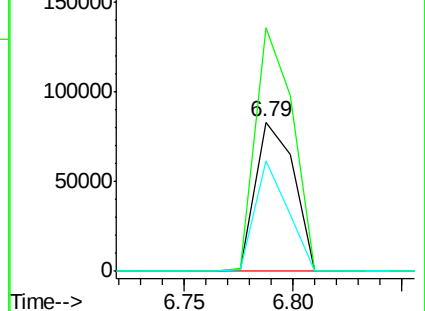

#5

2-Fluorophenol

Concen: 108.22 ng

RT: 5.39 min Scan# 333

Delta R.T. -0.01 min

Lab File: BF088613.D

Acq: 2 Jul 2016 13:16


Tgt Ion:112 Resp: 737009

Ion Ratio Lower Upper

112 100

64 50.8 42.2 63.2



63 25.9 21.8 32.8

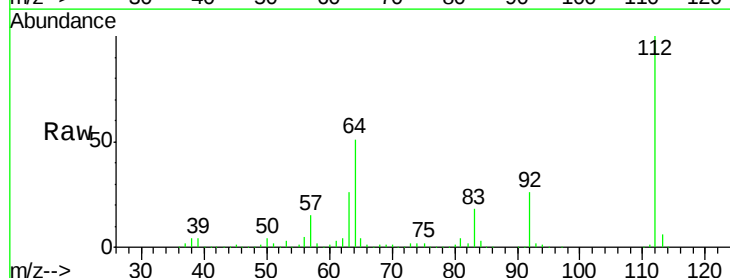


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

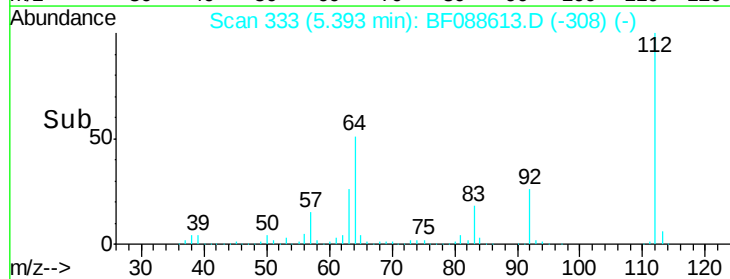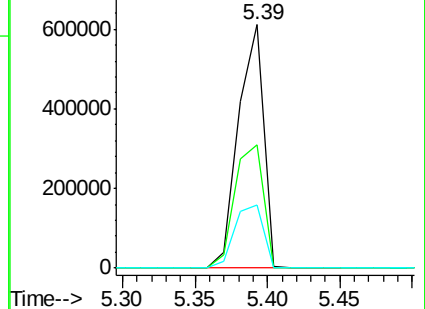

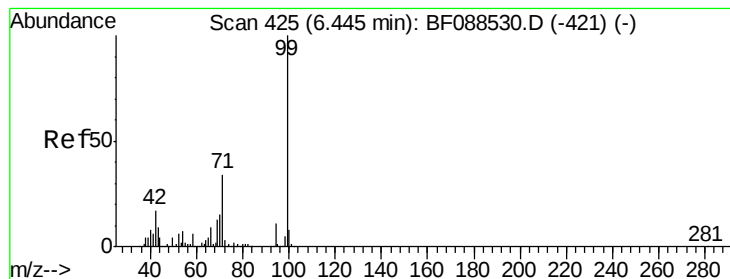

#7

Phenol-d6

Concen: 112.22 ng

RT: 6.43 min Scan# 424

Delta R.T. -0.01 min

Lab File: BF088613.D

Acq: 2 Jul 2016 13:16

Instrument :

BNA_F

ClientSampleId :

K8-B2(0-11)C





Tgt Ion: 99 Resp: 987477

Ion Ratio Lower Upper

99 100

42 13.8 12.2 18.2

71 31.6 23.4 35.0

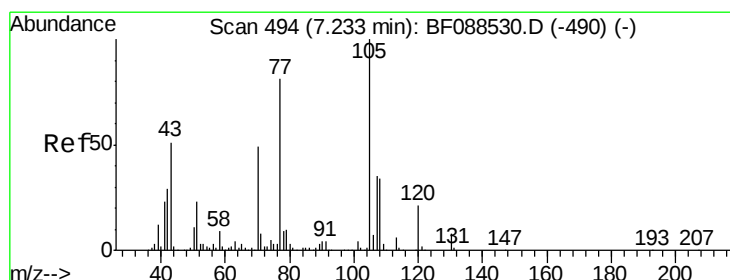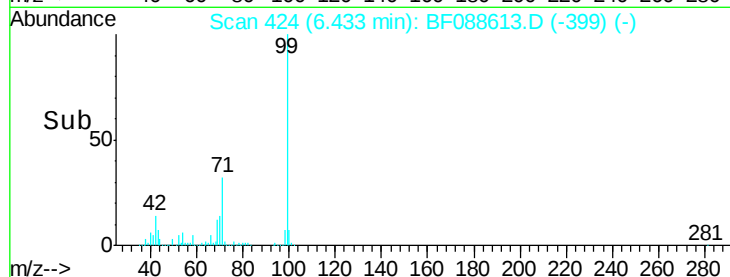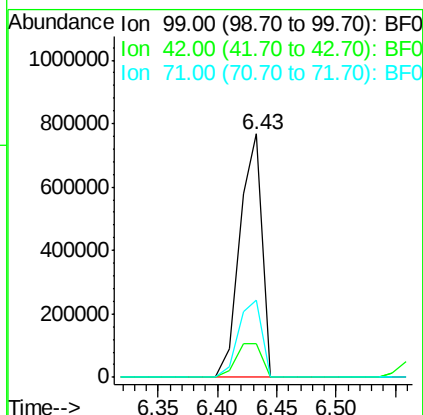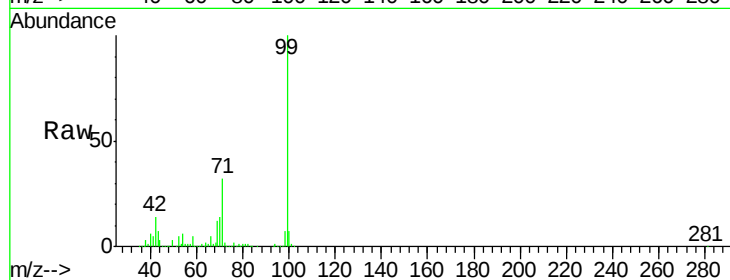

#19

n-Nitroso-di-n-propylamine

Concen: 14.69 ng

RT: 7.36 min Scan# 505

Delta R.T. 0.13 min

Lab File: BF088613.D

Acq: 2 Jul 2016 13:16

Tgt Ion: 70 Resp: 86829




Ion Ratio Lower Upper


70 100

42 40.7 49.6 74.4#

101 0.0 7.1 10.7#

130 2.0 15.4 23.2#

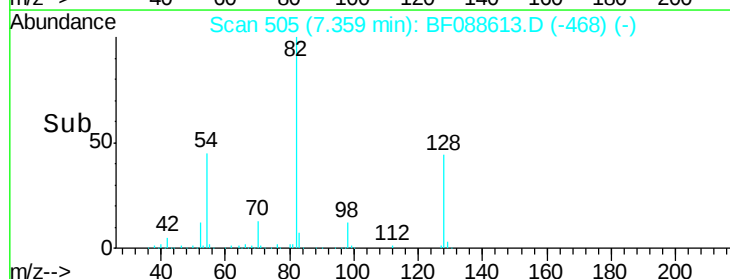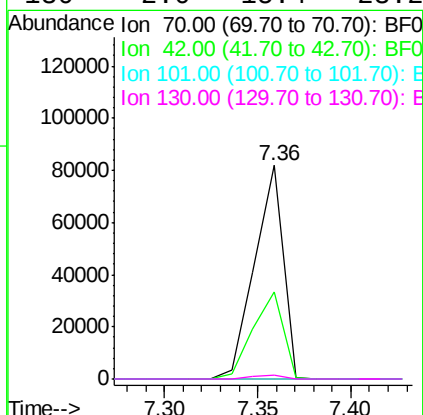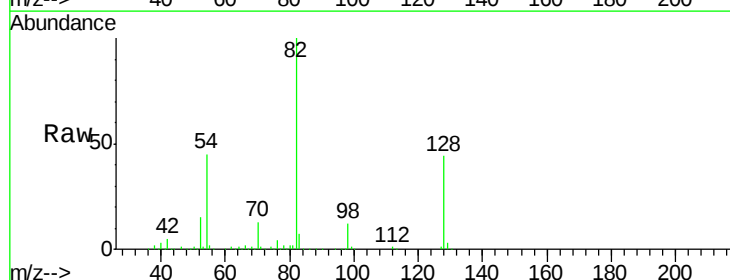







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.08 min Scan# 568
Delta R.T. -0.02 min
Lab File: BF088613.D
Acq: 2 Jul 2016 13:16

Instrument :
BNA_F
ClientSampleId :
K8-B2(0-11)C

Tgt Ion:	136	Resp:	435532
Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.1	13.7
54	7.2	6.6	10.0
68	6.3	5.1	7.7

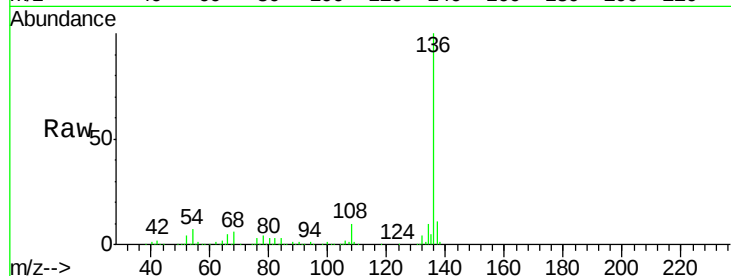


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

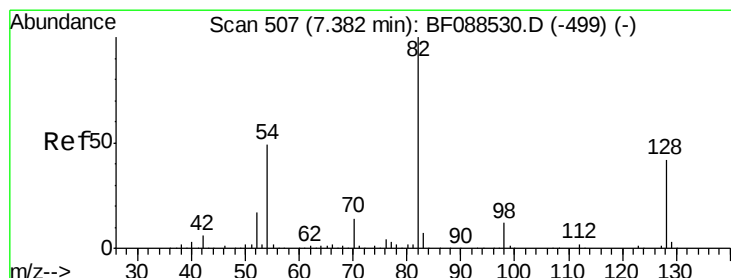
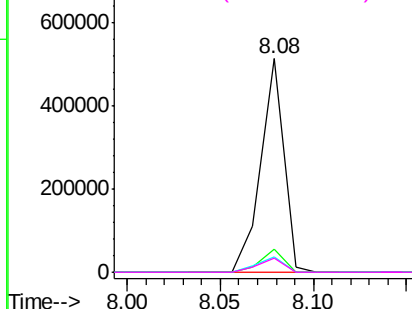



#23
Nitrobenzene-d5
Concen: 77.34 ng
RT: 7.36 min Scan# 505
Delta R.T. -0.02 min
Lab File: BF088613.D
Acq: 2 Jul 2016 13:16

Tgt Ion:	82	Resp:	642787
Ion	Ratio	Lower	Upper
82	100		
128	44.2	35.9	53.9
54	45.3	40.9	61.3

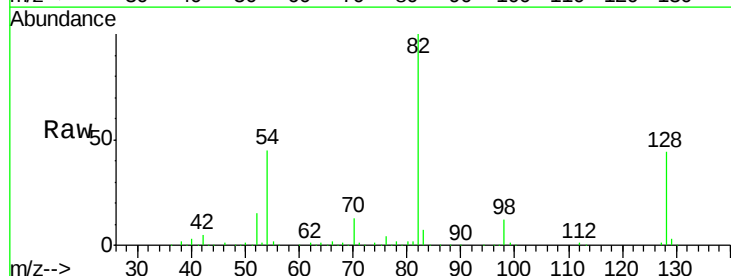

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0




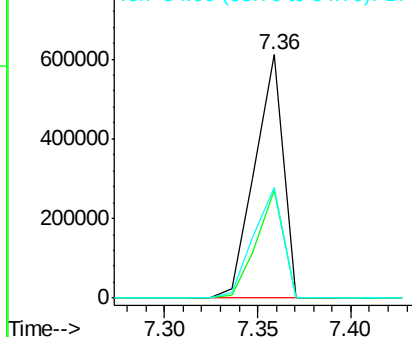




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.83 min Scan# 721
 Delta R.T. -0.02 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16




Instrument :
 BNA_F
 ClientSampleId :
 K8-B2(0-11)C


Tgt Ion:164 Resp: 190347
 Ion Ratio Lower Upper
 164 100
 162 103.7 85.4 128.2
 160 46.7 39.5 59.3

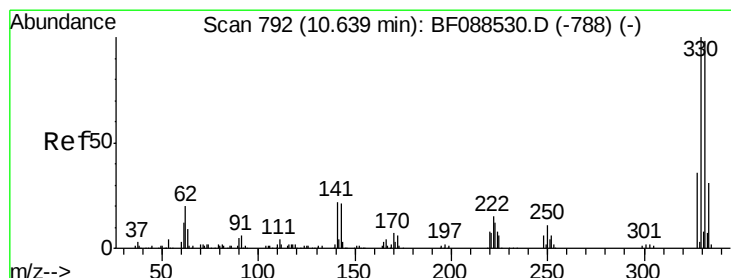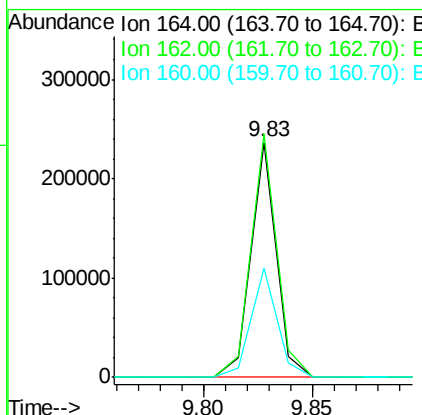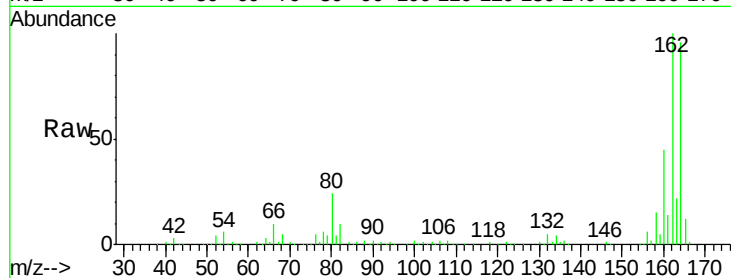

#41
 2,4,6-Tribromophenol
 Concen: 102.40 ng
 RT: 10.62 min Scan# 790
 Delta R.T. -0.02 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16

Tgt Ion:330 Resp: 180995
 Ion Ratio Lower Upper
 330 100
 332 94.5 0.0 0.0#
 141 37.3 0.0 0.0#

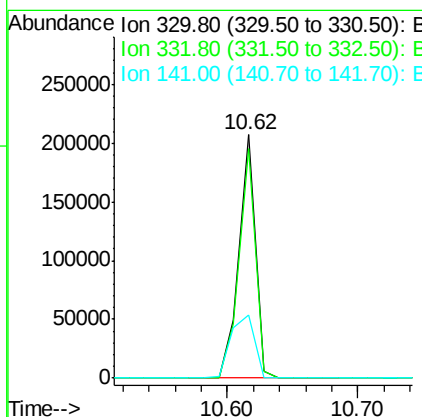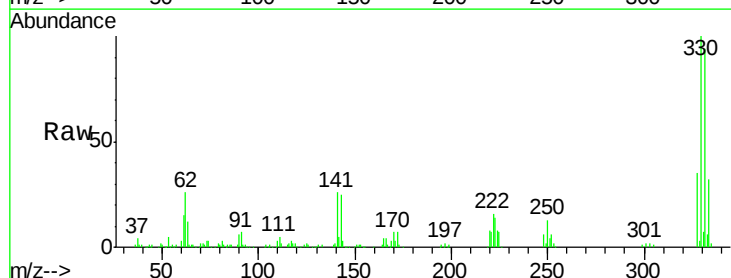







#44
 2-Fluorobiphenyl
 Concen: 68.80 ng
 RT: 9.15 min Scan# 662
 Delta R.T. -0.02 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16

Instrument :
 BNA_F
 ClientSampleId :
 K8-B2(0-11)C

Tgt Ion:172 Resp: 829024
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.6 43.0
 170 23.9 19.2 28.8

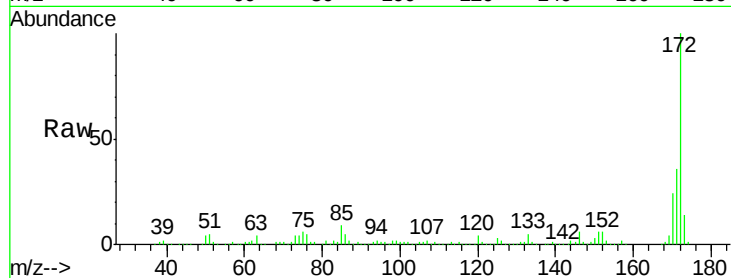


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

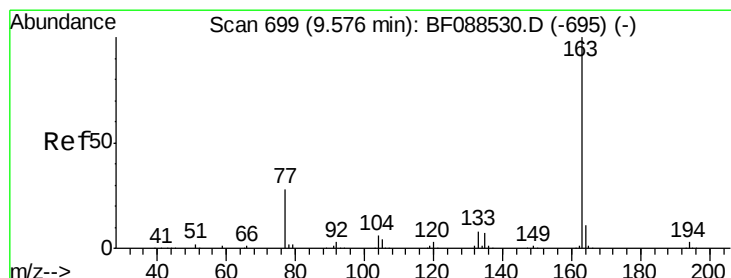
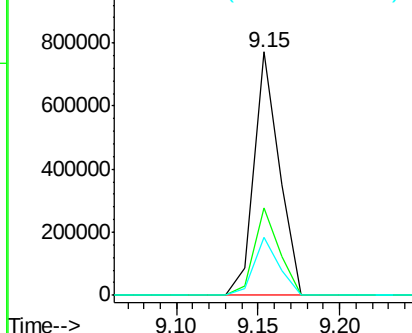



#49
 Dimethylphthalate
 Concen: 9.79 ng
 RT: 9.55 min Scan# 697
 Delta R.T. -0.02 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16

Tgt Ion:163 Resp: 132701
 Ion Ratio Lower Upper
 163 100
 194 3.8 2.8 4.2
 164 9.7 8.3 12.5

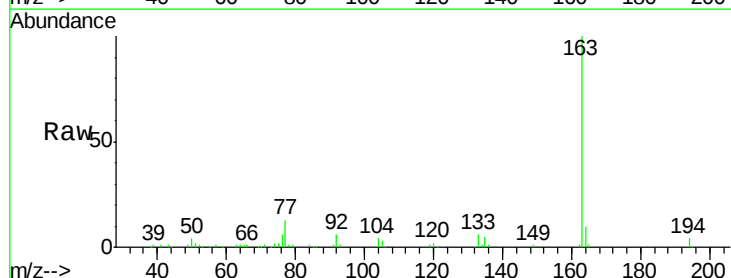

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E




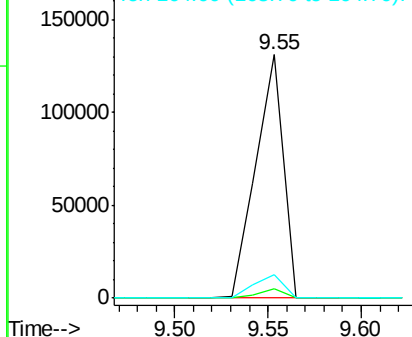


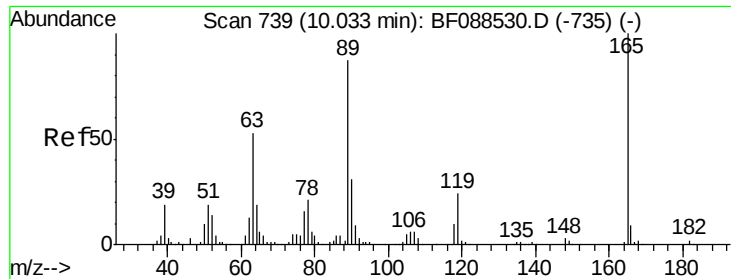

#56
 2,4-Dinitrotoluene
 Concen: 6.17 ng
 RT: 9.83 min Scan# 721
 Delta R.T. -0.21 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16




Instrument :
 BNA_F
 ClientSampleId :
 K8-B2(0-11)C


Tgt Ion:	165	Resp:	24236
Ion Ratio	Lower	Upper	
165	100		
63	1.7	22.0	33.0#
89	1.8	41.1	61.7#
182	0.0	2.0	3.0#

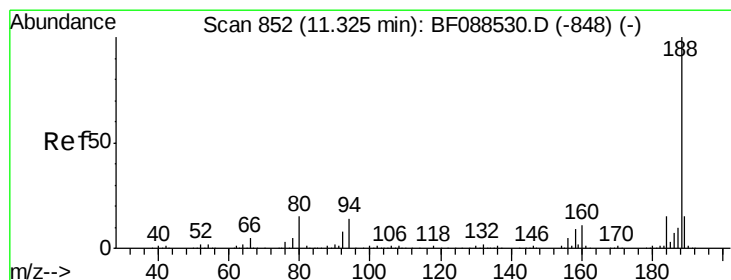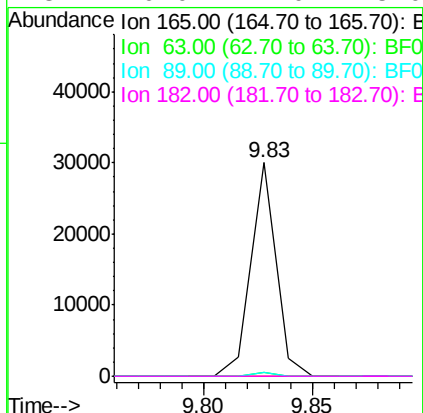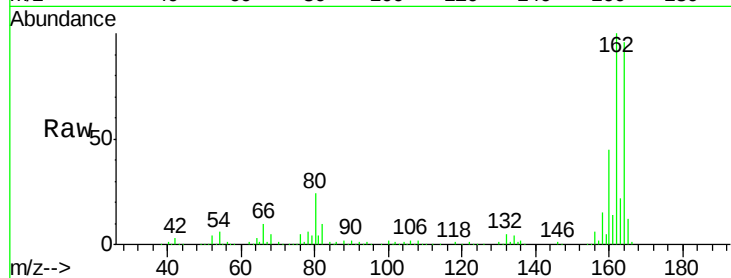

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.30 min Scan# 850
 Delta R.T. -0.02 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16

Tgt Ion:	188	Resp:	306262
Ion Ratio	Lower	Upper	
188	100		
94	13.3	9.0	13.6
80	15.5	10.0	15.0#

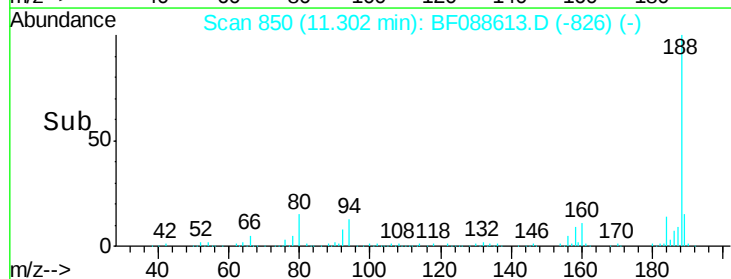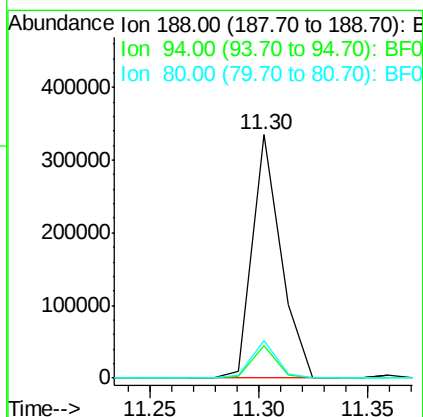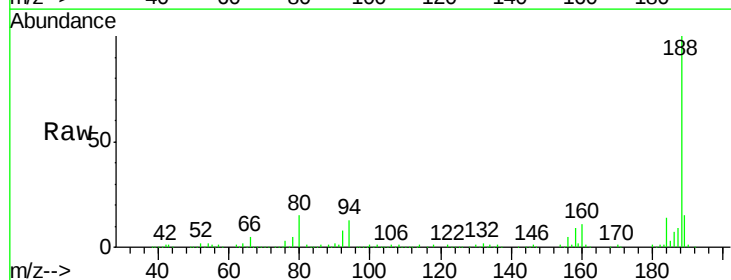


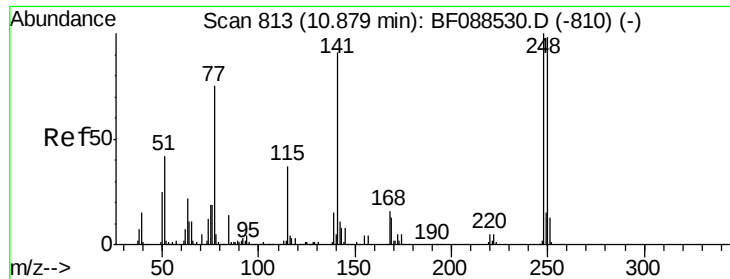




#66
4-Bromophenyl-phenylether
Concen: 3.96 ng
RT: 10.62 min Scan# 790
Delta R.T. -0.26 min
Lab File: BF088613.D
Acq: 2 Jul 2016 13:16

Instrument :
BNA_F
ClientSampleId :
K8-B2(0-11)C

Tgt Ion:248 Resp: 12237
Ion Ratio Lower Upper
248 100
250 204.1 77.1 115.7#
141 416.7 50.6 76.0#

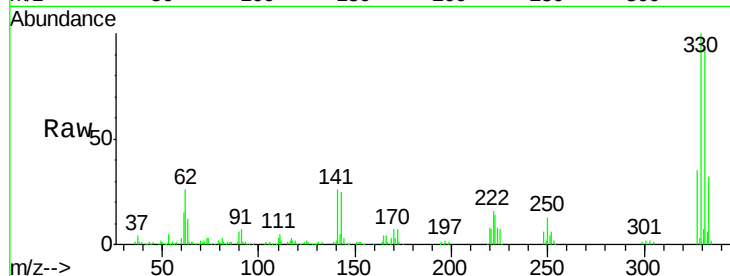


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

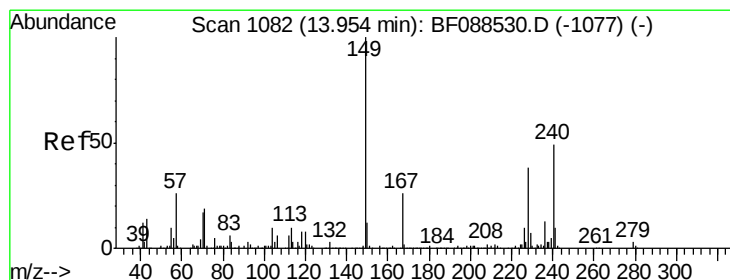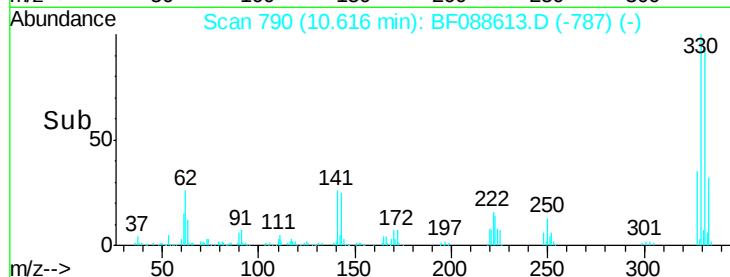
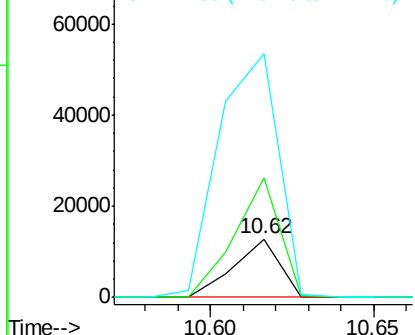



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.93 min Scan# 1080
Delta R.T. -0.02 min
Lab File: BF088613.D
Acq: 2 Jul 2016 13:16

Tgt Ion:240 Resp: 206312
Ion Ratio Lower Upper
240 100
120 12.2 6.8 10.2#
236 26.4 20.2 30.2

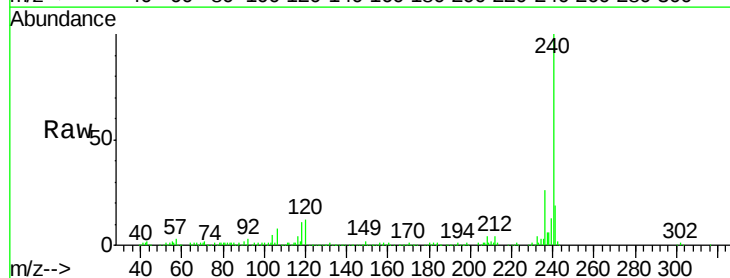

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



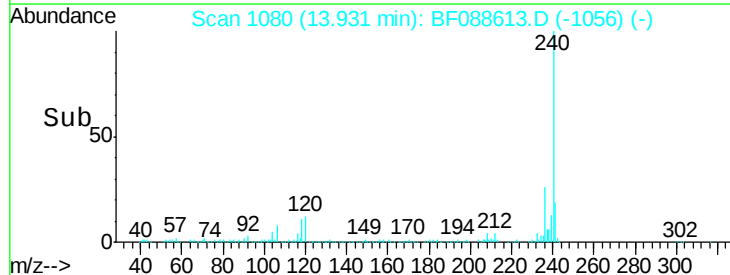
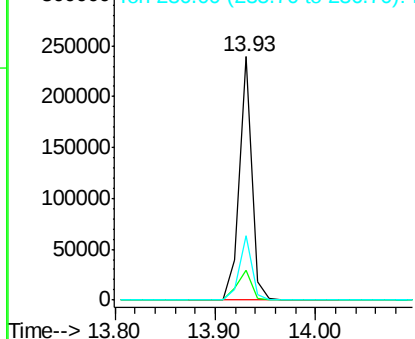




#78
 Terphenyl-d14
 Concen: 63.26 ng
 RT: 12.89 min Scan# 989
 Delta R.T. -0.02 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16

Instrument :
 BNA_F
 ClientSampleId :
 K8-B2(0-11)C

Tgt Ion:244 Resp: 585940
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.0 9.0
 122 13.8 11.2 16.8

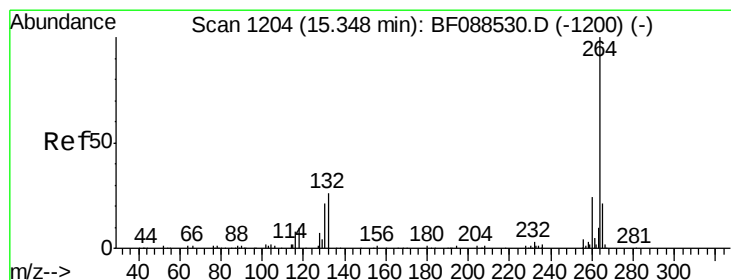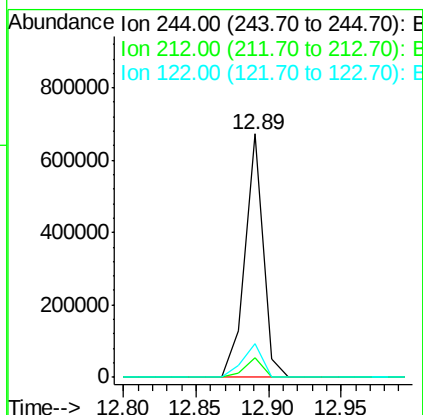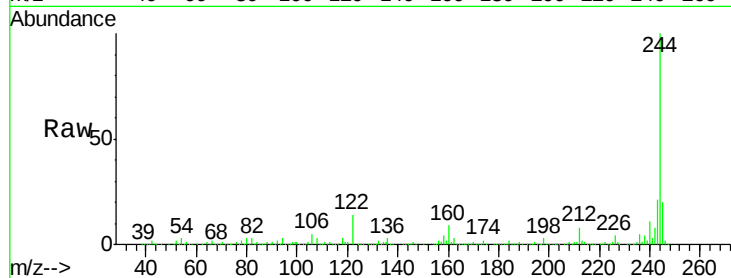

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.33 min Scan# 1202
 Delta R.T. -0.02 min
 Lab File: BF088613.D
 Acq: 2 Jul 2016 13:16

Tgt Ion:264 Resp: 213612
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.2 28.8
 265 21.4 16.9 25.3

