

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070217\
 Data File : BF096425.D
 Acq On : 2 Jul 2017 19:27
 Operator : SJ/MA
 Sample : I3950-07 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B5-0-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.281	30	33	38	rVB4	10696	13473	1.44%	0.181%
2	4.345	379	384	391	rVB3	7877	12825	1.37%	0.172%
3	4.910	477	480	486	rVB	40021	42430	4.53%	0.569%
4	5.340	549	553	557	rVB	326234	304169	32.44%	4.077%
5	6.363	723	727	733	rVB	338807	317614	33.87%	4.257%
6	6.498	746	750	758	rVB	394636	320502	34.18%	4.296%
7	6.734	786	790	793	rBV	936256	749779	79.96%	10.050%
8	6.886	813	816	821	rBV	294440	257448	27.46%	3.451%
9	7.286	879	884	891	rBV	249181	200040	21.33%	2.681%
10	7.345	891	894	897	rVB2	16293	13888	1.48%	0.186%
11	8.016	1004	1008	1011	rBV	1211510	937654	100.00%	12.568%
12	8.451	1080	1082	1086	rBV	14981	12435	1.33%	0.167%
13	8.622	1108	1111	1114	rBV	24443	19457	2.08%	0.261%
14	8.728	1124	1129	1132	rVB	26739	22352	2.38%	0.300%
15	8.828	1143	1146	1149	rBV	19811	16534	1.76%	0.222%
16	9.092	1187	1191	1194	rBV	378185	329819	35.17%	4.421%
17	9.186	1204	1207	1212	rVB2	24783	22002	2.35%	0.295%
18	9.351	1232	1235	1239	rVB3	8524	11653	1.24%	0.156%
19	9.427	1246	1248	1250	rBV	15268	12363	1.32%	0.166%
20	9.480	1254	1257	1260	rBV	51984	41905	4.47%	0.562%
21	9.627	1278	1282	1284	rBV	17249	16820	1.79%	0.225%
22	9.716	1294	1297	1301	rVB	20276	18736	2.00%	0.251%
23	9.769	1302	1306	1310	rBV	917798	803197	85.66%	10.766%
24	9.969	1338	1340	1344	rBV2	18916	17342	1.85%	0.232%
25	10.210	1379	1381	1386	rVB	23306	19688	2.10%	0.264%
26	10.310	1396	1398	1402	rVB2	16890	11973	1.28%	0.160%
27	10.433	1415	1419	1422	rBV2	11505	15547	1.66%	0.208%
28	10.469	1422	1425	1429	rVB5	7923	11635	1.24%	0.156%
29	10.545	1435	1438	1445	rVB2	144263	138557	14.78%	1.857%
30	10.680	1458	1461	1463	rBV2	31807	36311	3.87%	0.487%
31	11.127	1535	1537	1541	rBV4	20525	19149	2.04%	0.257%
32	11.245	1553	1557	1560	rBV	847086	734645	78.35%	9.847%
33	11.269	1560	1561	1564	rVV	105164	56456	6.02%	0.757%
34	11.321	1567	1570	1572	rVB	37469	30743	3.28%	0.412%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070217\
Data File : BF096425.D
Acq On : 2 Jul 2017 19:27
Operator : SJ/MA
Sample : I3950-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B5-0-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.745	1640	1642	1644	rBV2	15173	14678	1.57%	0.197%
36	11.774	1644	1647	1650	rVB	29482	28863	3.08%	0.387%
37	11.857	1658	1661	1663	rBV2	29569	31076	3.31%	0.417%
38	11.963	1675	1679	1683	rBV5	20080	35547	3.79%	0.476%
39	12.063	1694	1696	1700	rVB5	15730	20148	2.15%	0.270%
40	12.192	1717	1718	1721	rBV3	12861	14325	1.53%	0.192%
41	12.298	1733	1736	1739	rVB3	19402	20409	2.18%	0.274%
42	12.327	1739	1741	1742	rBV2	15370	12801	1.37%	0.172%
43	12.451	1759	1762	1766	rBV	156560	137028	14.61%	1.837%
44	12.680	1796	1801	1804	rBV	138086	137971	14.71%	1.849%
45	12.827	1823	1826	1833	rVB	268041	242971	25.91%	3.257%
46	13.074	1866	1868	1870	rVB2	25686	19570	2.09%	0.262%
47	13.315	1906	1909	1913	rVB	105571	96874	10.33%	1.298%
48	13.874	2000	2004	2007	rBV	635752	653956	69.74%	8.765%
49	15.286	2241	2244	2248	rBV2	336008	405323	43.23%	5.433%


Sum of corrected areas: 7460681

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070217\
Data File : BF096425.D
Acq On : 2 Jul 2017 19:27
Operator : SJ/MA
Sample : I3950-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B5-0-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

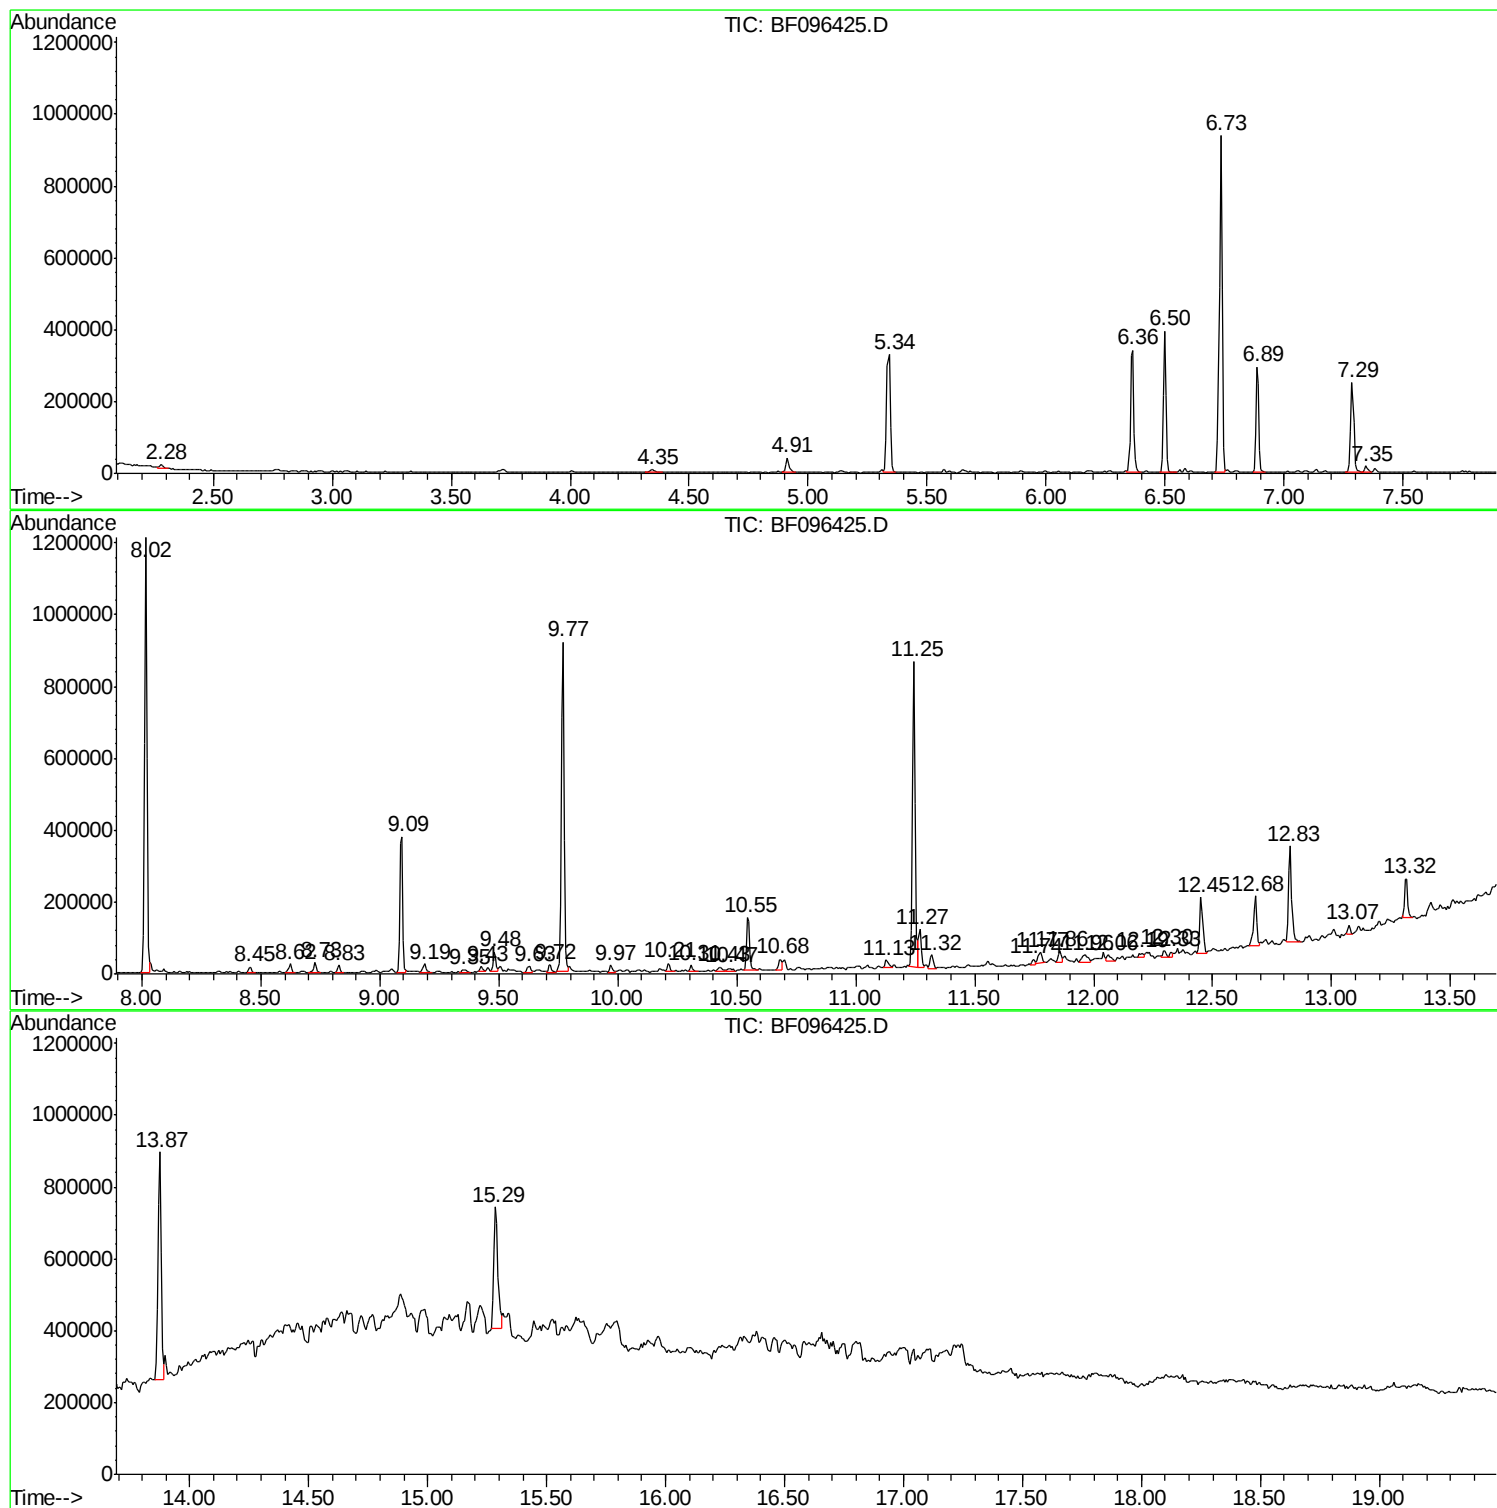

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070217\
Data File : BF096425.D
Acq On : 2 Jul 2017 19:27
Operator : SJ/MA
Sample : I3950-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B5-0-2










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	8.55 ng	320502	1,4-Dichlorobenzene-d4	6.73

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3			1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4			4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

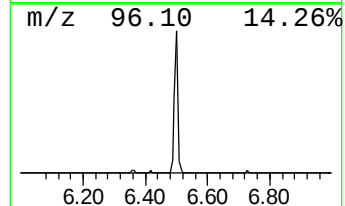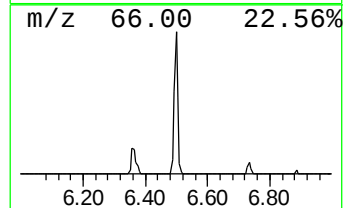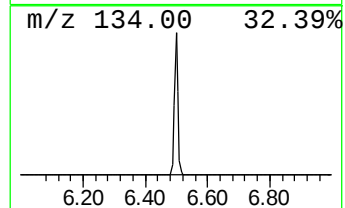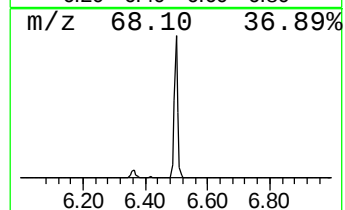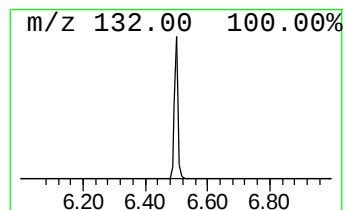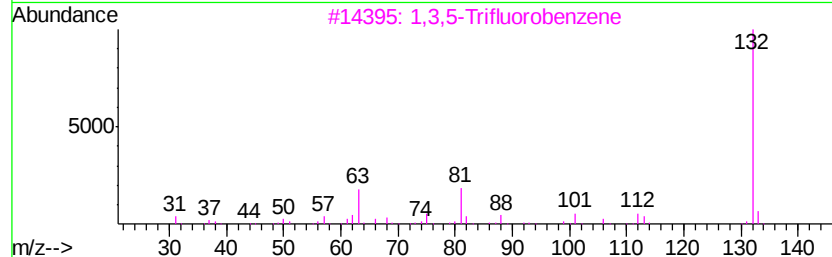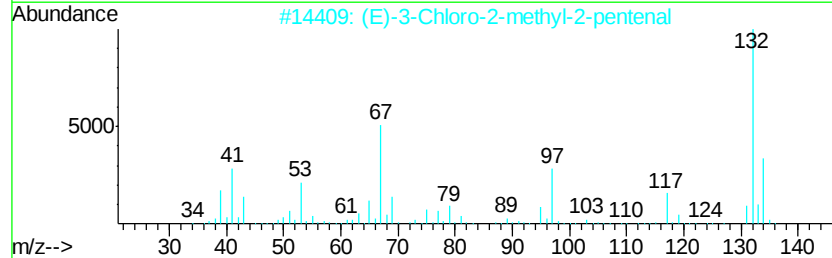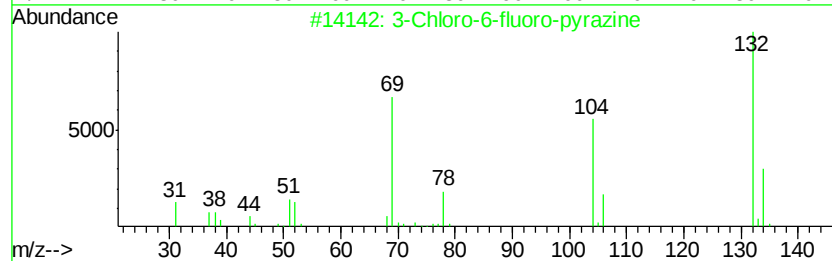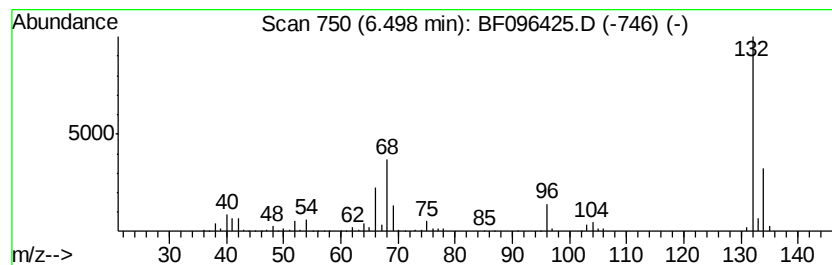

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070217\
Data File : BF096425.D
Acq On : 2 Jul 2017 19:27
Operator : SJ/MA
Sample : I3950-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B5-0-2










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 9-Octadecenamide, (Z)- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.32	2.96 ng	96874	Chrysene-d12	13.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	87
2		Tetradecanamide	227	C14H29NO	000638-58-4	78
3		Pentanamide	101	C5H11NO	000626-97-1	64
4		Undecanamide, 11-bromo-	263	C11H22BrNO	005875-26-3	59
5		Octanamide	143	C8H17NO	000629-01-6	59

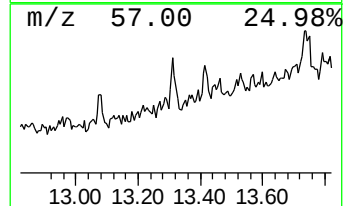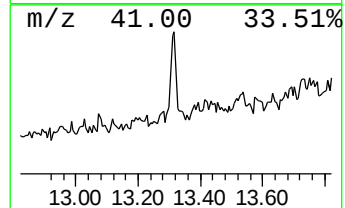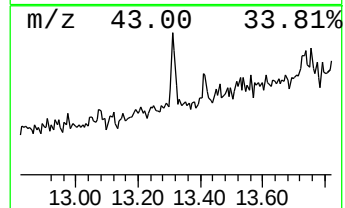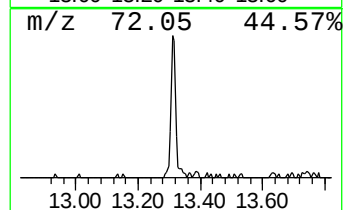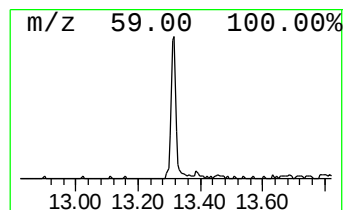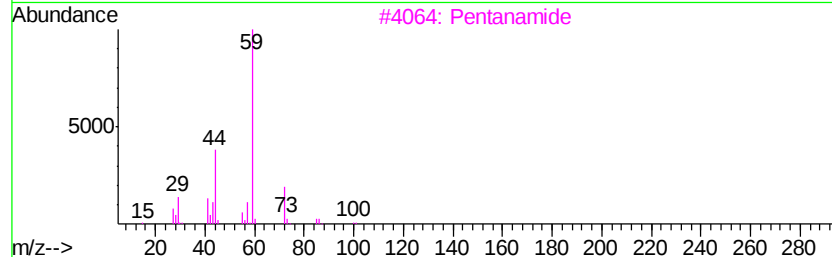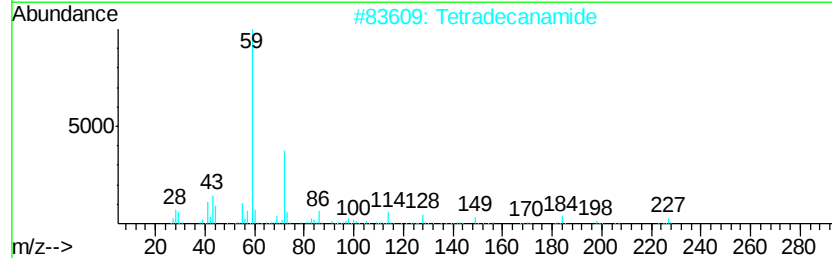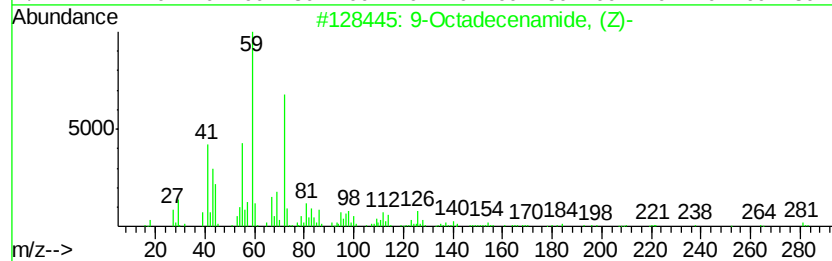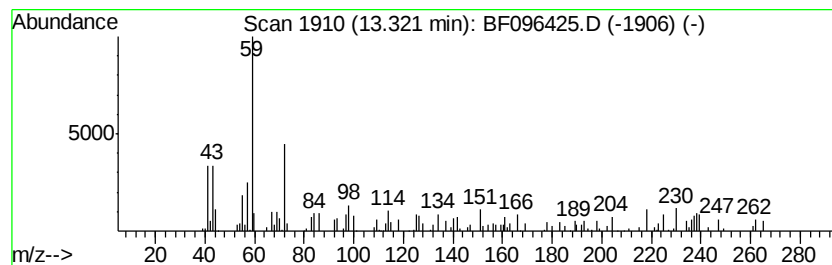

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070217\
Data File : BF096425.D
Acq On : 2 Jul 2017 19:27
Operator : SJ/MA
Sample : I3950-07 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B5-0-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	8.6	ng	320502	1	6.73	749779	20.0
9-Octadecenamide,...	13.32	3.0	ng	96874	5	13.87	653956	20.0